


Data Path : Z:\HPCHEM1\BNA M\Data\BM052217\
 Data File : BM010093.D
 Acq On : 22 May 2017 09:38
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

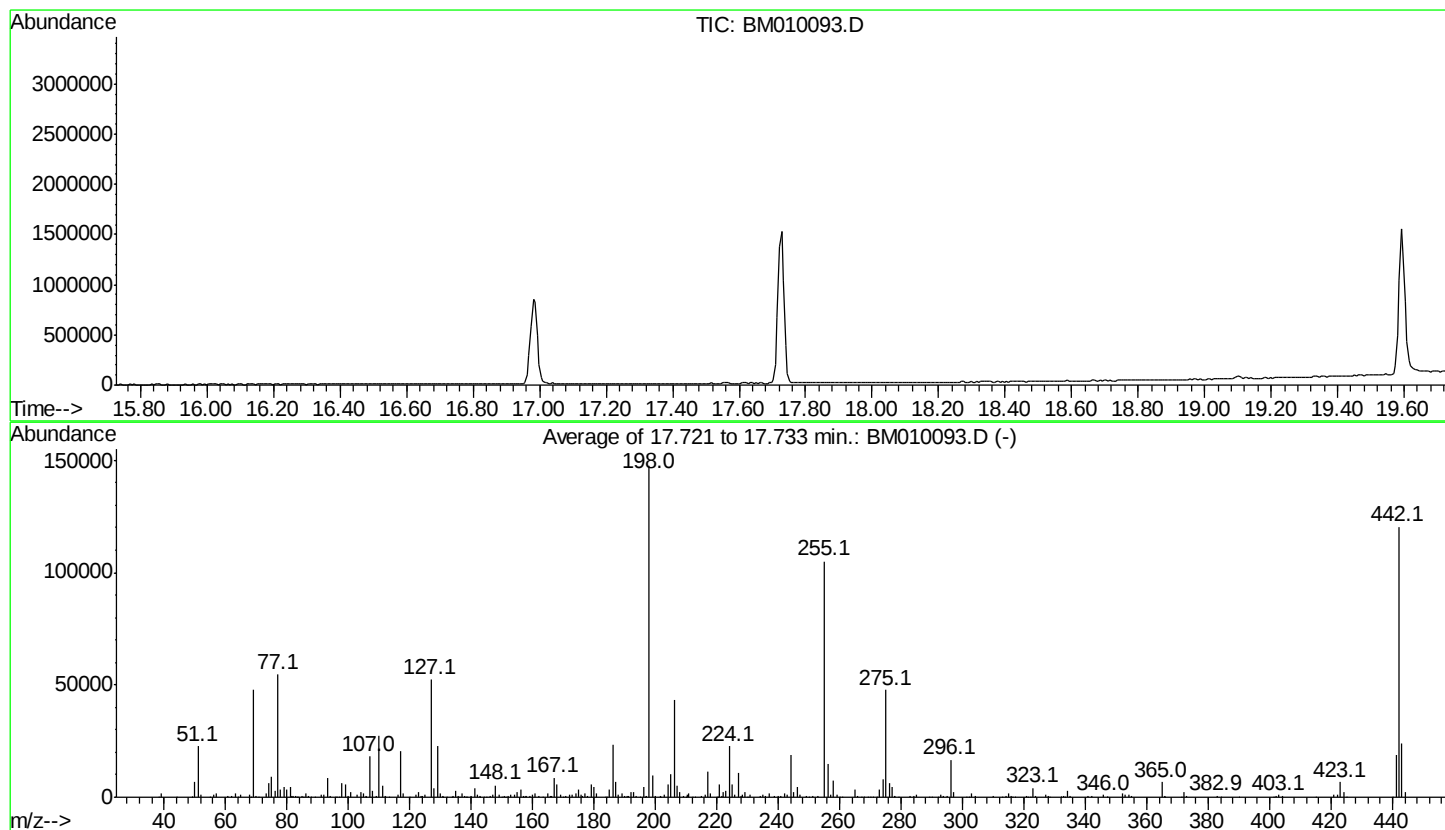

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.4	22717	PASS
68	69	0.00	2	1.9	896	PASS
69	198	0.00	100	32.4	47754	PASS
70	69	0.00	2	0.9	421	PASS
127	198	10	80	35.4	52298	PASS
197	198	0.00	2	0.6	837	PASS
198	198	100	100	100.0	147597	PASS
199	198	5	9	6.6	9707	PASS
275	198	10	60	32.4	47856	PASS
365	198	1	100	4.5	6607	PASS
441	442	0.01	24	15.8	18976	PASS
442	198	50	100	81.6	120381	PASS
443	442	15	24	20.0	24072	PASS