


Data Path : Z:\HPCHEM1\BNA M\Data\BM052217\
 Data File : BM010113.D
 Acq On : 22 May 2017 21:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

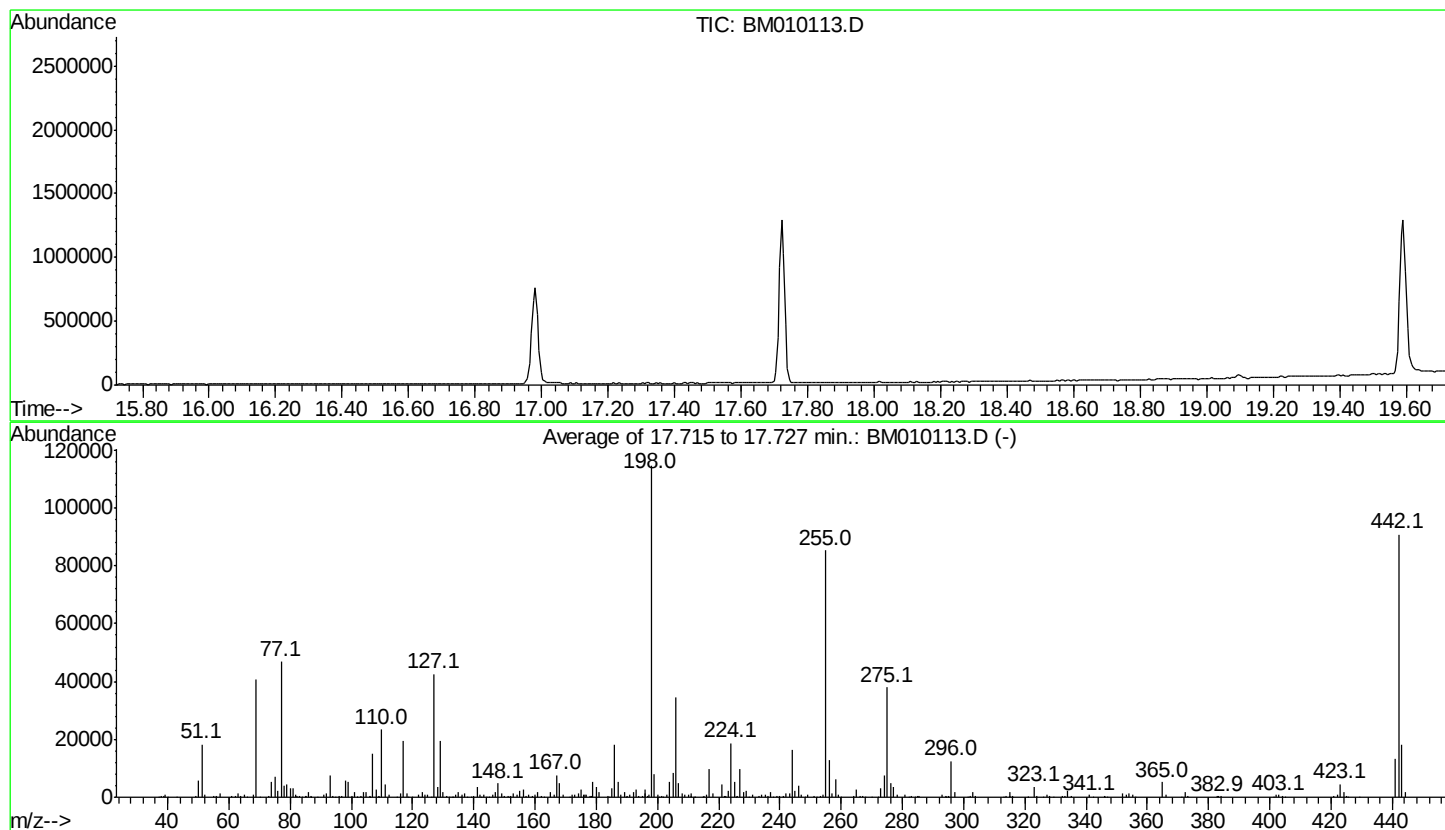

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.8	18147	PASS
68	69	0.00	2	1.9	758	PASS
69	198	0.00	100	35.5	40666	PASS
70	69	0.00	2	0.5	222	PASS
127	198	10	80	37.1	42496	PASS
197	198	0.00	2	0.6	694	PASS
198	198	100	100	100.0	114616	PASS
199	198	5	9	6.8	7847	PASS
275	198	10	60	33.1	37901	PASS
365	198	1	100	4.6	5293	PASS
441	442	0.01	24	14.8	13408	PASS
442	198	50	100	79.2	90746	PASS
443	442	15	24	20.1	18265	PASS