
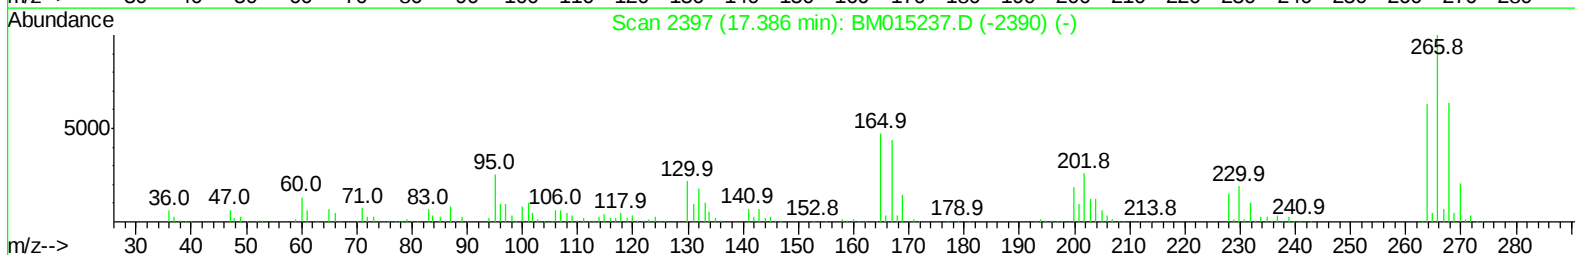
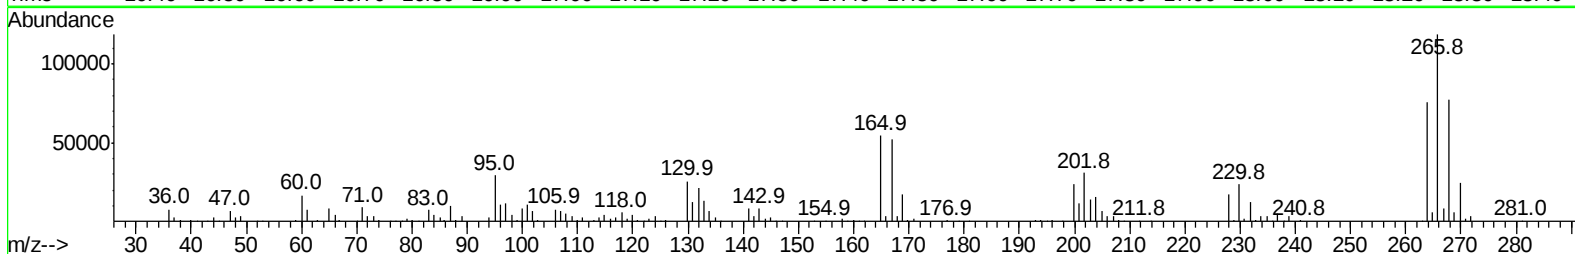


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM052218\
Data File : BM015233.D
Acq On : 22 May 2018 10:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 06:44:21 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM052218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 22 15:47:28 2018
Response via : Initial Calibration

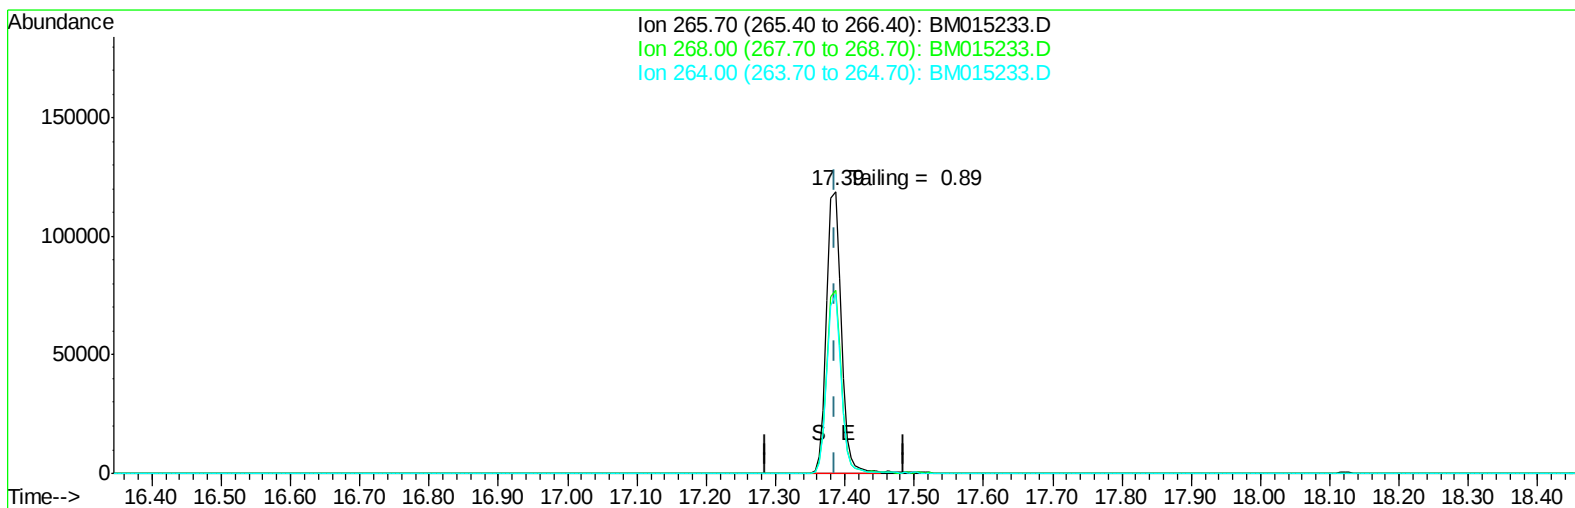

TIC: BM015233.D

(69) Pentachlorophenol (C)




17.386min (+0.000) 0.00ng

response 175356

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.13
264.00	61.20	63.59
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM052218\
Data File : BM015233.D
Acq On : 22 May 2018 10:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 06:44:21 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM052218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 22 15:47:28 2018
Response via : Initial Calibration

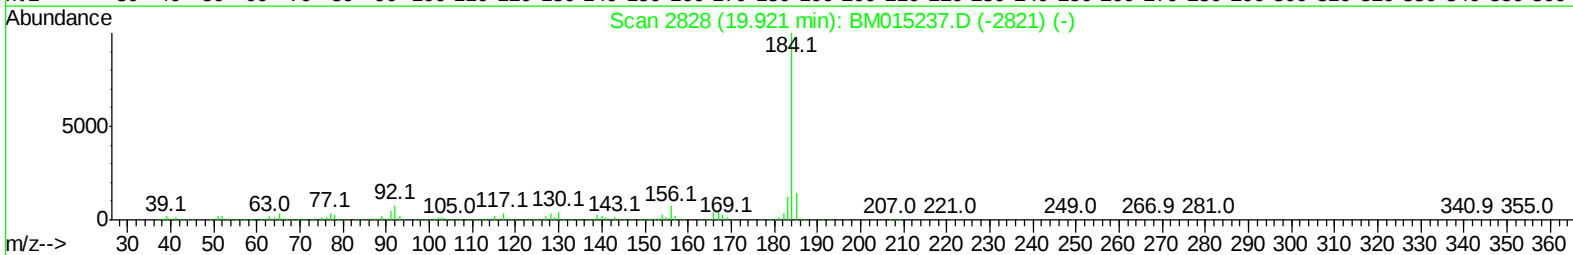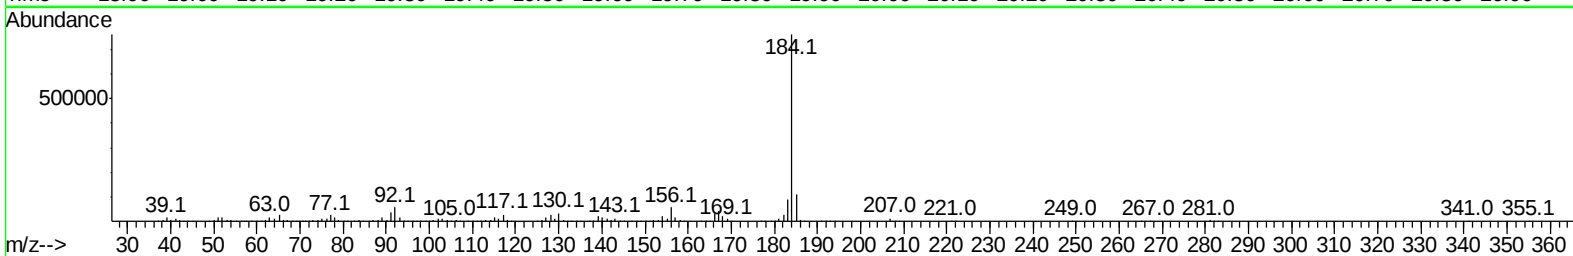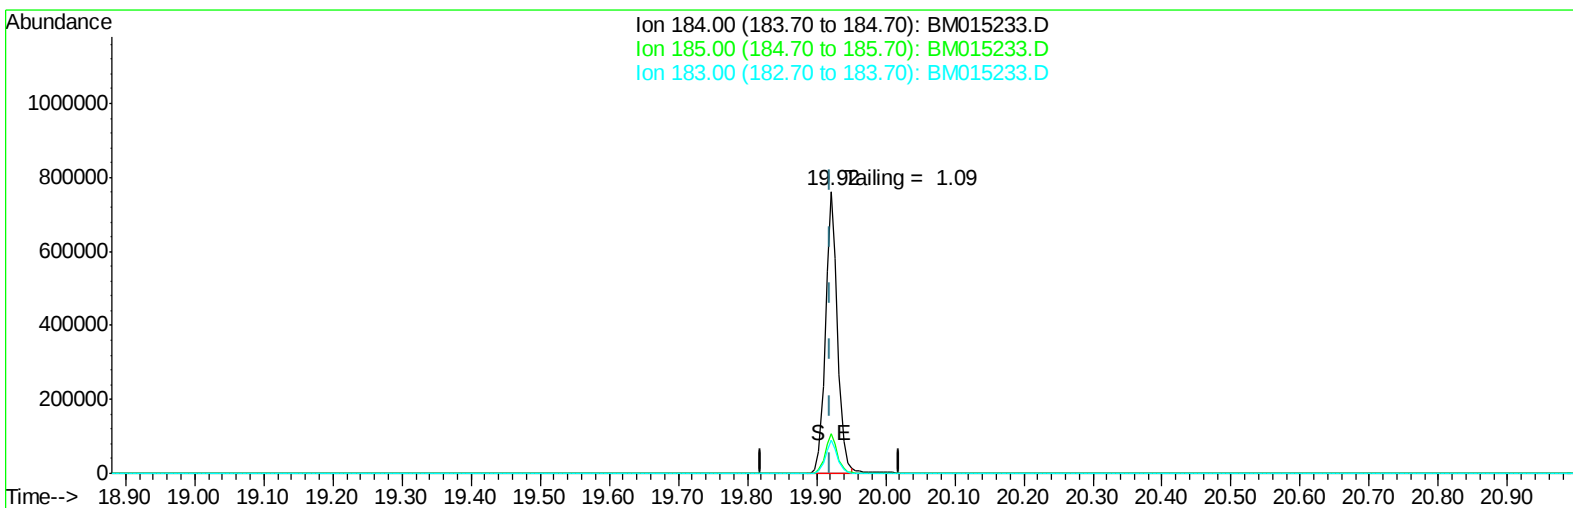

TIC: BM015233.D

(76) Benzidine

19.921min (+0.000) 0.00ng

response 926093

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.12
183.00	11.10	11.69
0.00	0.00	0.00