
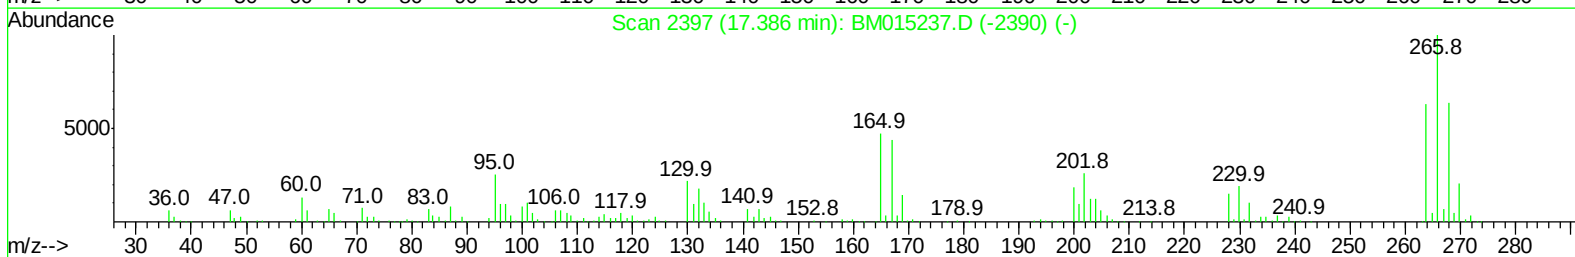
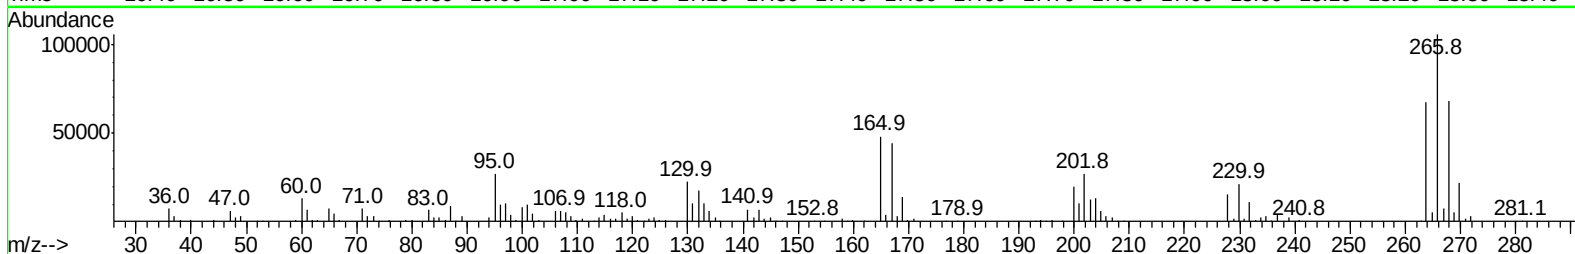


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM052218\
Data File : BM015242.D
Acq On : 22 May 2018 16:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 06:12:54 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM052218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 22 15:47:28 2018
Response via : Initial Calibration

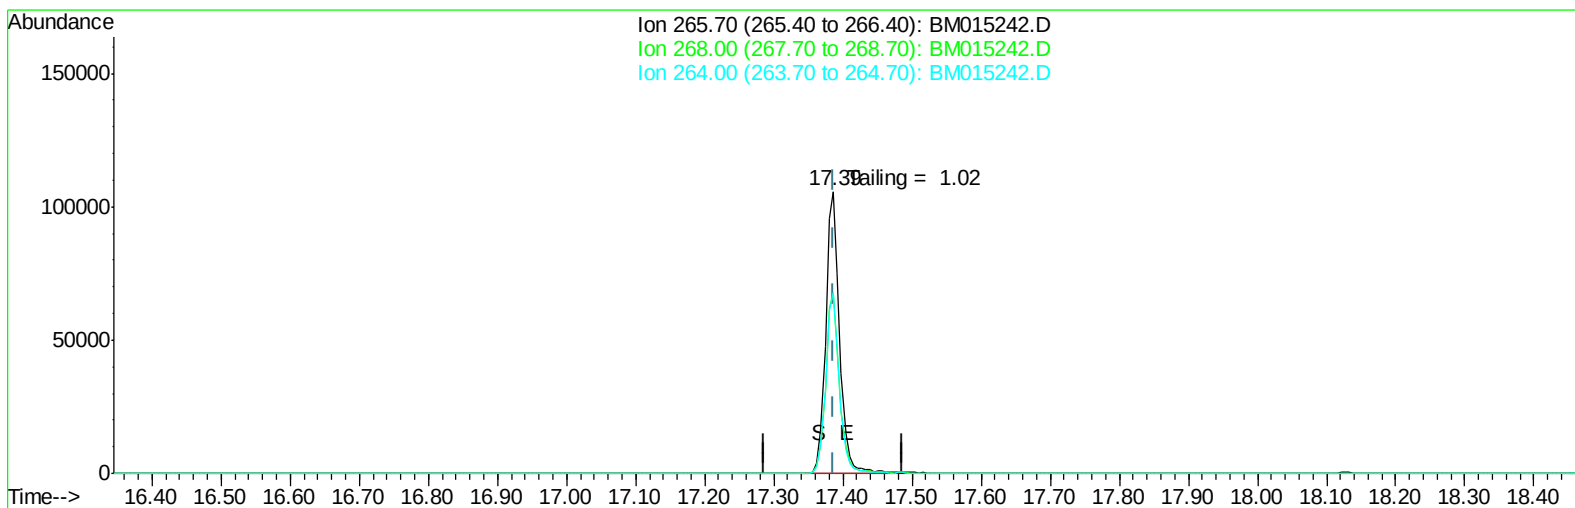

TIC: BM015242.D

(69) Pentachlorophenol (C)

17.386min (-0.000) 0.00ng

response 146712

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.18
264.00	61.20	63.94
0.00	0.00	0.00

