


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052218\
 Data File : BM015233.D
 Acq On : 22 May 2018 10:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM052218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 22 15:47:28 2018

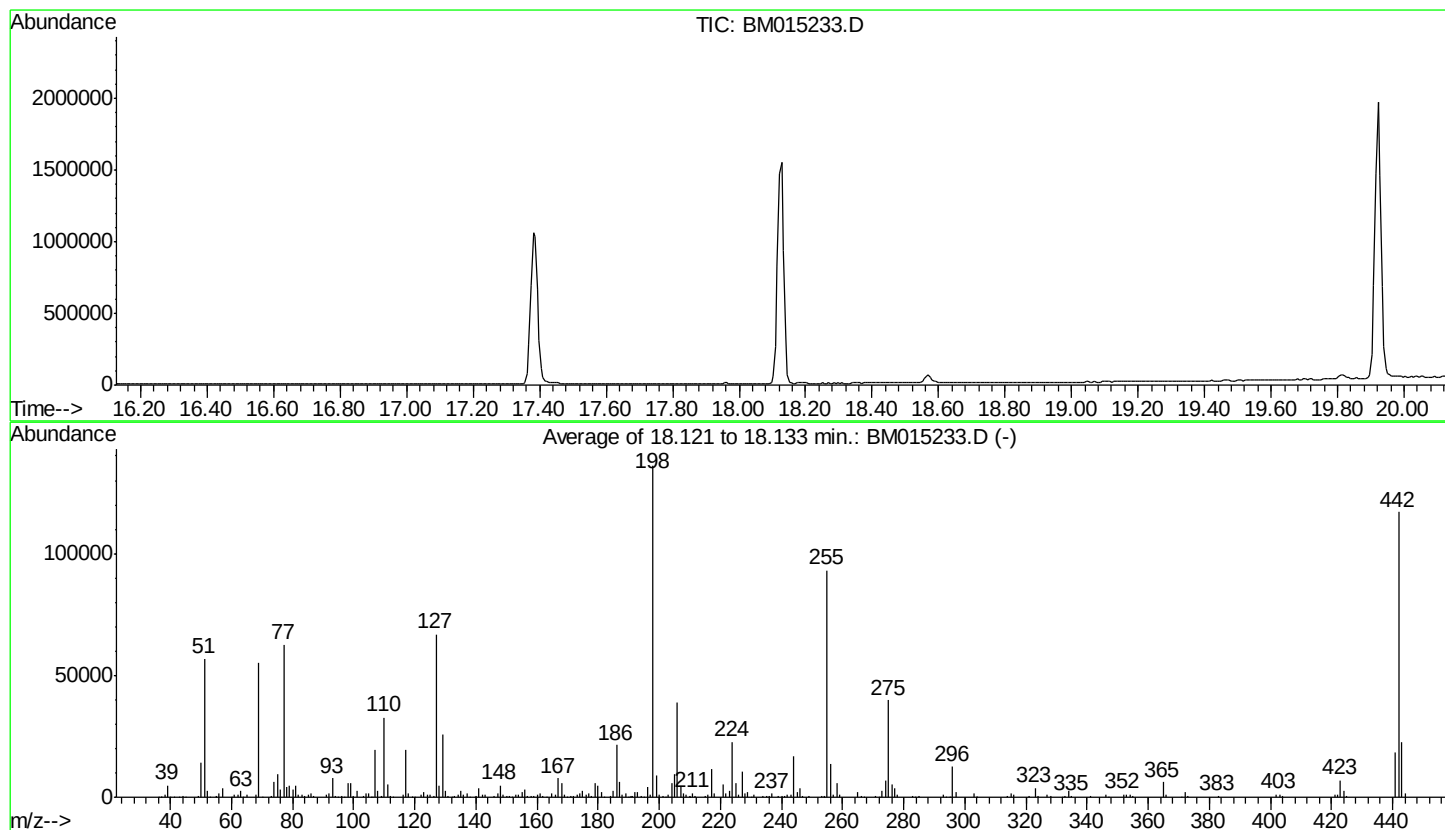

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	56856	PASS
68	69	0.00	2	2.0	1083	PASS
69	198	0.00	100	40.6	55256	PASS
70	69	0.00	2	0.3	163	PASS
127	198	10	80	49.2	66957	PASS
197	198	0.00	2	0.6	815	PASS
198	198	100	100	100.0	136069	PASS
199	198	5	9	6.6	8930	PASS
275	198	10	60	29.3	39874	PASS
365	198	1	100	4.5	6092	PASS
441	443	0.01	100	82.8	18604	PASS
442	198	50	100	86.1	117101	PASS
443	442	15	24	19.2	22472	PASS