

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026088.D
 Acq On : 22 May 2020 20:22
 Operator : MA/SJ
 Sample : L2737-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B07

Quant Time: May 23 01:43:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 22 13:18:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	150877	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	598217	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	341891	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	715488	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	777199	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	837236	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	28041	5.61	ng/uL	0.00
5) Phenol-d5	6.68	99	103952	7.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	271820	28.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	254689	23.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	173777	16.85	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	145090	29.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	146223	30.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	259581	26.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	29142	2.97	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	885283	32.29	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	995403	30.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	31820	6.55	ng/ul	0.00
58) Fluorene-d10	15.13	176	758095	31.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	118923	28.51	ng/ul	0.00
71) Anthracene-d10	16.98	188	1266028	35.91	ng/ul	0.00
79) Pyrene-d10	19.28	212	1451527	36.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	1646308	36.94	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.60	163	128177	4.453	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
Data File : BM026088.D
Acq On : 22 May 2020 20:22
Operator : MA/SJ
Sample : L2737-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B07

Quant Time: May 23 01:43:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 22 13:18:41 2020
Response via : Initial Calibration

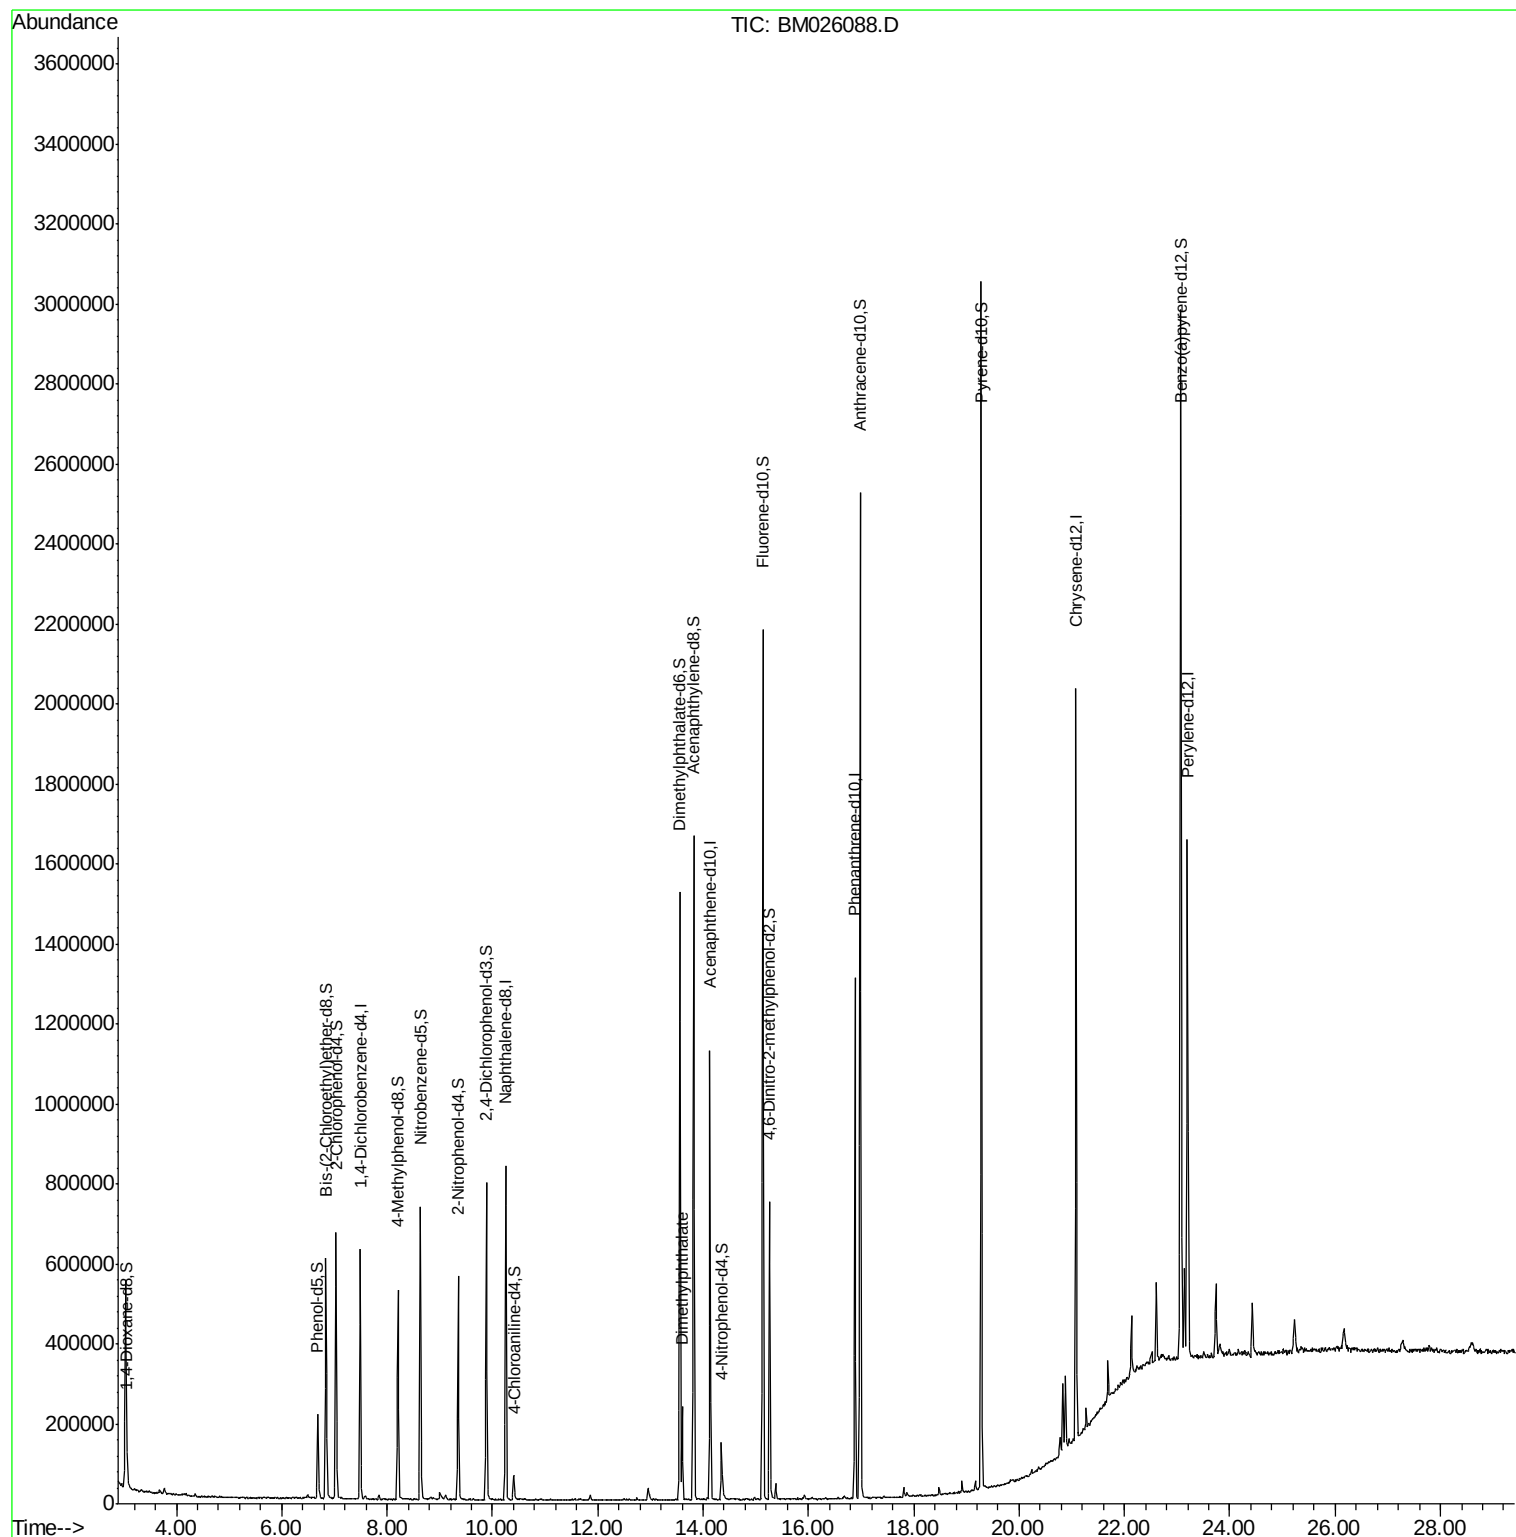

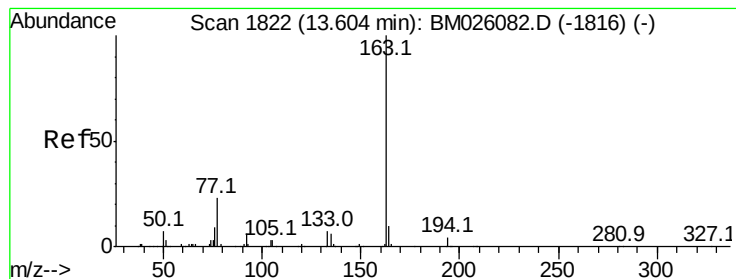

#45

Dimethylphthalate

Concen: 4.453 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. 0.00 min

Lab File: BM026088.D

Acq: 22 May 2020 20:22

Instrument :

BNA_M

ClientSampleId :

F9B07


Tot Ion:163 Resp: 128177

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.0 8.0 12.0

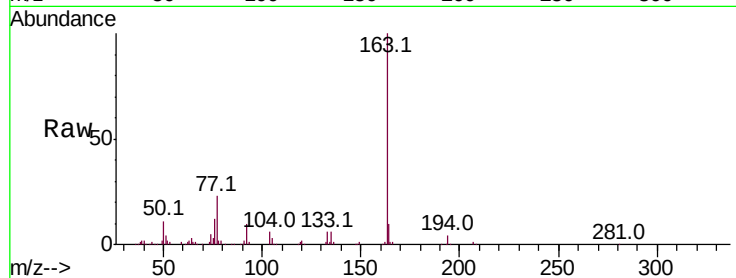

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

