

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026089.D
 Acq On : 22 May 2020 20:58
 Operator : MA/SJ
 Sample : L2737-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B16

Quant Time: May 23 01:43:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 22 13:18:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	155396	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	624995	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	359583	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	775666	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	815041	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	874560	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	26254	5.10	ng/uL	0.00
5) Phenol-d5	6.68	99	113769	8.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	285658	29.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	270453	24.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	195696	18.42	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	153929	30.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	161259	31.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.89	165	294695	29.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	29632	2.89	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	968245	33.58	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1111821	32.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	36099	7.07	ng/ul	0.00
58) Fluorene-d10	15.13	176	832569	33.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	132458	29.29	ng/ul	0.00
71) Anthracene-d10	16.98	188	1320915	34.56	ng/ul	0.00
79) Pyrene-d10	19.28	212	1508959	36.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	1657418	35.61	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.60	163	121160	4.002	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
Data File : BM026089.D
Acq On : 22 May 2020 20:58
Operator : MA/SJ
Sample : L2737-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B16

Quant Time: May 23 01:43:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 22 13:18:41 2020
Response via : Initial Calibration

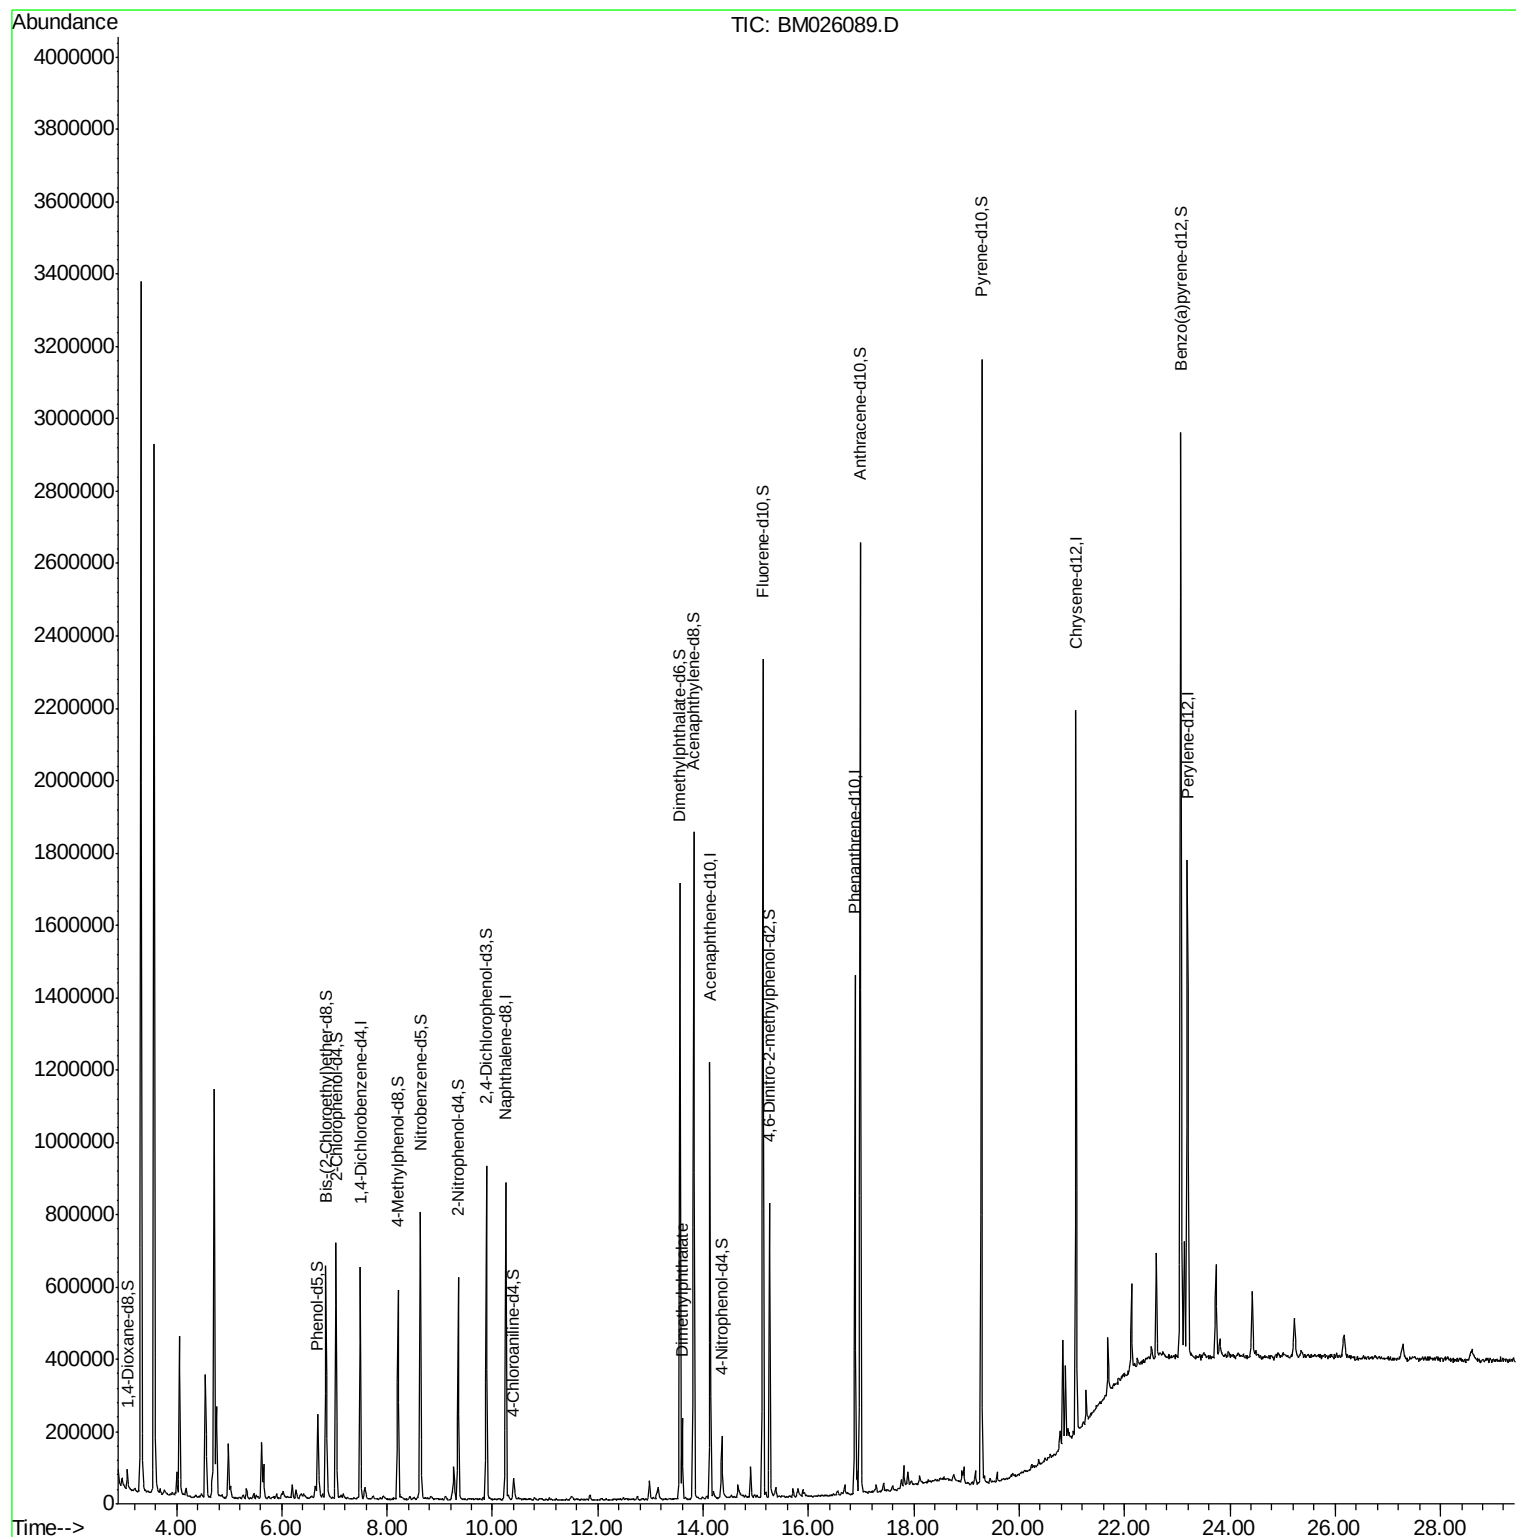

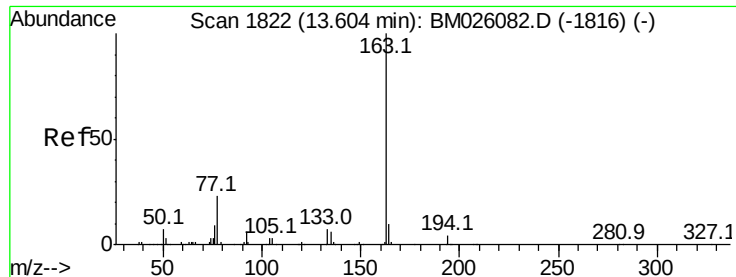

#45

Dimethylphthalate

Concen: 4.002 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. -0.00 min

Lab File: BM026089.D

Acq: 22 May 2020 20:58

Instrument :

BNA_M

ClientSampleId :

F9B16


Tot Ion:163 Resp: 121160

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 9.2 8.0 12.0

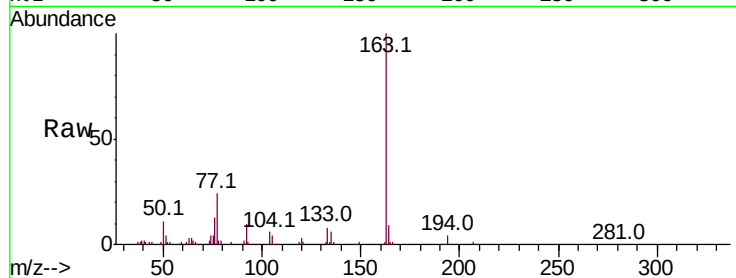

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

