

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026090.D
 Acq On : 22 May 2020 21:35
 Operator : MA/SJ
 Sample : L2737-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B09

Quant Time: May 23 01:43:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 22 13:18:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	153382	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	618751	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	349004	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	741887	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	811383	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	864448	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	25800	5.07	ng/uL	0.00
5) Phenol-d5	6.68	99	128958	9.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	320659	33.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	303531	27.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	220930	21.07	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	176031	34.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	184210	36.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	337706	33.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	33003	3.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1096039	39.16	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1271002	38.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	41219	8.32	ng/ul	0.00
58) Fluorene-d10	15.13	176	941492	38.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	145987	33.75	ng/ul	0.00
71) Anthracene-d10	16.98	188	1449690	39.65	ng/ul	0.00
79) Pyrene-d10	19.29	212	1677262	40.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	1849514	40.20	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.60	163	100466	3.419	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
Data File : BM026090.D
Acq On : 22 May 2020 21:35
Operator : MA/SJ
Sample : L2737-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B09

Quant Time: May 23 01:43:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 22 13:18:41 2020
Response via : Initial Calibration

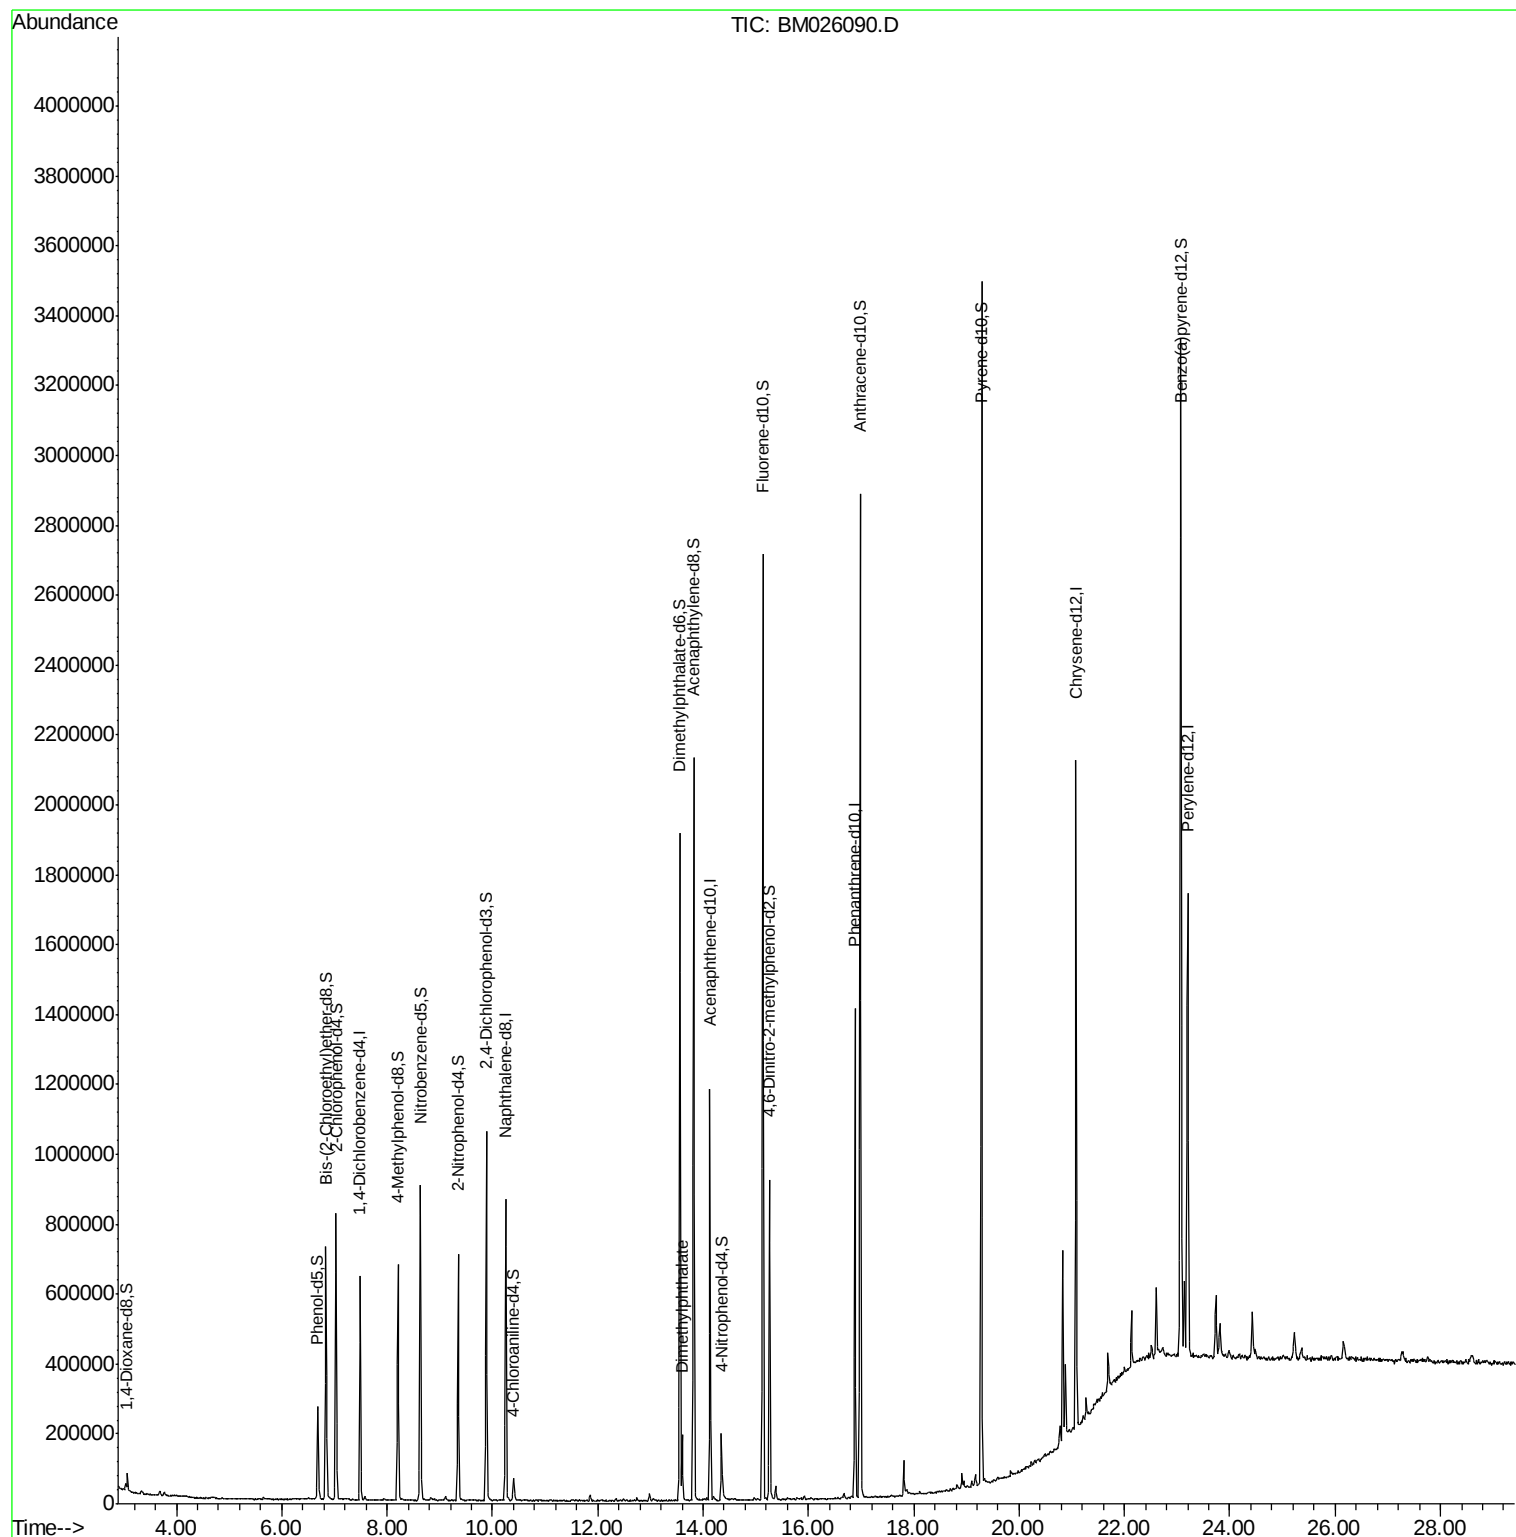

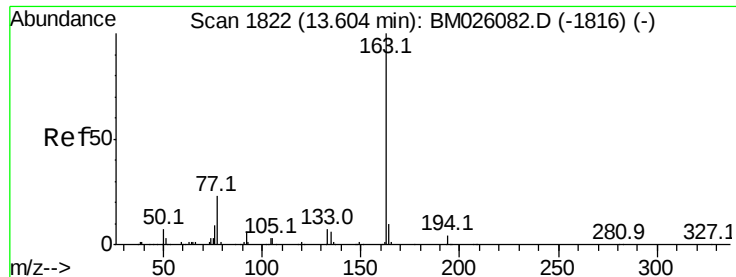

#45

Dimethylphthalate

Concen: 3.419 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. 0.00 min

Lab File: BM026090.D

Acq: 22 May 2020 21:35

Instrument :

BNA_M

ClientSampleId :

F9B09


Tot Ion:163 Resp: 100466

Ion Ratio Lower Upper

163 100

194 5.0 3.2 4.8#

164 10.2 8.0 12.0

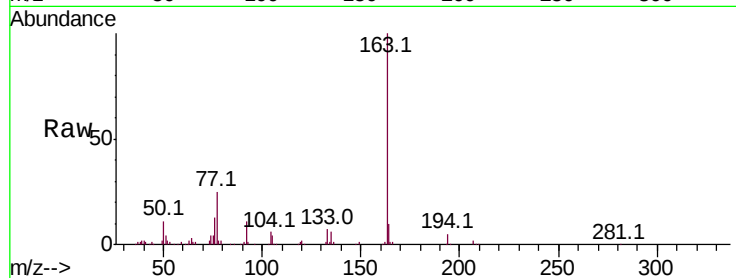

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

