

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026081.D
 Acq On : 22 May 2020 15:28
 Operator : MA/SJ
 Sample : L2735-04DL 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CB9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	68	70	72	rBV3	3428	2841	0.14%	0.022%
2	3.693	135	137	143	rBV7	2312	3781	0.19%	0.030%
3	3.775	146	151	156	rVB2	12303	18875	0.95%	0.149%
4	4.528	275	279	280	rVB3	1951	2392	0.12%	0.019%
5	5.110	374	378	381	rVB6	2118	2849	0.14%	0.023%
6	5.269	403	405	409	rVB5	1863	2463	0.12%	0.019%
7	5.316	409	413	418	rVB8	1310	2711	0.14%	0.021%
8	5.734	480	484	485	rBV4	2311	2843	0.14%	0.022%
9	6.098	543	546	547	rBV3	2304	2404	0.12%	0.019%
10	6.687	642	646	654	rBV3	11422	17754	0.89%	0.140%
11	6.845	668	673	678	rBV	27751	48411	2.43%	0.383%
12	7.034	699	705	710	rBV	29944	51019	2.56%	0.403%
13	7.404	766	768	773	rVB5	1926	2976	0.15%	0.024%
14	7.492	776	783	791	rVV	574698	873964	43.83%	6.911%
15	7.610	799	803	808	rVB6	3899	6499	0.33%	0.051%
16	7.669	811	813	817	rBV4	1941	3179	0.16%	0.025%
17	7.739	822	825	827	rBV4	1963	2691	0.13%	0.021%
18	7.810	834	837	838	rBV3	3488	2900	0.15%	0.023%
19	7.857	841	845	849	rVB7	4209	6001	0.30%	0.047%
20	8.145	892	894	897	rVB4	2885	3330	0.17%	0.026%
21	8.210	897	905	916	rBV3	21707	45071	2.26%	0.356%
22	8.639	973	978	987	rVV2	32677	61120	3.07%	0.483%
23	8.716	987	991	994	rVV6	2371	3646	0.18%	0.029%
24	8.769	997	1000	1002	rBV4	2546	3124	0.16%	0.025%
25	8.928	1023	1027	1030	rBV5	2701	2611	0.13%	0.021%
26	9.104	1054	1057	1058	rBV3	2862	2638	0.13%	0.021%
27	9.192	1070	1072	1078	rVB6	2391	4029	0.20%	0.032%
28	9.357	1094	1100	1107	rBV	23990	41063	2.06%	0.325%
29	9.475	1116	1120	1123	rVB6	2788	3616	0.18%	0.029%
30	9.892	1185	1191	1198	rBV2	31459	62095	3.11%	0.491%
31	9.980	1203	1206	1209	rBV4	2270	3345	0.17%	0.026%
32	10.251	1245	1252	1259	rBV	710064	1181479	59.25%	9.343%
33	10.304	1259	1261	1269	rVV4	13351	19105	0.96%	0.151%
34	10.375	1271	1273	1276	rVV4	3873	4872	0.24%	0.039%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026081.D
 Acq On : 22 May 2020 15:28
 Operator : MA/SJ
 Sample : L2735-04DL 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CB9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	10.422	1276	1281	1285	rVV4	6581	12525	0.63%	0.099%
36	10.498	1289	1294	1297	rVB6	1580	2753	0.14%	0.022%
37	10.722	1330	1332	1336	rVB4	2331	2437	0.12%	0.019%
38	10.927	1364	1367	1369	rVB4	2290	2393	0.12%	0.019%
39	11.363	1437	1441	1443	rBV5	2353	2949	0.15%	0.023%
40	12.151	1570	1575	1582	rVB2	17523	31180	1.56%	0.247%
41	12.304	1599	1601	1605	rVB4	2479	2726	0.14%	0.022%
42	12.639	1654	1658	1664	rVB8	1949	3359	0.17%	0.027%
43	12.963	1709	1713	1717	rVB2	9137	11964	0.60%	0.095%
44	13.145	1740	1744	1747	rVV6	3165	4875	0.24%	0.039%
45	13.180	1747	1750	1757	rVB8	4648	8515	0.43%	0.067%
46	13.310	1767	1772	1776	rBV7	2618	5514	0.28%	0.044%
47	13.463	1792	1798	1800	rBV7	4855	8317	0.42%	0.066%
48	13.486	1800	1802	1804	rVV3	2999	2799	0.14%	0.022%
49	13.516	1804	1807	1809	rVV3	2767	2951	0.15%	0.023%
50	13.557	1809	1814	1820	rVV	71077	102723	5.15%	0.812%
51	13.604	1820	1822	1827	rVB	9565	13056	0.65%	0.103%
52	13.698	1833	1838	1839	rBV5	3179	4565	0.23%	0.036%
53	13.727	1841	1843	1846	rVB4	3062	2544	0.13%	0.020%
54	13.821	1852	1859	1865	rBV	77937	115996	5.82%	0.917%
55	13.992	1881	1888	1897	rVV	6369	15438	0.77%	0.122%
56	14.133	1906	1912	1921	rVB	1004709	1454284	72.93%	11.500%
57	14.198	1921	1923	1926	rVB4	3162	2626	0.13%	0.021%
58	14.239	1926	1930	1931	rBV4	3049	3343	0.17%	0.026%
59	14.368	1947	1952	1953	rBV4	5463	6786	0.34%	0.054%
60	14.415	1958	1960	1962	rVV3	2972	2685	0.13%	0.021%
61	14.545	1978	1982	1985	rVB5	4601	6476	0.32%	0.051%
62	14.692	2000	2007	2012	rVB6	10684	15701	0.79%	0.124%
63	14.733	2012	2014	2015	rVV2	2912	2527	0.13%	0.020%
64	14.774	2015	2021	2028	rVB2	42694	63984	3.21%	0.506%
65	14.933	2043	2048	2050	rBV6	1578	3209	0.16%	0.025%
66	15.068	2069	2071	2074	rBV4	2884	3184	0.16%	0.025%
67	15.133	2076	2082	2088	rBV	108154	150564	7.55%	1.191%
68	15.186	2088	2091	2097	rVB4	4834	8398	0.42%	0.066%
69	15.268	2100	2105	2107	rBV3	18254	24722	1.24%	0.195%
70	15.357	2117	2120	2122	rVB3	4070	3317	0.17%	0.026%
71	15.492	2141	2143	2147	rVB5	2865	3502	0.18%	0.028%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026081.D
 Acq On : 22 May 2020 15:28
 Operator : MA/SJ
 Sample : L2735-04DL 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5CB9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

72	15.615	2161	2164	2166	rBV3	2997	4000	0.20%	0.032%
73	15.639	2166	2168	2171	rVB3	2264	2425	0.12%	0.019%
74	16.180	2257	2260	2262	rBV4	2495	2729	0.14%	0.022%
75	16.251	2270	2272	2276	rVB5	3724	2777	0.14%	0.022%
76	16.280	2276	2277	2281	rVB4	2625	2405	0.12%	0.019%
77	16.433	2302	2303	2307	rVB3	2266	2654	0.13%	0.021%
78	16.545	2315	2322	2339	rBV	1263448	1727399	86.63%	13.660%
79	16.668	2339	2343	2348	rVV4	7317	12217	0.61%	0.097%
80	16.815	2364	2368	2369	rBV4	2382	2605	0.13%	0.021%
81	16.886	2373	2380	2391	rBV	1172485	1687286	84.62%	13.343%
82	16.980	2391	2396	2402	rBV	109778	156210	7.83%	1.235%
83	17.080	2411	2413	2414	rBV2	3661	2740	0.14%	0.022%
84	17.180	2427	2430	2431	rBV3	2646	2529	0.13%	0.020%
85	17.268	2442	2445	2446	rBV3	3255	2894	0.15%	0.023%
86	17.456	2475	2477	2478	rBV2	5002	3743	0.19%	0.030%
87	17.503	2482	2485	2489	rVV6	2137	4108	0.21%	0.032%
88	17.733	2521	2524	2525	rBV3	2295	2800	0.14%	0.022%
89	17.809	2534	2537	2539	rBV4	6427	6261	0.31%	0.050%
90	18.115	2587	2589	2592	rVB4	4195	4037	0.20%	0.032%
91	18.445	2643	2645	2646	rBV2	2676	2458	0.12%	0.019%
92	18.598	2667	2671	2673	rBV5	3403	4512	0.23%	0.036%
93	18.686	2684	2686	2687	rBV2	3051	3094	0.16%	0.024%
94	18.898	2720	2722	2724	rBV2	3289	2866	0.14%	0.023%
95	19.286	2783	2788	2794	rVB	133001	181436	9.10%	1.435%
96	19.345	2795	2798	2802	rBV	19734	24428	1.23%	0.193%
97	20.833	3048	3051	3055	rBV	64606	82949	4.16%	0.656%
98	20.880	3056	3059	3065	rVV	148049	179755	9.01%	1.421%
99	21.080	3089	3093	3103	rBV	1575020	1925988	96.59%	15.230%
100	23.203	3448	3454	3464	rVB	1164428	1994039	100.00%	15.768%


Sum of corrected areas: 12645928

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
Data File : BM026081.D
Acq On : 22 May 2020 15:28
Operator : MA/SJ
Sample : L2735-04DL 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

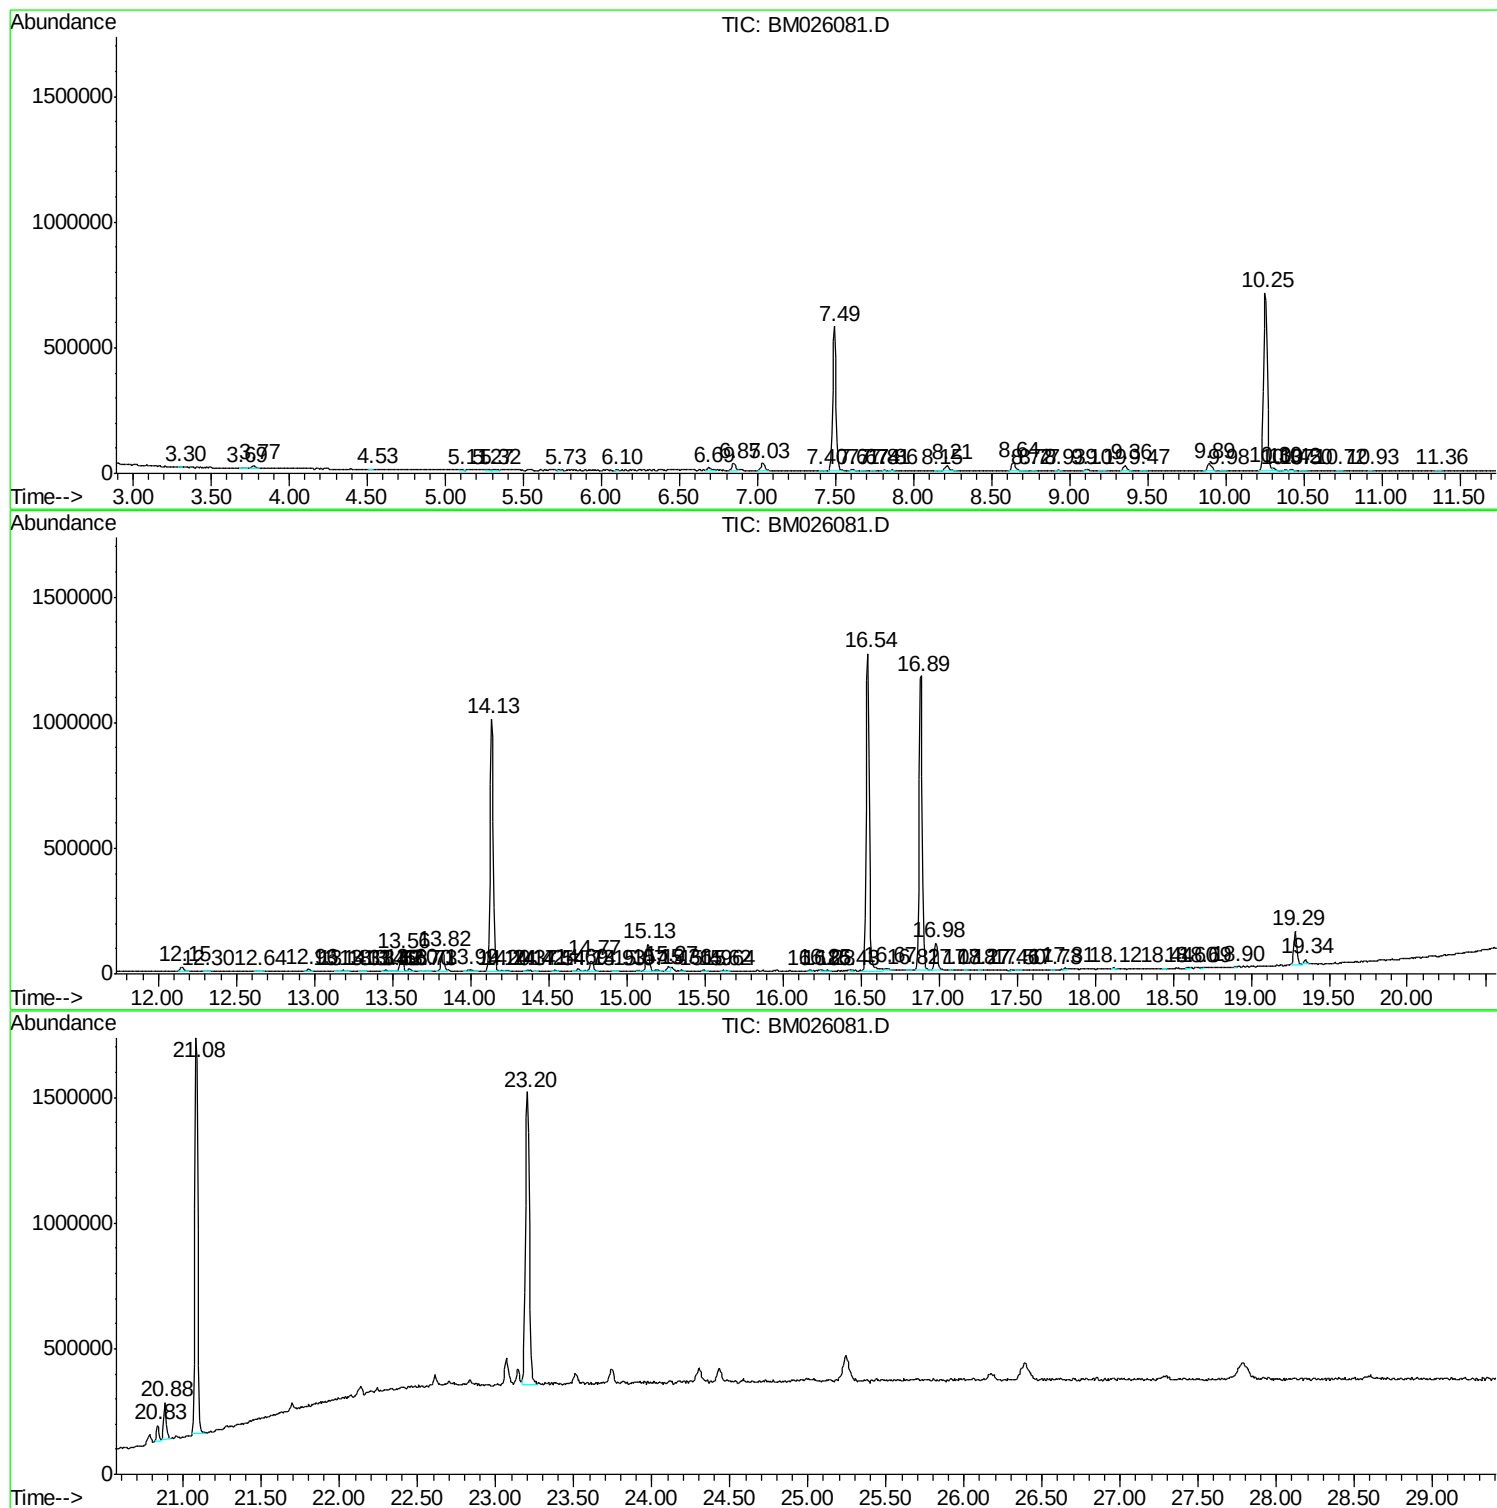

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052220\
Data File : BM026081.D
Acq On : 22 May 2020 15:28
Operator : MA/SJ
Sample : L2735-04DL 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052220\
Data File : BM026081.D
Acq On : 22 May 2020 15:28
Operator : MA/SJ
Sample : L2735-04DL 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5CB9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc