

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026085.D
 Acq On : 22 May 2020 18:32
 Operator : MA/SJ
 Sample : PB129075BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	27	31	41	rVB	72108	121300	2.38%	0.224%
2	3.605	118	122	131	rVB	41283	65368	1.28%	0.121%
3	3.770	146	150	155	rBV3	11800	18809	0.37%	0.035%
4	4.234	227	229	236	rVB5	9926	15666	0.31%	0.029%
5	6.128	547	551	557	rVB8	2877	6441	0.13%	0.012%
6	6.687	639	646	656	rBV	1290231	1933739	37.92%	3.567%
7	6.840	666	672	683	rBV	896468	1356741	26.60%	2.503%
8	7.034	696	705	717	rBV	1191728	1900716	37.27%	3.506%
9	7.493	775	783	793	rBV	751628	1190951	23.35%	2.197%
10	8.205	897	904	918	rBV	1420223	2142128	42.00%	3.952%
11	8.634	970	977	985	rBV	1097205	1700719	33.35%	3.138%
12	9.352	1090	1099	1108	rBV	838096	1346120	26.40%	2.483%
13	9.887	1182	1190	1201	rBV	1282885	2080755	40.80%	3.839%
14	10.252	1245	1252	1265	rBV	1004033	1613284	31.63%	2.976%
15	10.393	1269	1276	1292	rVV	1200090	2053397	40.26%	3.788%
16	11.816	1513	1518	1520	rBV6	4769	8794	0.17%	0.016%
17	11.851	1520	1524	1532	rVB3	19354	33001	0.65%	0.061%
18	13.557	1807	1814	1824	rBV	2009173	2612135	51.22%	4.819%
19	13.822	1852	1859	1872	rBV	2337958	3154453	61.85%	5.819%
20	13.987	1883	1887	1890	rBV6	3577	5944	0.12%	0.011%
21	14.134	1906	1912	1921	rBV2	1373619	1951022	38.26%	3.599%
22	14.351	1939	1949	1964	rBV	993360	1488854	29.19%	2.747%
23	15.134	2074	2082	2089	rBV	2740975	3830412	75.11%	7.066%
24	15.263	2098	2104	2116	rBV	845391	1131567	22.19%	2.088%
25	15.375	2119	2123	2129	rVB	33570	47059	0.92%	0.087%
26	15.669	2167	2173	2175	rVB6	3471	5385	0.11%	0.010%
27	15.845	2194	2203	2207	rBV9	5784	14754	0.29%	0.027%
28	15.922	2211	2216	2220	rBV4	10721	16011	0.31%	0.030%
29	16.675	2340	2344	2346	rBV4	5912	8302	0.16%	0.015%
30	16.886	2373	2380	2389	rBV	1650241	2306449	45.23%	4.255%
31	16.980	2390	2396	2408	rVV2	2904115	4042528	79.27%	7.458%
32	17.063	2408	2410	2415	rVB6	4478	5631	0.11%	0.010%
33	17.816	2533	2538	2541	rBV6	5796	8747	0.17%	0.016%
34	18.122	2584	2590	2593	rBV8	7369	13545	0.27%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
 Data File : BM026085.D
 Acq On : 22 May 2020 18:32
 Operator : MA/SJ
 Sample : PB129075BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	18.180	2598	2600	2605	rVB6	3825	5293	0.10%	0.010%
36	18.851	2710	2714	2716	rVB4	4374	5211	0.10%	0.010%
37	18.916	2720	2725	2733	rBV	33891	56660	1.11%	0.105%
38	19.169	2764	2768	2772	rVB	28268	37786	0.74%	0.070%
39	19.286	2777	2788	2794	rBV	3667582	4748636	93.11%	8.760%
40	19.345	2796	2798	2802	rVB2	12087	14589	0.29%	0.027%
41	20.780	3037	3042	3047	rBV	50978	102245	2.00%	0.189%
42	20.833	3048	3051	3055	rVV	71603	91387	1.79%	0.169%
43	20.880	3055	3059	3066	rVV	191040	245816	4.82%	0.453%
44	21.080	3088	3093	3101	rBV	2274394	2762104	54.16%	5.096%
45	23.074	3425	3432	3439	rBV	3000704	5099765	100.00%	9.408%
46	23.204	3448	3454	3462	rVB	1628699	2805360	55.01%	5.175%


Sum of corrected areas: 54205579

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052220\
Data File : BM026085.D
Acq On : 22 May 2020 18:32
Operator : MA/SJ
Sample : PB129075BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

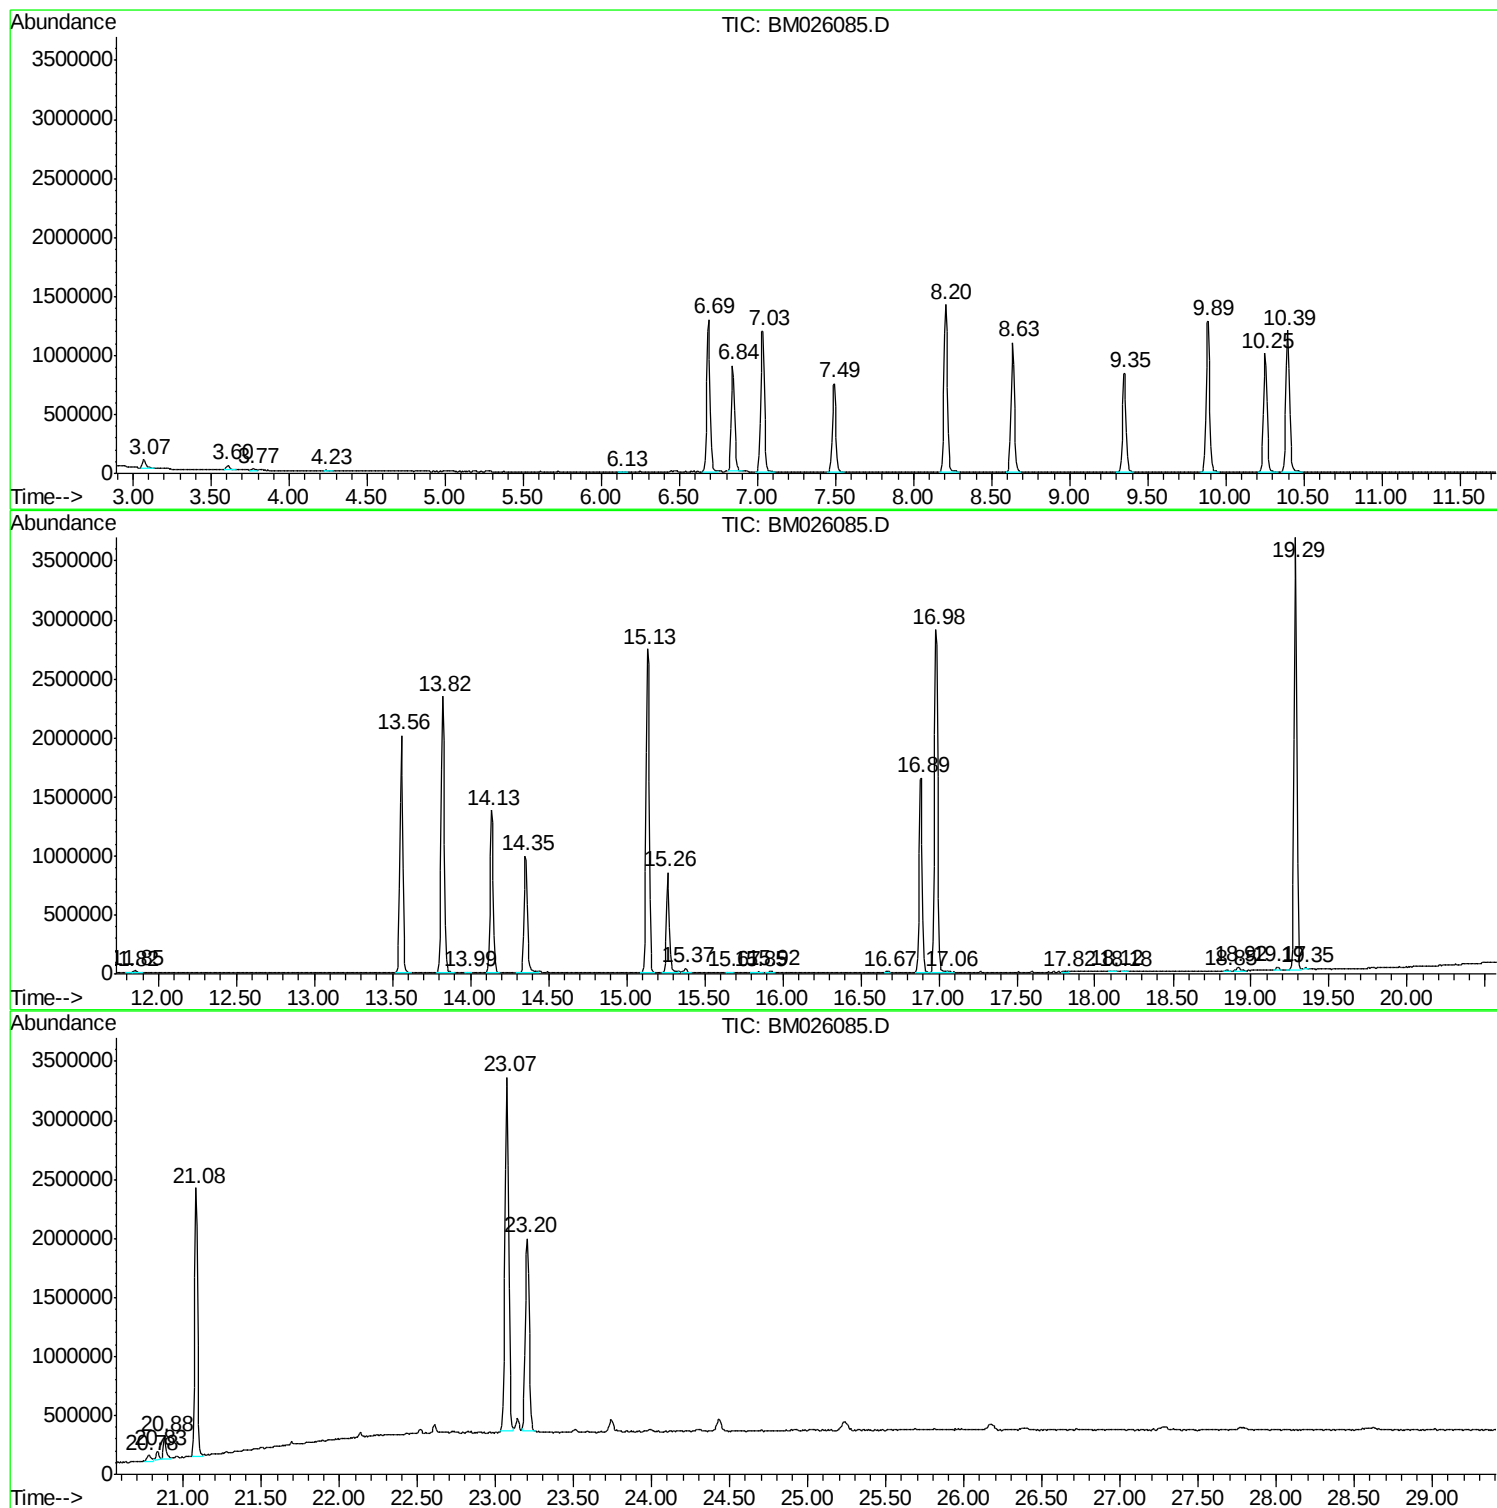

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052220\
Data File : BM026085.D
Acq On : 22 May 2020 18:32
Operator : MA/SJ
Sample : PB129075BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052220\
Data File : BM026085.D
Acq On : 22 May 2020 18:32
Operator : MA/SJ
Sample : PB129075BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK75

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
