

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045747.D
Acq On : 22 May 2024 18:04
Operator : MA/JU
Sample : PB160974BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160974BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM045747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.252	362	368	388	rBV	5948652	8911656	55.58%	11.204%
2	6.840	630	638	652	rBV	5540810	9211902	57.45%	11.581%
3	7.569	755	762	770	rBV	1148215	1736516	10.83%	2.183%
4	8.734	951	960	974	rBV	3456093	6034683	37.64%	7.587%
5	10.339	1226	1233	1244	rBV	1424042	2385389	14.88%	2.999%
6	12.827	1648	1656	1664	rBV	7859498	11829103	73.78%	14.872%
7	14.198	1881	1889	1899	rBV	2059223	3078946	19.20%	3.871%
8	15.704	2132	2145	2160	rBV	6369984	9359492	58.37%	11.767%
9	16.945	2350	2356	2363	rBV	2534729	3556903	22.18%	4.472%
10	19.586	2799	2805	2810	rBV	12828405	16033685	100.00%	20.158%
11	21.162	3068	3073	3079	rBV	2788368	3622138	22.59%	4.554%
12	23.956	3541	3548	3558	rVB	1655917	3779575	23.57%	4.752%




Sum of corrected areas: 79539988

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045747.D
Acq On : 22 May 2024 18:04
Operator : MA/JU
Sample : PB160974BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160974BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

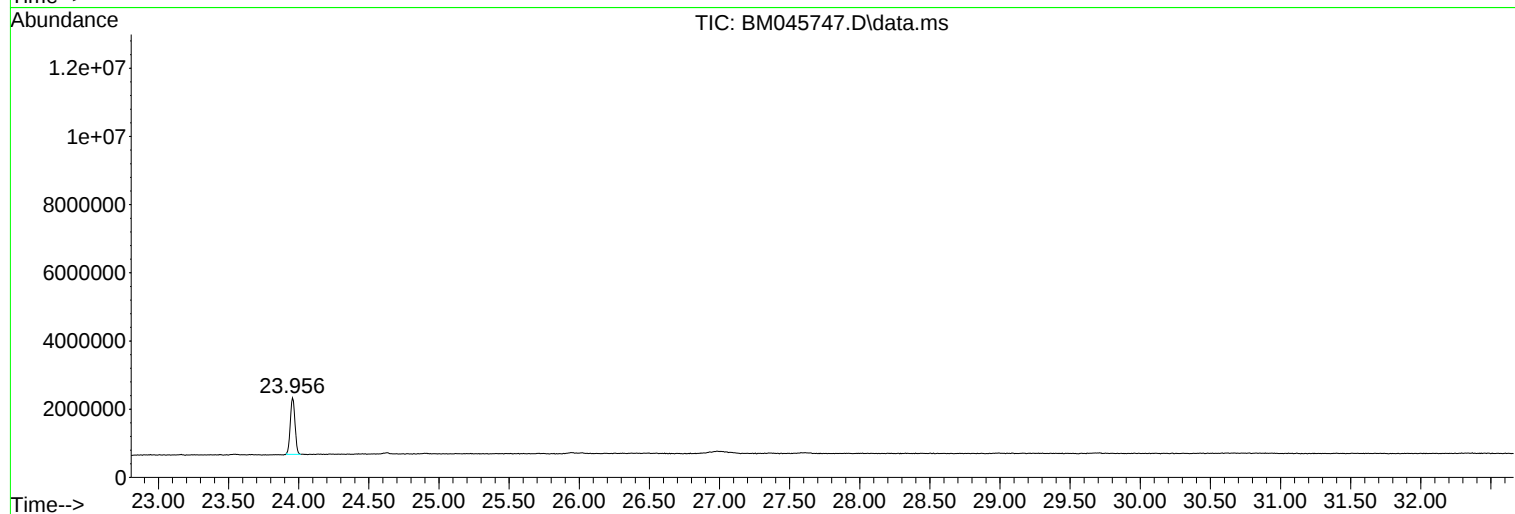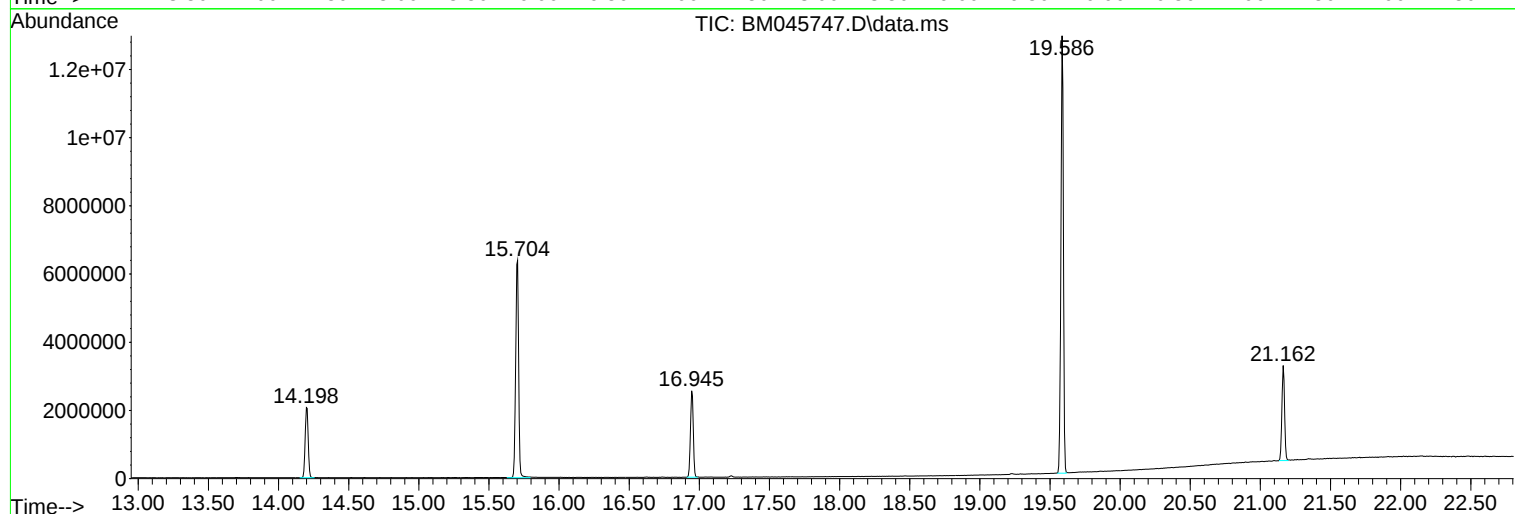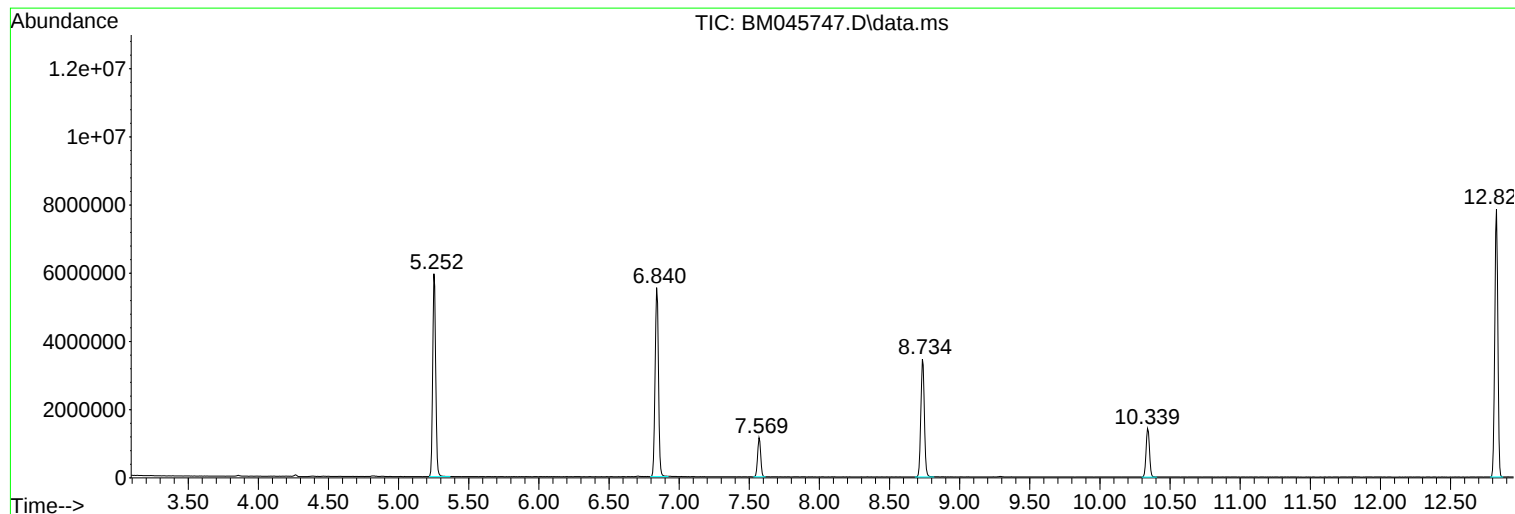

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045747.D
Acq On : 22 May 2024 18:04
Operator : MA/JU
Sample : PB160974BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160974BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045747.D
Acq On : 22 May 2024 18:04
Operator : MA/JU
Sample : PB160974BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160974BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------