


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045737.D
Acq On : 22 May 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 23 04:12:56 2024

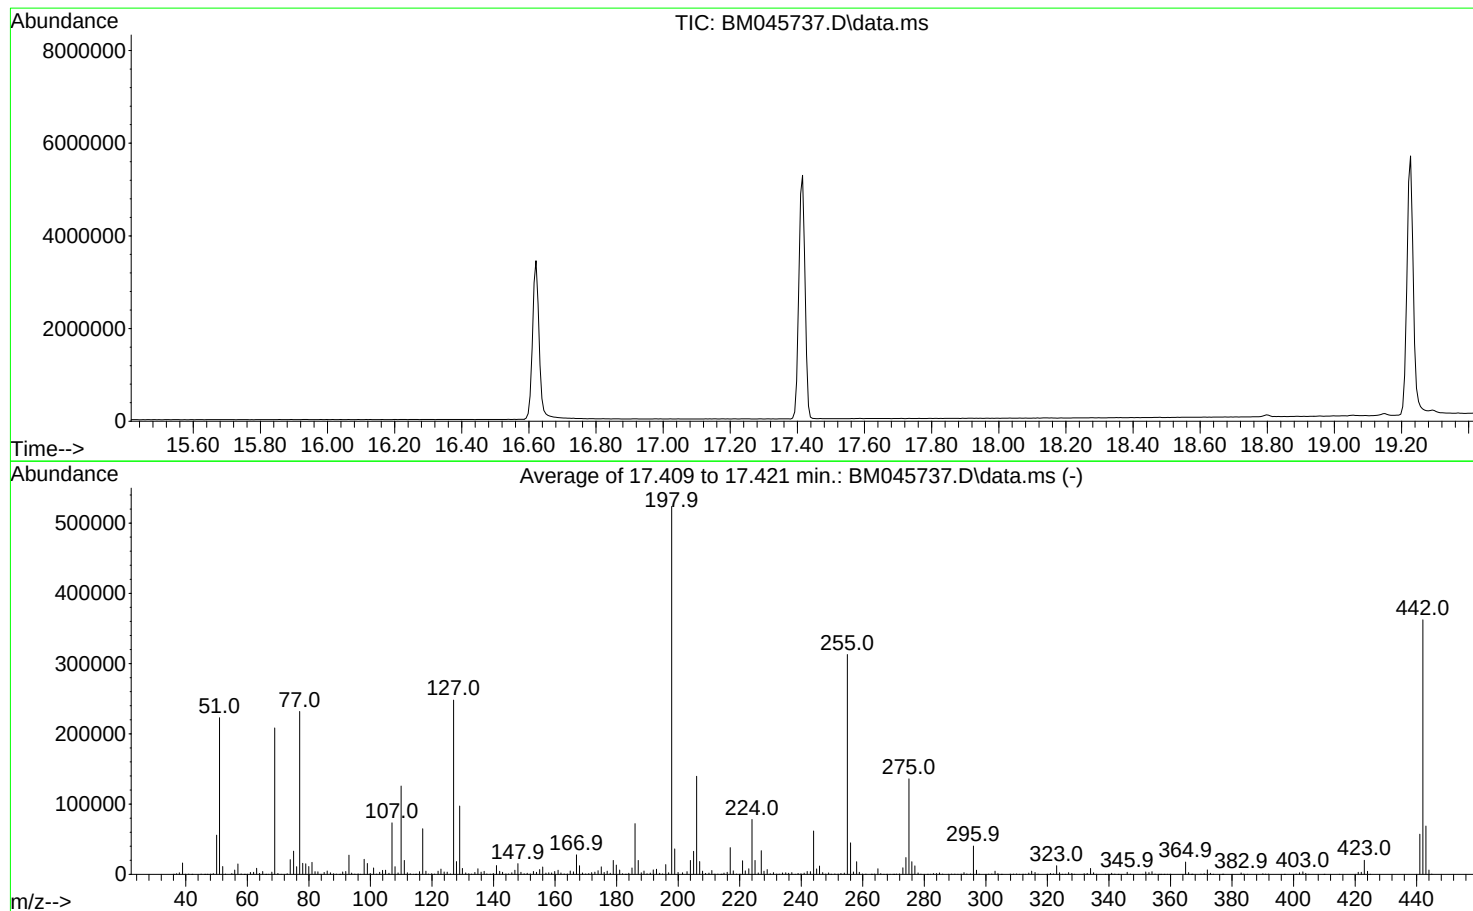




AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	222977	PASS
68	69	0.00	2	1.5	3129	PASS
69	198	0.00	100	39.8	208428	PASS
70	69	0.00	2	0.6	1295	PASS
127	198	10	80	47.4	248107	PASS
197	198	0.00	2	0.4	2301	PASS
198	198	100	100	100.0	523584	PASS
199	198	5	9	6.9	36240	PASS
275	198	10	60	26.0	135976	PASS
365	198	1	100	3.4	17604	PASS
441	198	0.01	100	10.9	57304	PASS
442	442	50	100	100.0	362325	PASS
443	442	15	24	19.0	68867	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045737.D
Acq On : 22 May 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 23 04:19:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

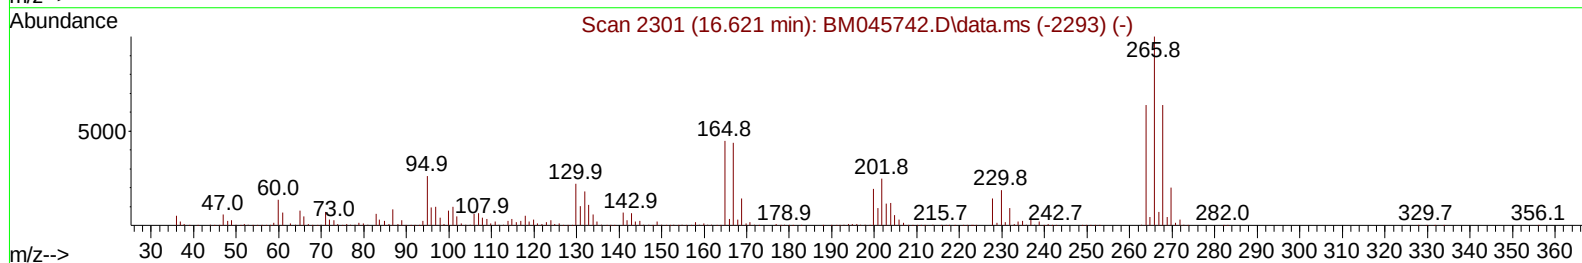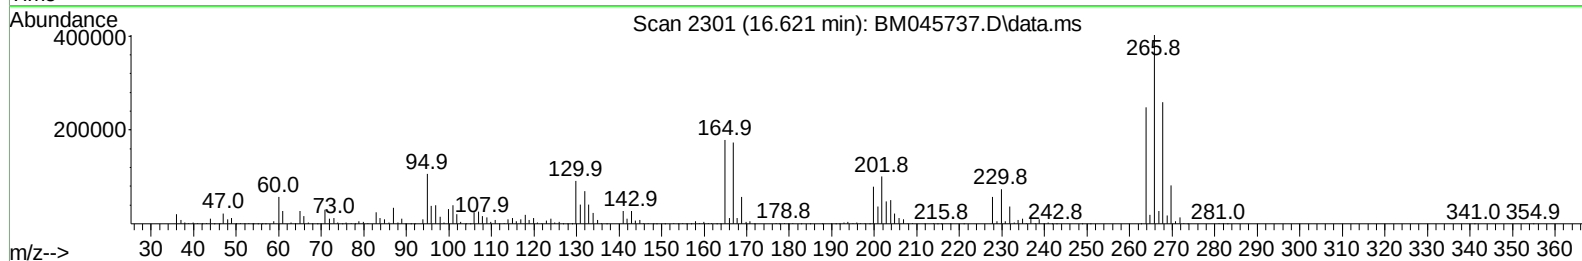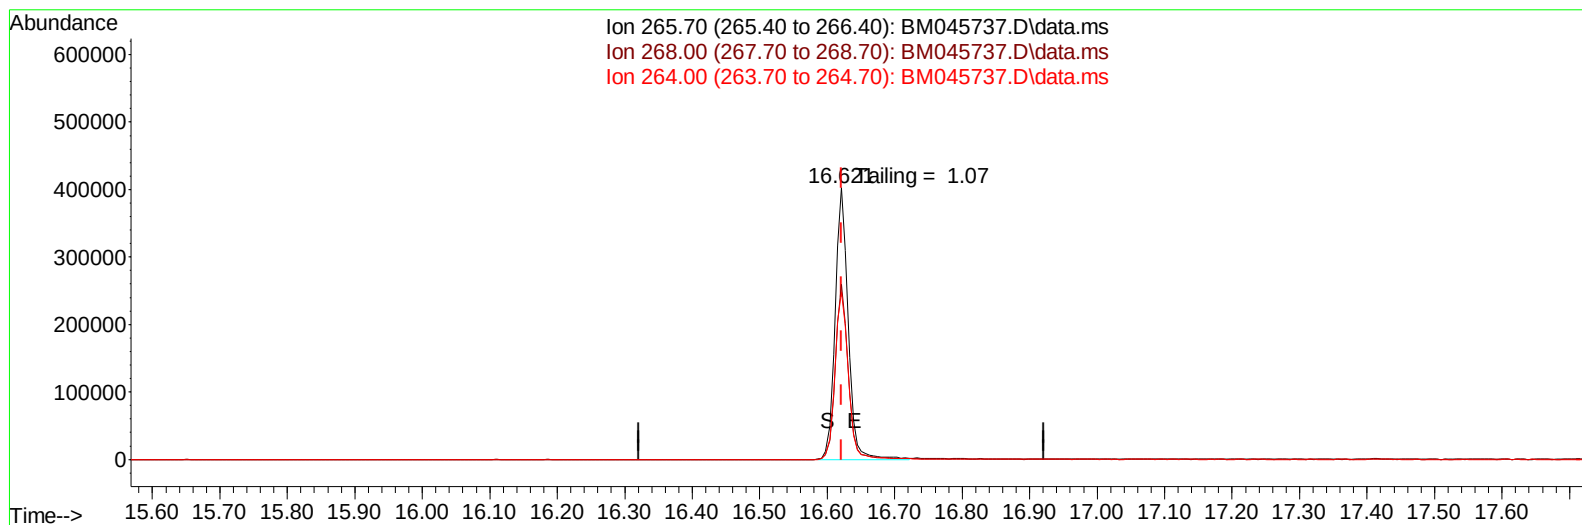

TIC: BM045737.D\data.ms

(70) Pentachlorophenol (C)

16.621min (+ 0.000) 0.00 ng




response 542727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.58
264.00	63.60	61.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052224\
Data File : BM045737.D
Acq On : 22 May 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 23 04:19:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

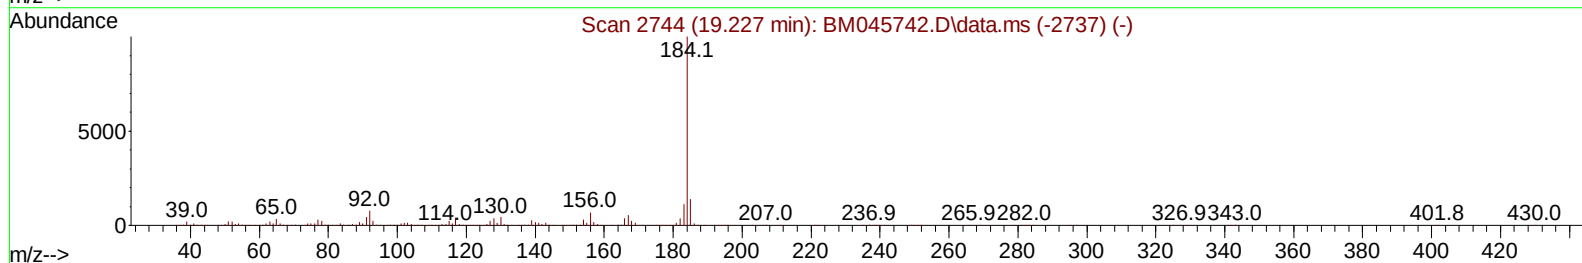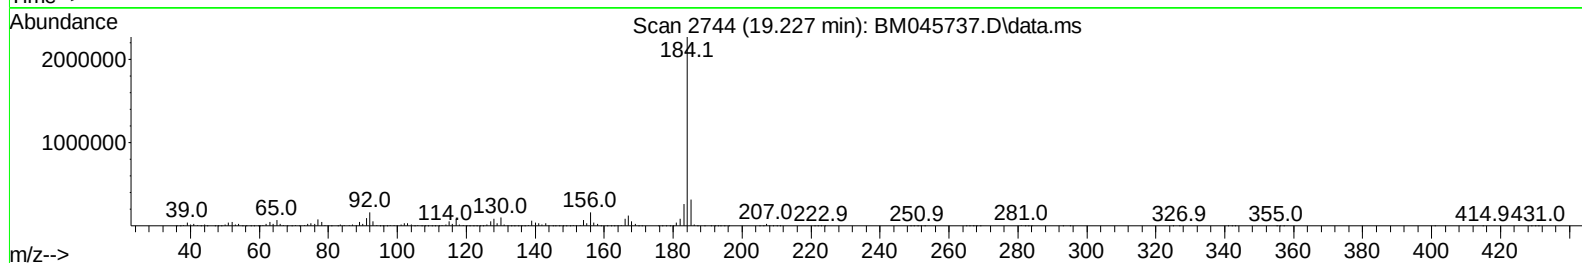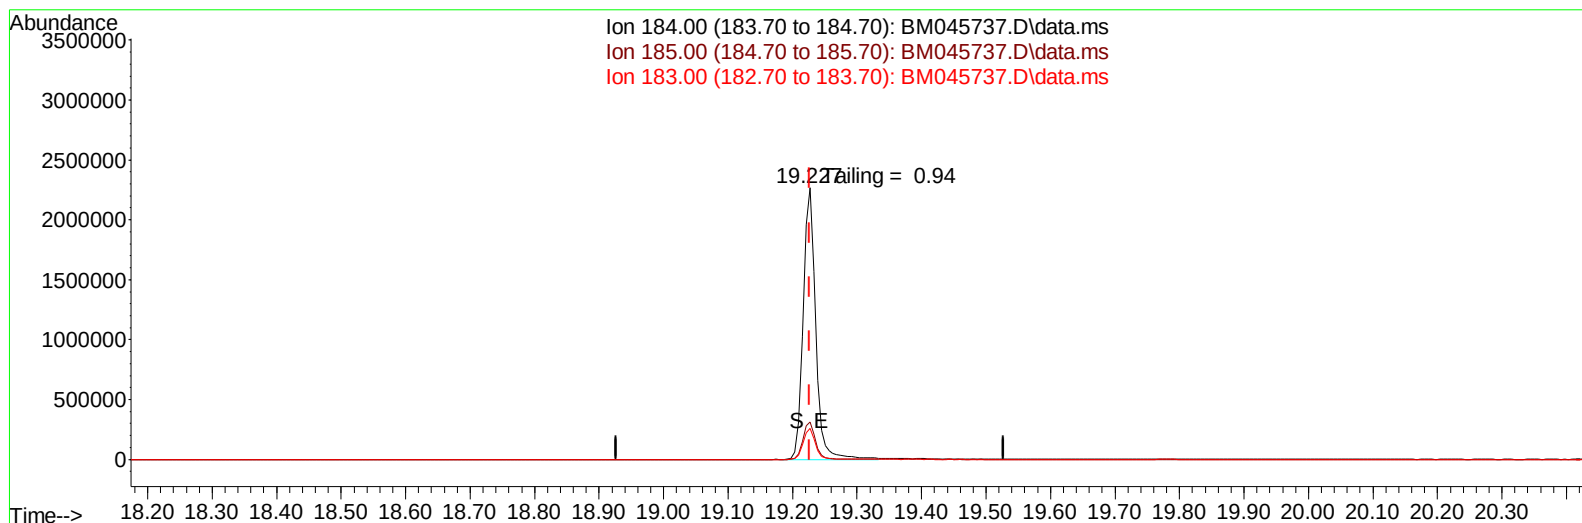

TIC: BM045737.D\data.ms

(77) Benzidine

19.227min (+ 0.000) 0.00 ng

response 3070049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.86
183.00	11.30	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/22/2024	BNA_M	<u>BM045737.D</u>
Compound Name	Response	Retention Time
DDT	1730211	20.444
DDD	21958	20.056
DDE	1726	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23684	1753895	1.35

Instrument :
BNA_M
ClientSampleId :
DFTPP