

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052317\
 Data File : BM010150.D
 Acq On : 23 May 2017 20:05
 Operator : SJ/MA
 Sample : I3282-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 24 05:25:24 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 20 04:25:49 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	141249	20.00	ng	-0.02
21) Naphthalene-d8	10.76	136	475559	20.00	ng	-0.02
38) Acenaphthene-d10	14.59	164	311409	20.00	ng	-0.02
63) Phenanthrene-d10	17.33	188	806037	20.00	ng	-0.02
75) Chrysene-d12	21.49	240	1200751	20.00	ng	-0.02
86) Perylene-d12	23.86	264	1322571	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	506843	64.80	ng	-0.02
7) Phenol-d6	7.14	99	389106	38.66	ng	-0.03
23) Nitrobenzene-d5	9.15	82	894501	101.48	ng	-0.02
41) 2,4,6-Tribromophenol	16.08	330	731150	154.59	ng	-0.02
44) 2-Fluorobiphenyl	13.21	172	2287057	94.41	ng	-0.02
78) Terphenyl-d14	19.93	244	4148939	78.57	ng	-0.02
Target Compounds						
15) Benzyl Alcohol	8.27	79	18377	2.41	ng	# 38
18) Hexachloroethane	9.05	117	8586	2.38	ng	# 8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052317\
Data File : BM010150.D
Acq On : 23 May 2017 20:05
Operator : SJ/MA
Sample : I3282-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 24 05:25:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

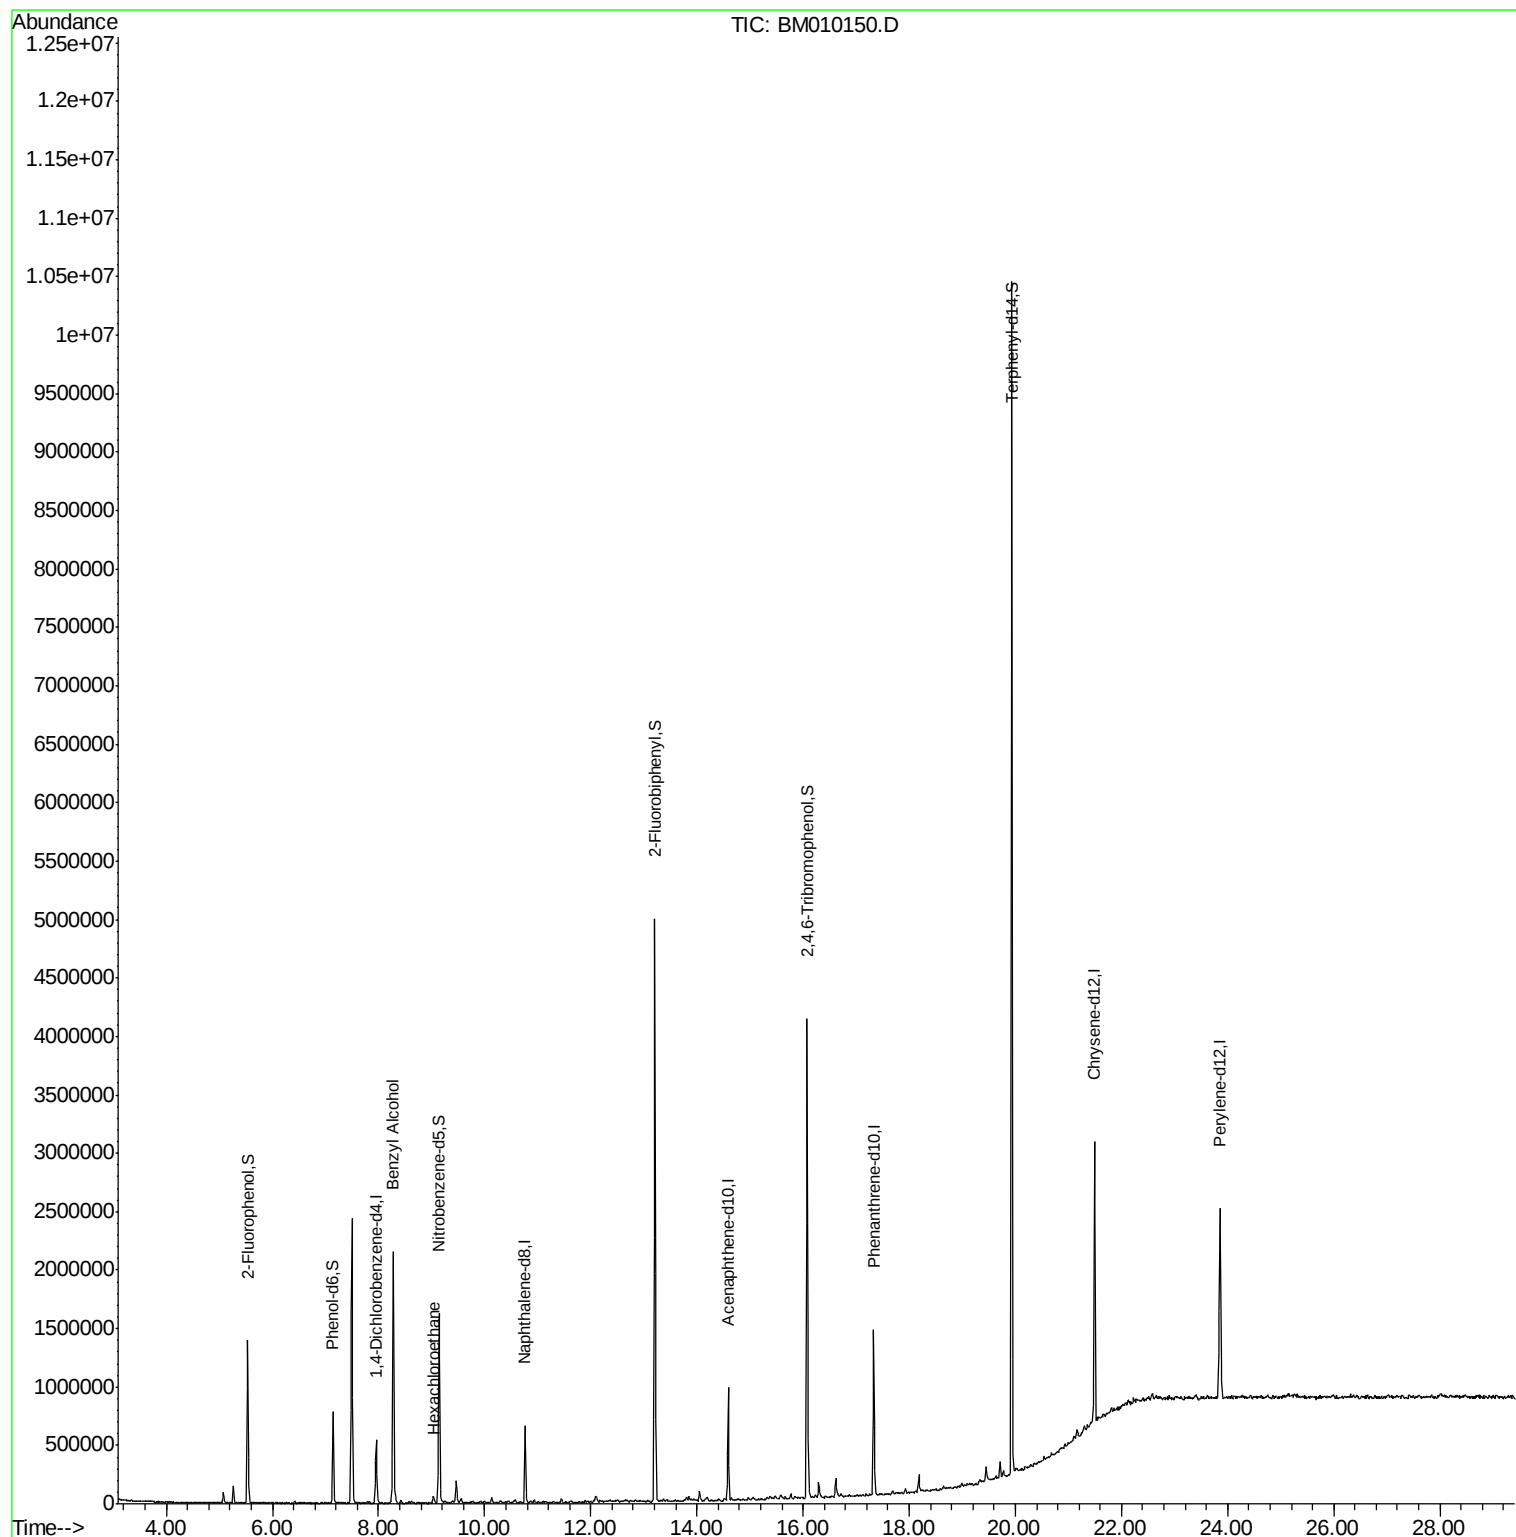

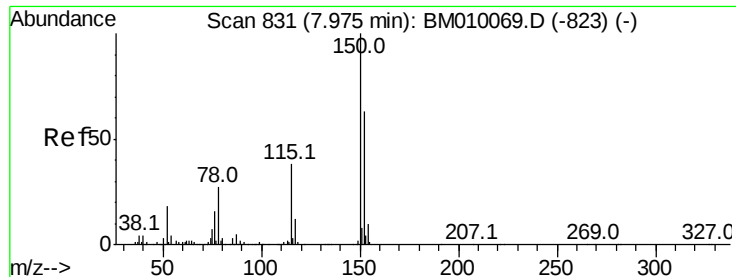

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.96 min Scan# 828

Delta R.T. -0.02 min

Lab File: BM010150.D

Acq: 23 May 2017 20:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:152 Resp: 141249

Ion Ratio Lower Upper

152 100

150 150.5 119.5 179.3




115 57.8 43.0 64.4

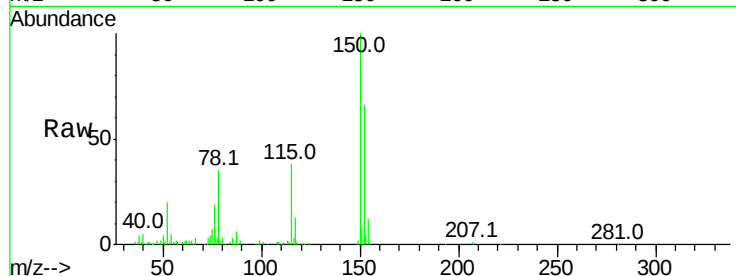

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

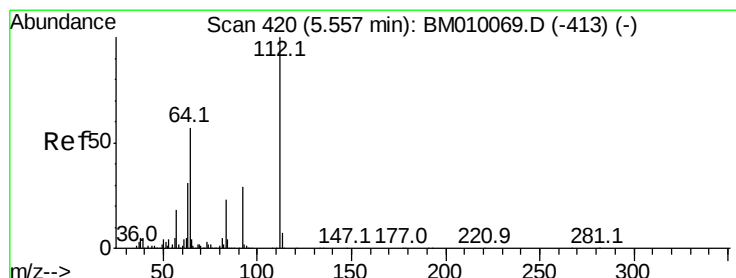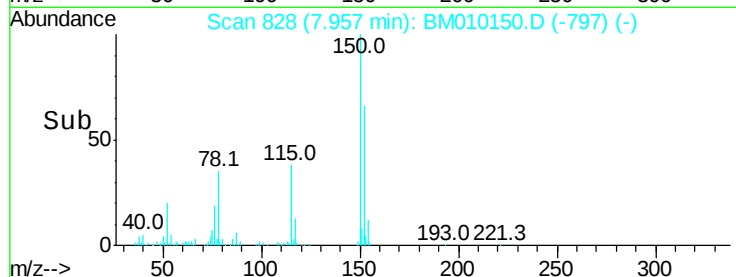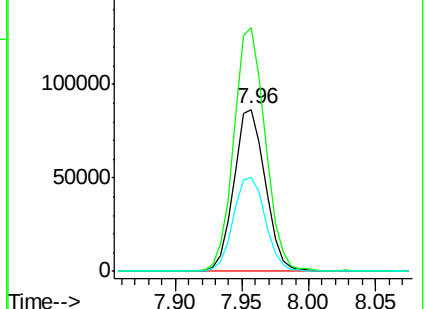

#5

2-Fluorophenol

Concen: 64.80 ng

RT: 5.53 min Scan# 416

Delta R.T. -0.02 min

Lab File: BM010150.D

Acq: 23 May 2017 20:05


Tgt Ion:112 Resp: 506843

Ion Ratio Lower Upper

112 100

64 64.2 38.6 57.8#



63 38.5 19.3 28.9#

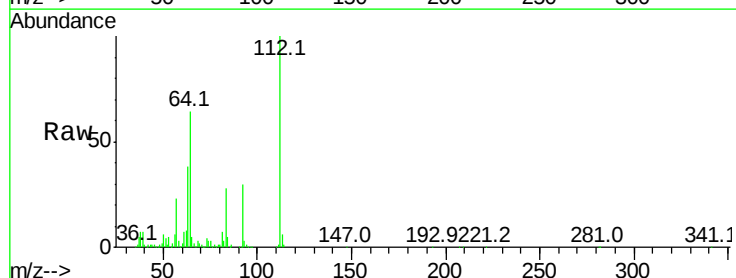


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

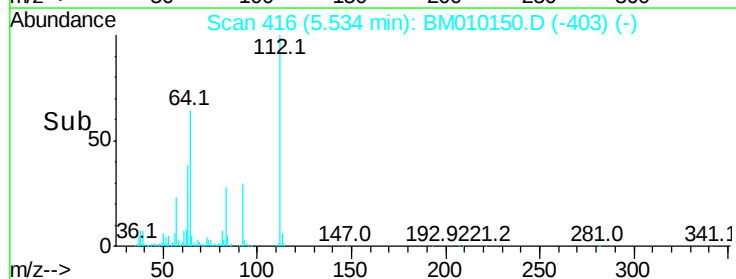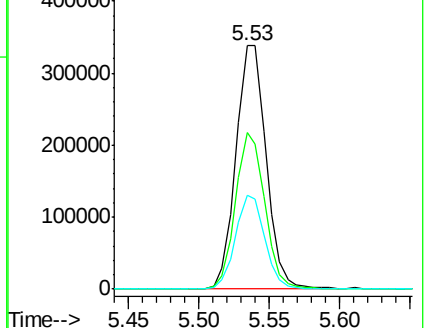

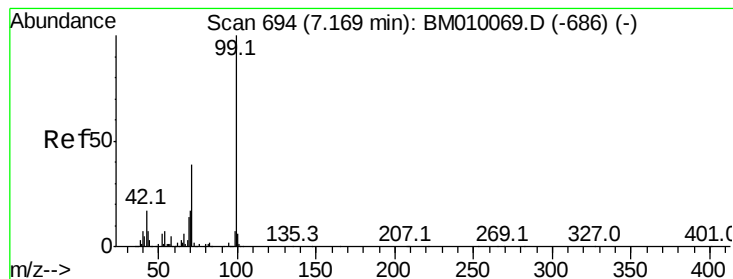

#7

Phenol-d6

Concen: 38.66 ng

RT: 7.14 min Scan# 689

Delta R.T. -0.03 min

Lab File: BM010150.D

Acq: 23 May 2017 20:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 389106

Ion Ratio Lower Upper

99 100

42 21.6 11.0 16.4#




71 48.4 23.4 35.2#

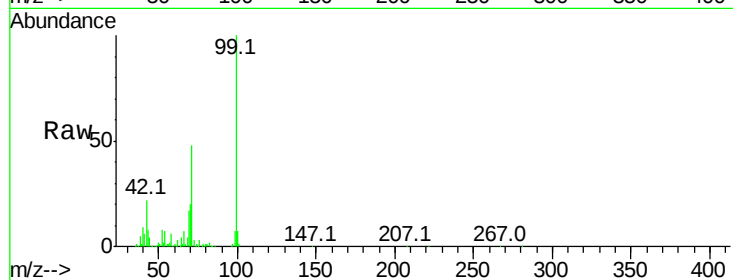

Abundance Ion 99.00 (98.70 to 99.70): BM010150.D (-686) (-)

Ion 42.00 (41.70 to 42.70): BM010150.D (-686) (-)

Ion 71.00 (70.70 to 71.70): BM010150.D (-686) (-)

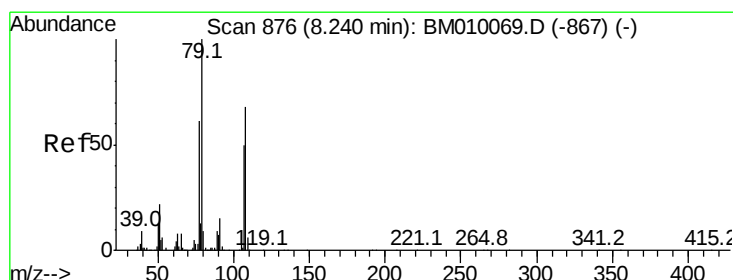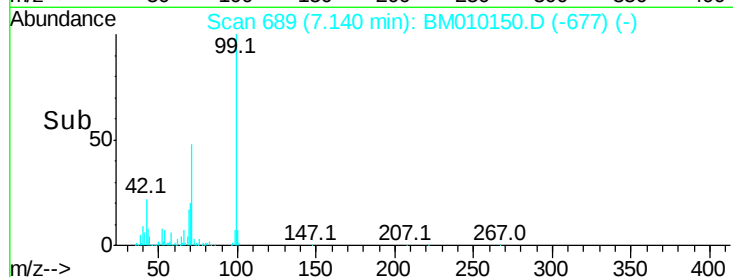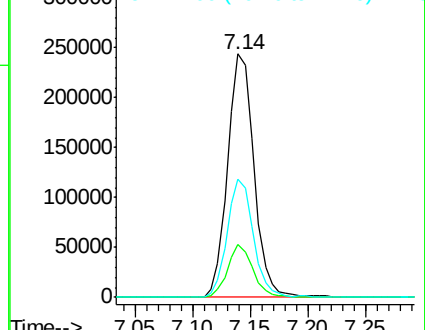

#15

Benzyl Alcohol

Concen: 2.41 ng

RT: 8.27 min Scan# 882

Delta R.T. 0.04 min

Lab File: BM010150.D

Acq: 23 May 2017 20:05


Tgt Ion: 79 Resp: 18377

Ion Ratio Lower Upper

79 100

108 41.1 65.0 97.4#



77 131.7 53.0 79.6#

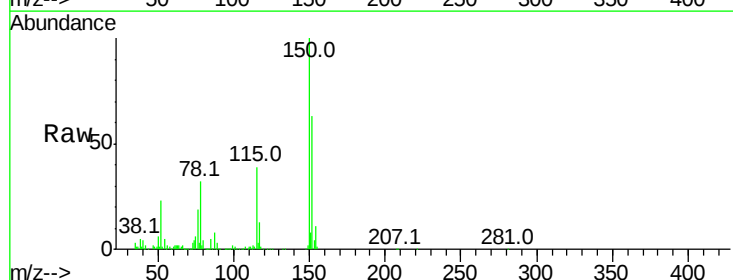


Abundance Ion 79.00 (78.70 to 79.70): BM010150.D (-867) (-)

Ion 108.00 (107.70 to 108.70): BM010150.D (-867) (-)

Ion 77.00 (76.70 to 77.70): BM010150.D (-867) (-)

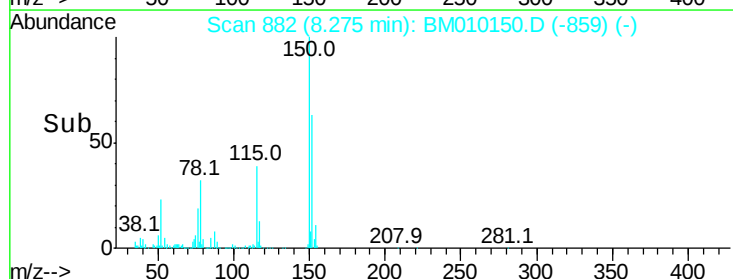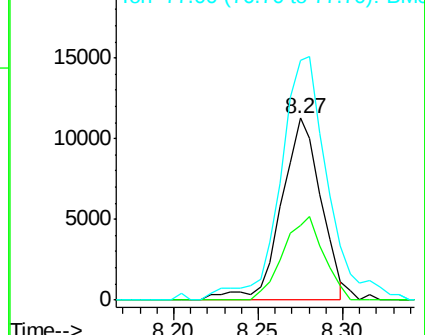

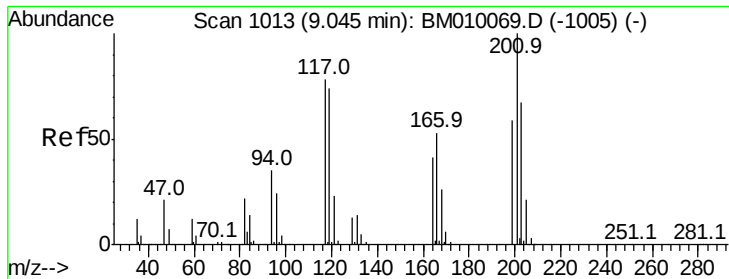

#18

Hexachloroethane

Concen: 2.38 ng

RT: 9.05 min Scan# 1013

Delta R.T. -0.00 min

Lab File: BM010150.D

Acq: 23 May 2017 20:05

Instrument :

BNA_M

ClientSampled :


Tot Ion:117 Resp: 8586

Ion Ratio Lower Upper

117 100

119 187.8 79.2 118.8#




201 0.0 69.8 104.6#

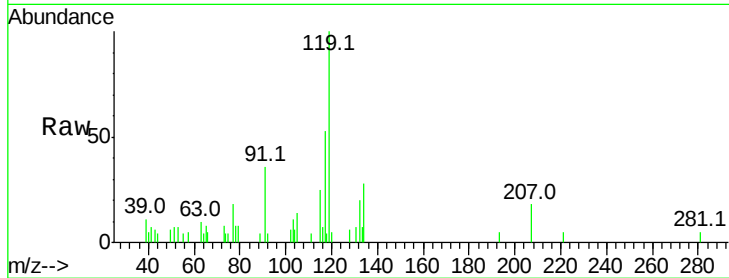

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 119.00 (118.70 to 119.70): E

Ion 201.00 (200.70 to 201.70): E

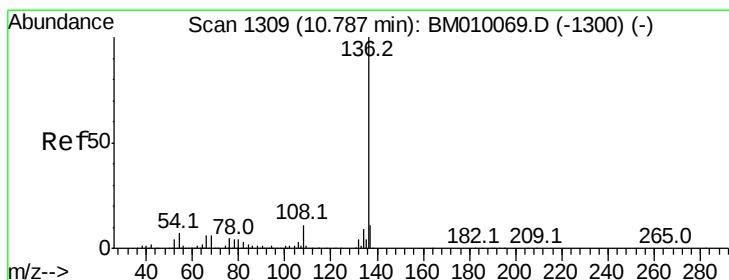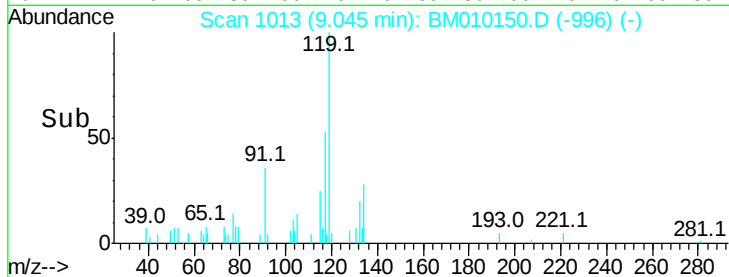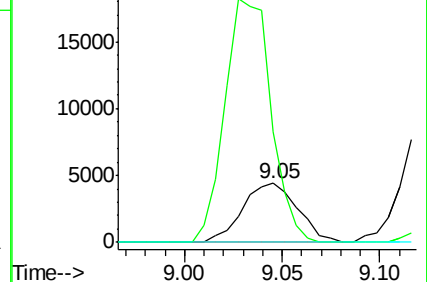

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.76 min Scan# 1305

Delta R.T. -0.02 min

Lab File: BM010150.D

Acq: 23 May 2017 20:05

Tgt Ion:136 Resp: 475559


Ion Ratio Lower Upper

136 100

137 10.4 8.7 13.1

54 6.6 4.6 6.8

68 4.8 3.7 5.5


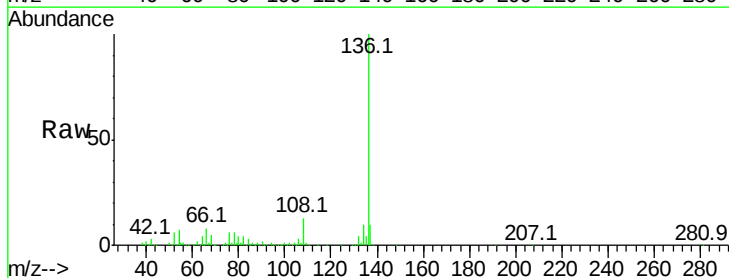



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM0

Ion 68.00 (67.70 to 68.70): BM0



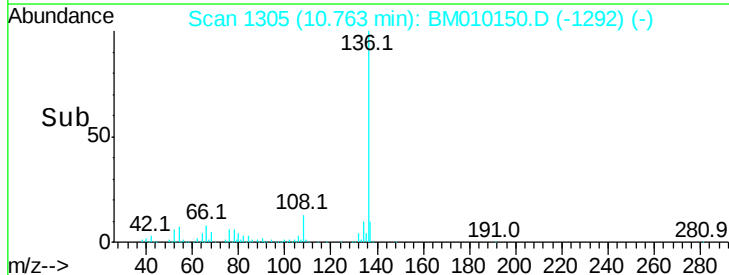
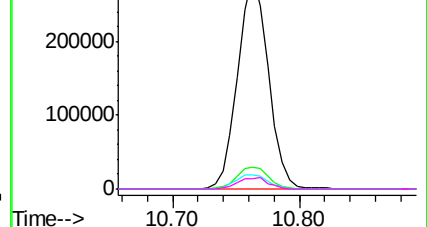


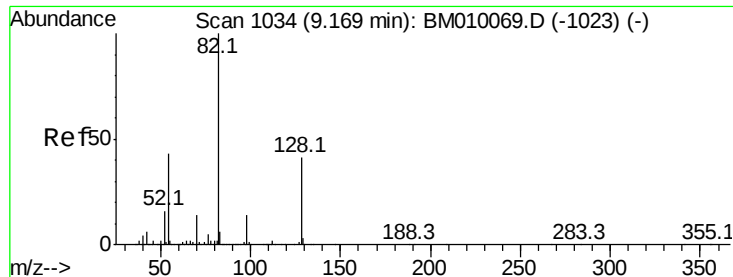

#23
 Nitrobenzene-d5
 Concen: 101.48 ng
 RT: 9.15 min Scan# 1030
 Delta R.T. -0.02 min
 Lab File: BM010150.D
 Acq: 23 May 2017 20:05




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
82	100		
128	36.3	32.8	49.2
54	46.4	40.6	60.8

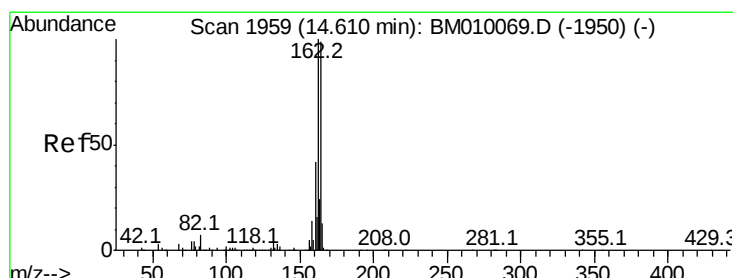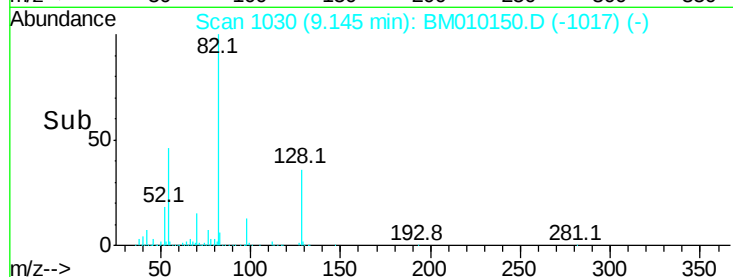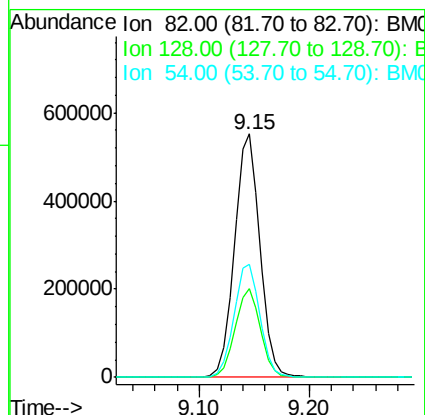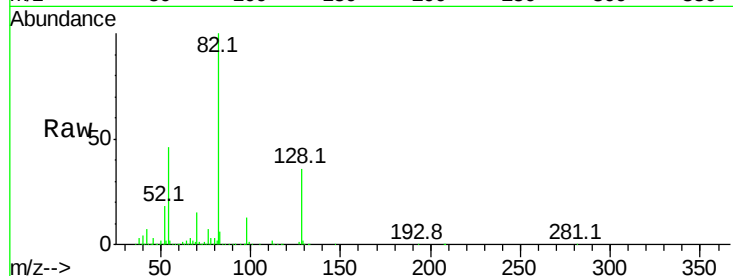

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.59 min Scan# 1955
 Delta R.T. -0.02 min
 Lab File: BM010150.D
 Acq: 23 May 2017 20:05

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.5	82.4	123.6
160	45.5	35.8	53.6


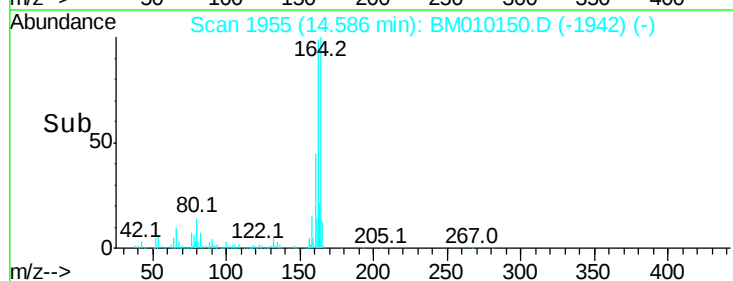
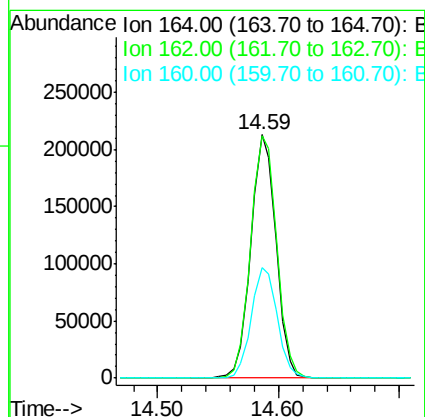
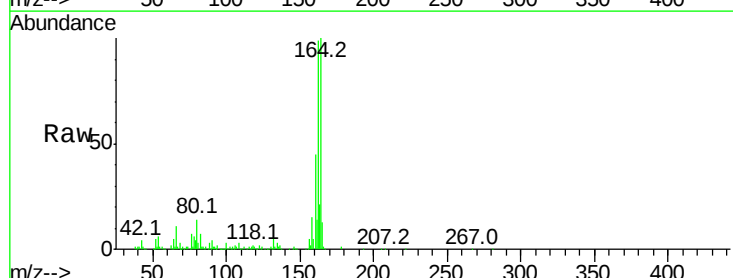


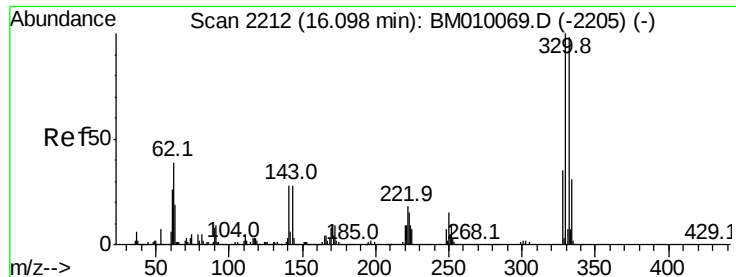

#41
 2,4,6-Tribromophenol
 Concen: 154.59 ng
 RT: 16.08 min Scan# 2209
 Delta R.T. -0.02 min
 Lab File: BM010150.D
 Acq: 23 May 2017 20:05




Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	0.0	0.0#
141	33.2	0.0	0.0#

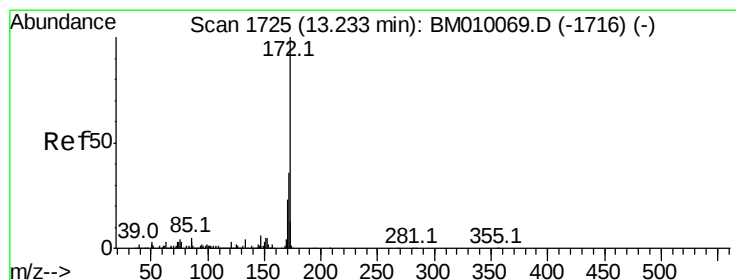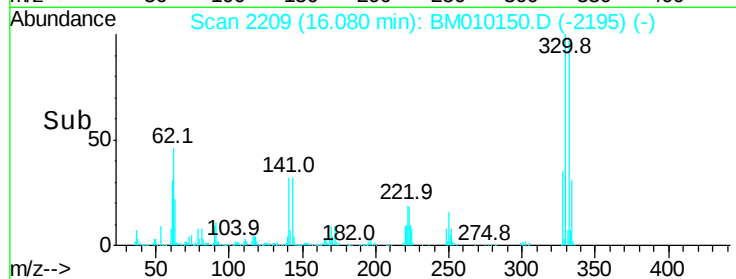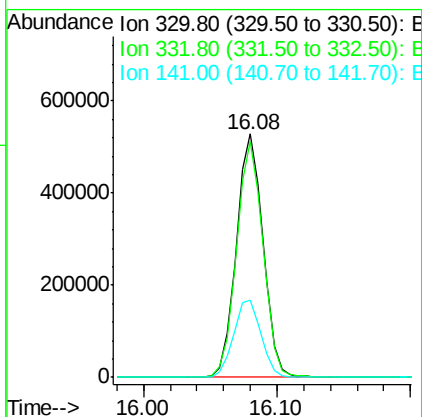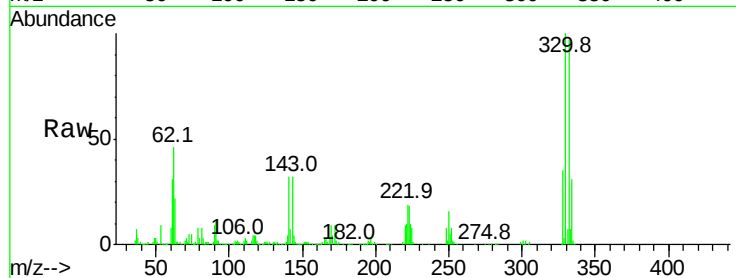

#44
 2-Fluorobiphenyl
 Concen: 94.41 ng
 RT: 13.21 min Scan# 1721
 Delta R.T. -0.02 min
 Lab File: BM010150.D
 Acq: 23 May 2017 20:05

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.2	28.5	42.7
170	22.7	18.8	28.2


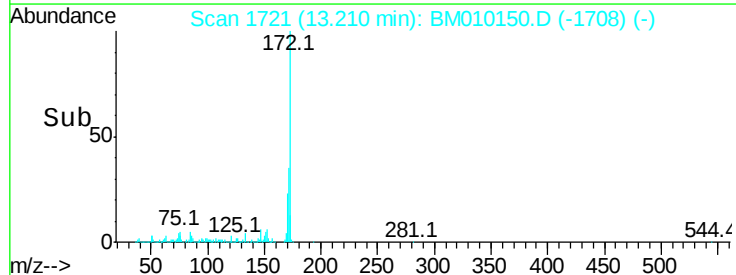
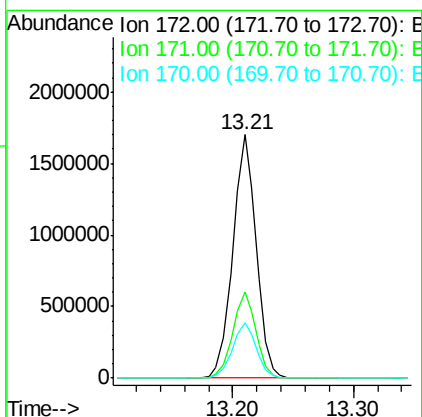
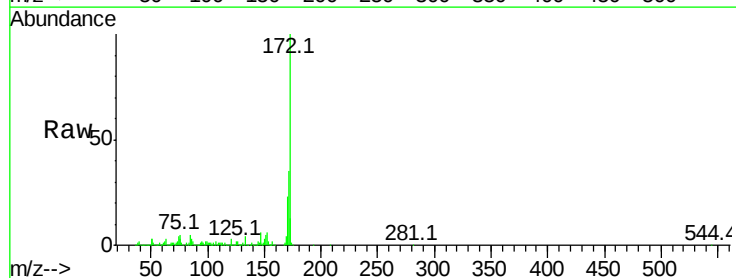




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.33 min Scan# 2422
Delta R.T. -0.02 min
Lab File: BM010150.D
Acq: 23 May 2017 20:05




Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
188	100		
94	6.0	8.7	13.1#
80	6.6	9.3	13.9#

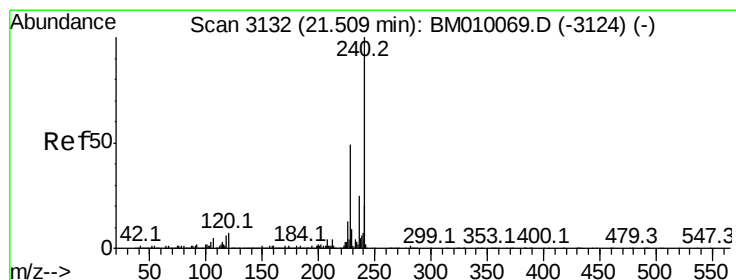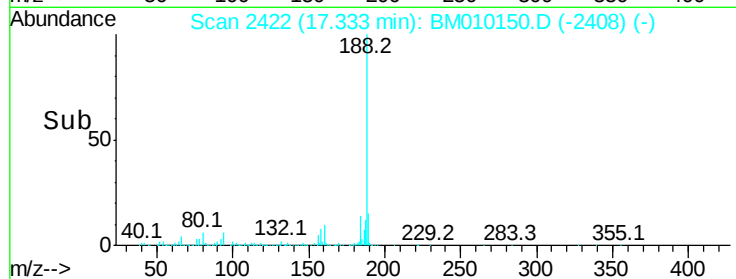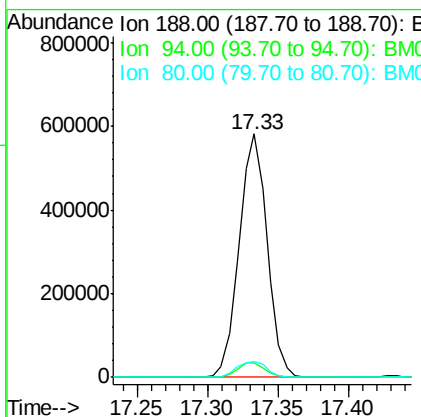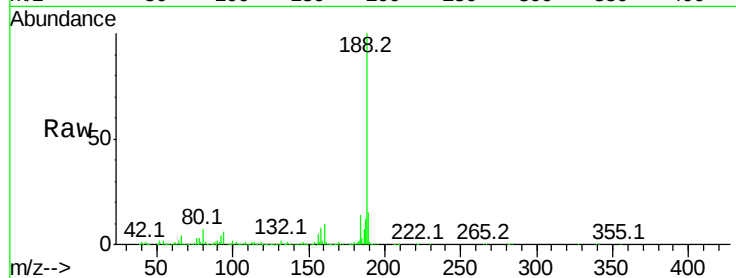

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.49 min Scan# 3129
Delta R.T. -0.02 min
Lab File: BM010150.D
Acq: 23 May 2017 20:05

Tgt Ion	Ratio	Lower	Upper
240	100		
120	5.7	8.2	12.2#
236	25.4	20.0	30.0


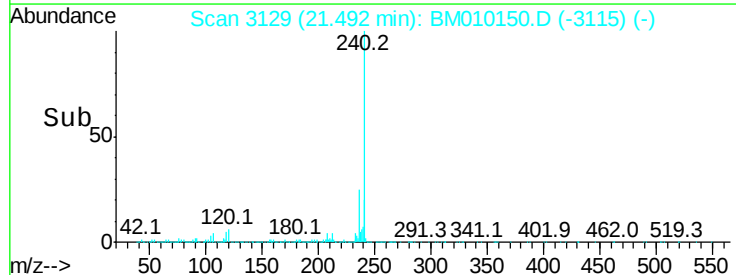
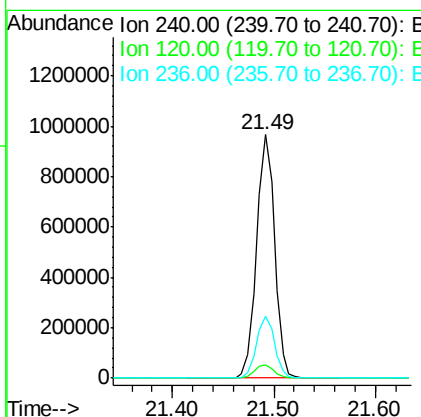
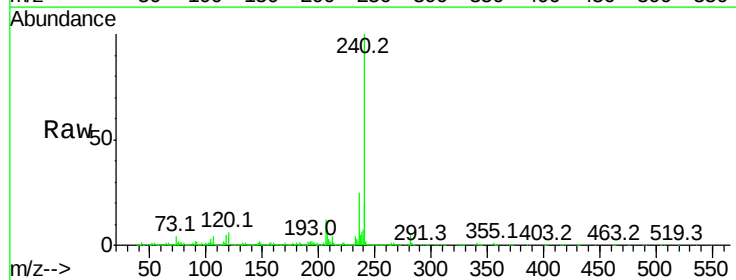




#78
 Terphenyl-d14
 Concen: 78.57 ng
 RT: 19.93 min Scan# 2864
 Delta R.T. -0.02 min
 Lab File: BM010150.D
 Acq: 23 May 2017 20:05

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:244 Resp: 4148939
 Ion Ratio Lower Upper
 244 100
 212 7.5 4.9 7.3#
 122 6.8 6.2 9.4

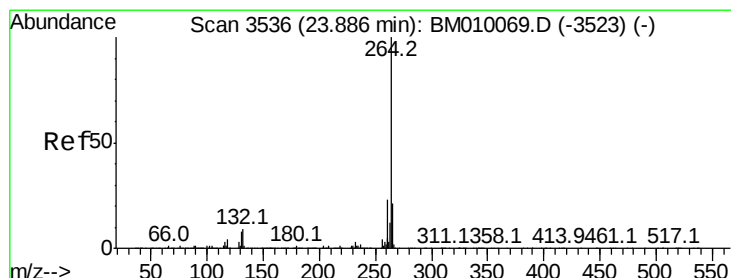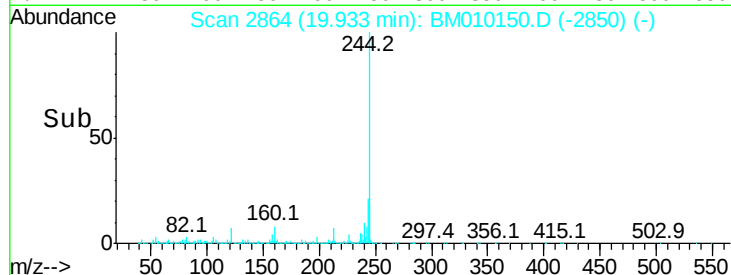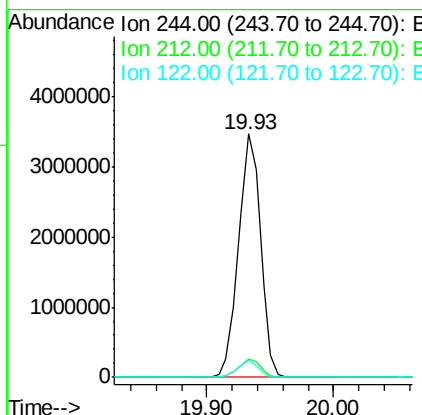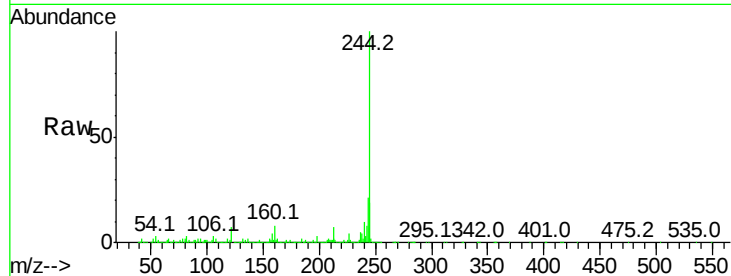

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.86 min Scan# 3531
 Delta R.T. -0.03 min
 Lab File: BM010150.D
 Acq: 23 May 2017 20:05

Tgt Ion:264 Resp: 1322571
 Ion Ratio Lower Upper
 264 100
 260 23.8 18.6 27.8
 265 22.3 17.3 25.9

