
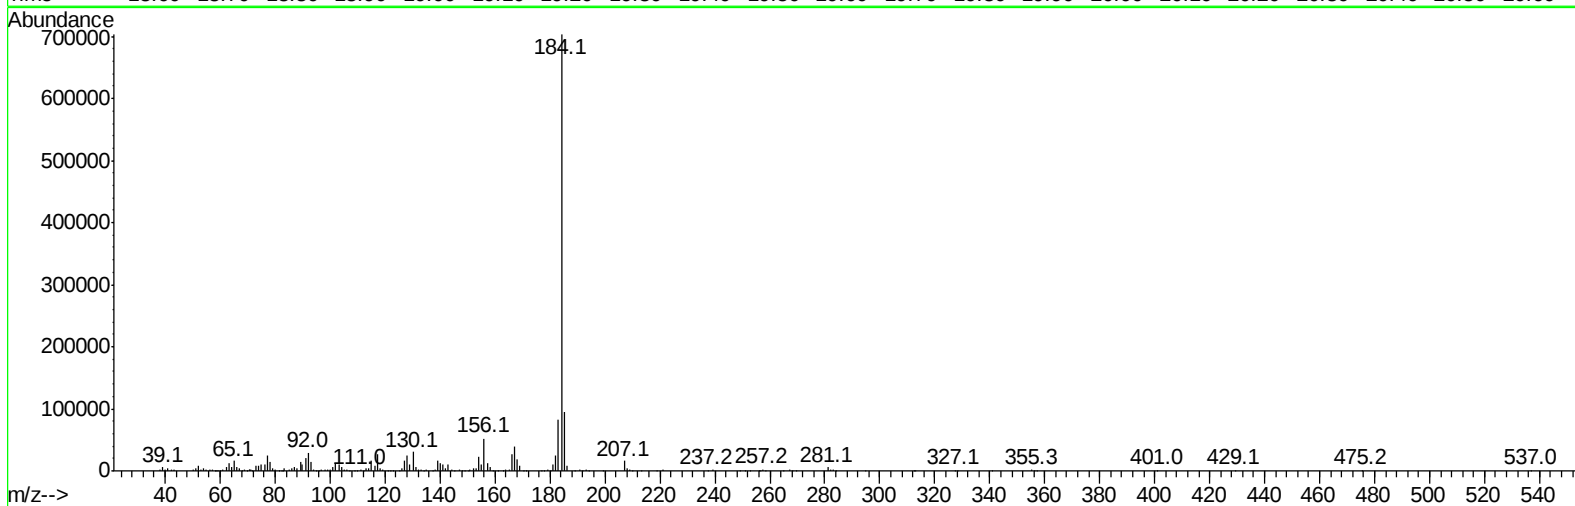


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052317\
Data File : BM010153.D
Acq On : 23 May 2017 22:22
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: May 24 06:57:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

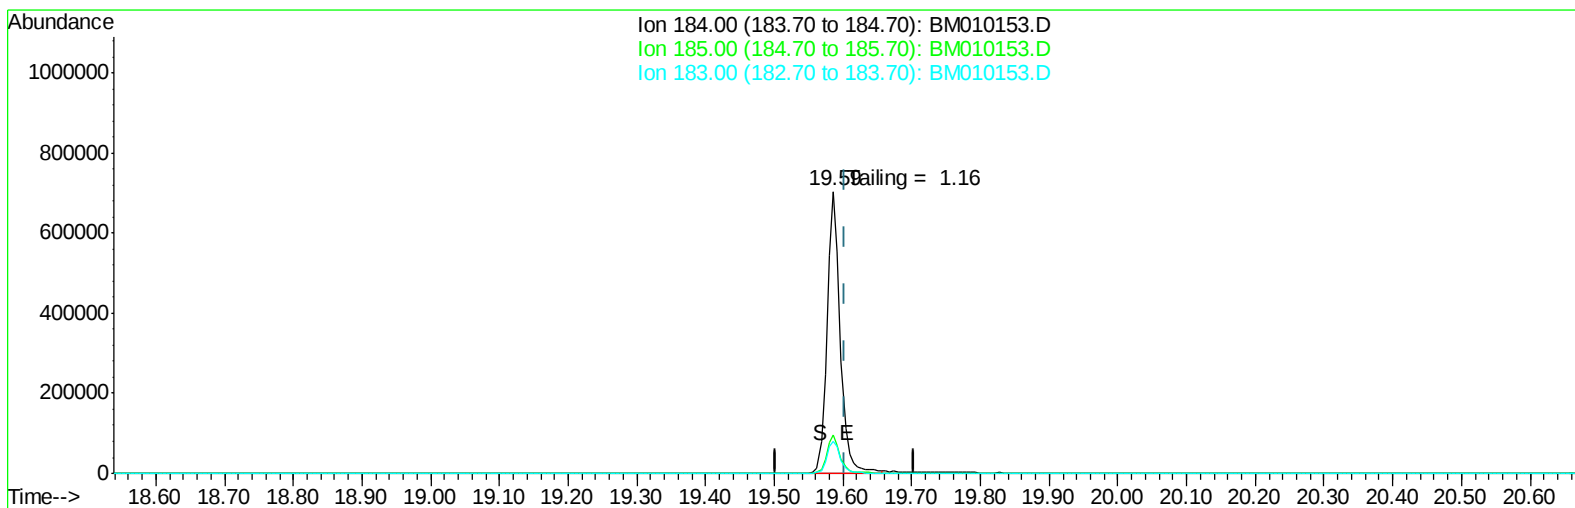

TIC: BM010153.D

(76) Benzidine



19.586min (-0.018) 33609.67ng

response 947866

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.43
183.00	11.10	11.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052317\
Data File : BM010153.D
Acq On : 23 May 2017 22:22
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: May 24 06:57:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

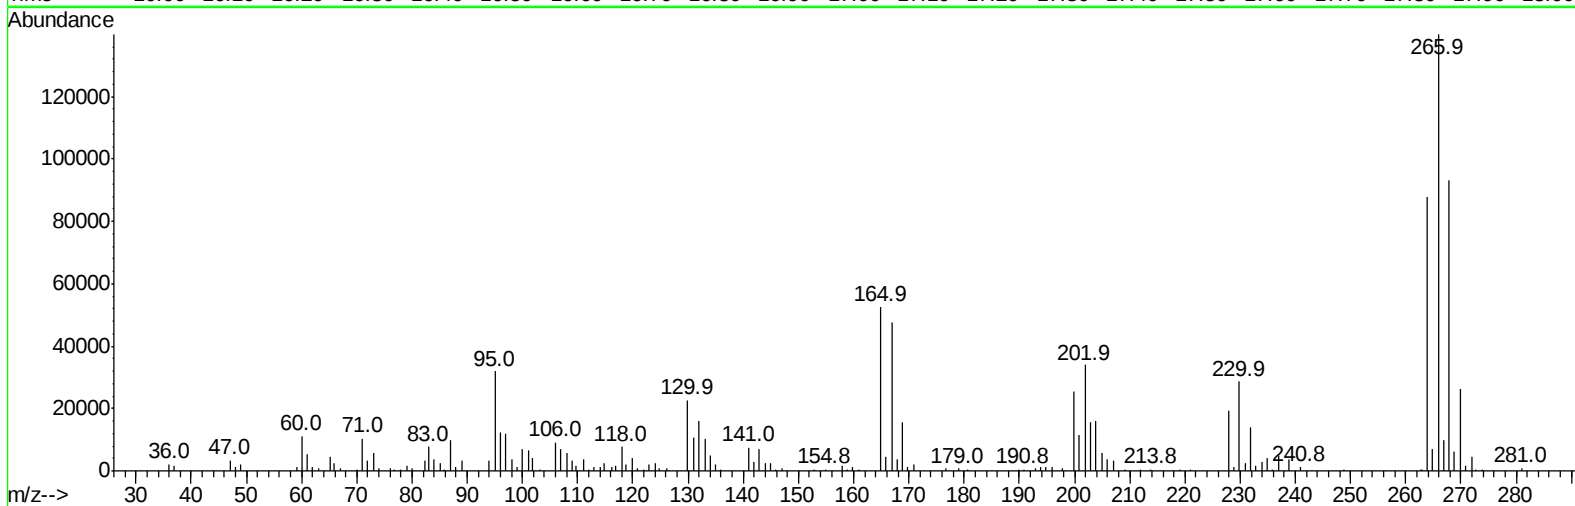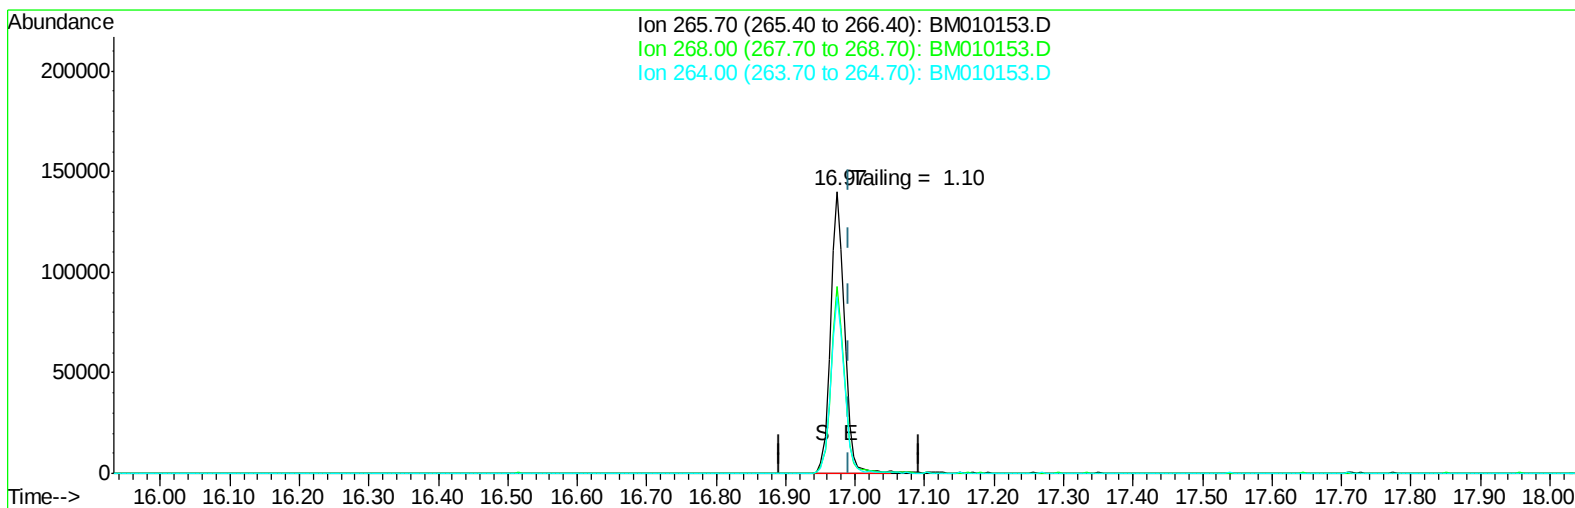

TIC: BM010153.D

(69) Pentachlorophenol (C)

16.974min (-0.018) 0.00ng

response 193553

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	66.59
264.00	61.20	62.66
0.00	0.00	0.00