


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052317\
 Data File : BM010134.D
 Acq On : 23 May 2017 10:30
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

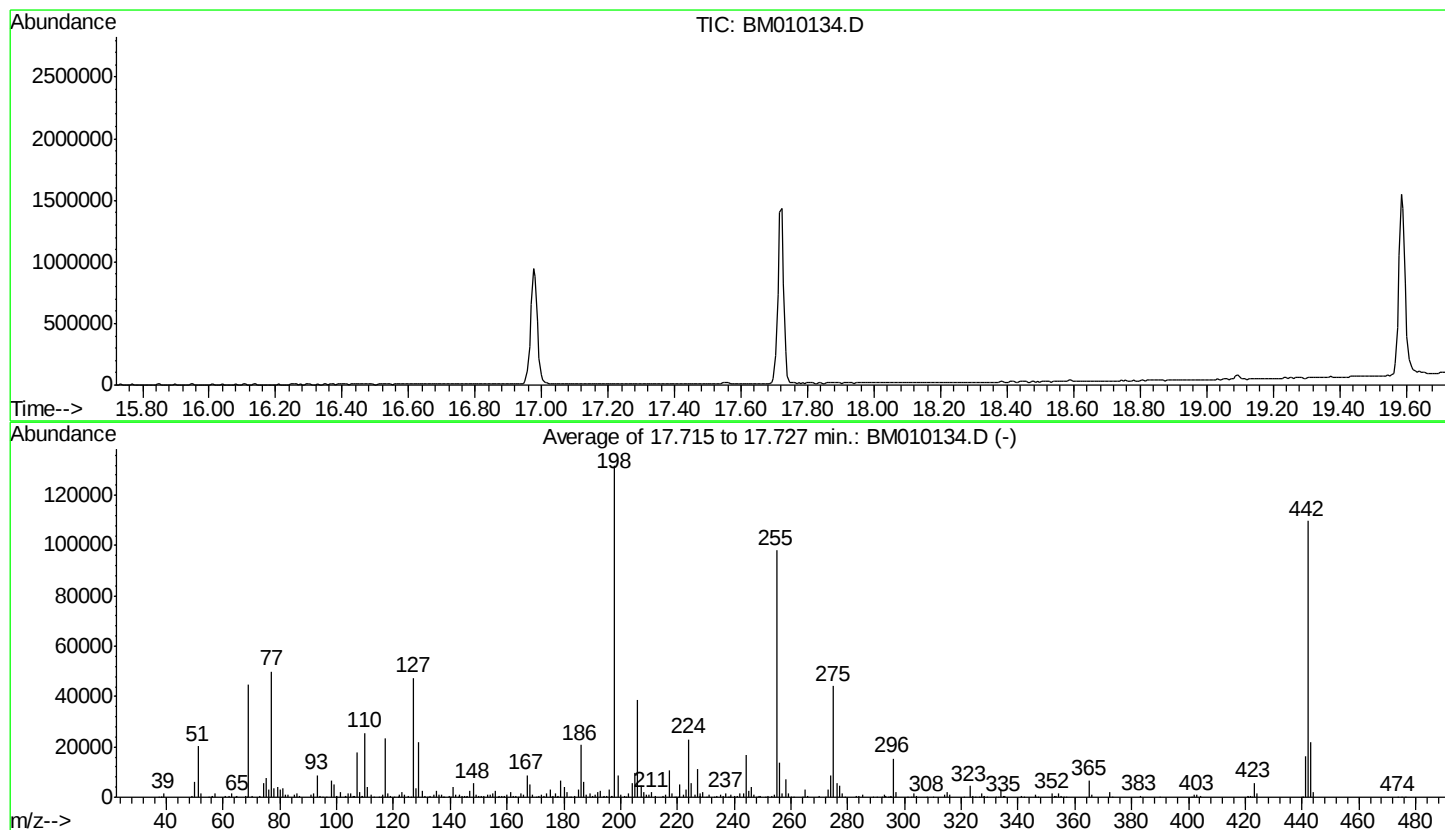

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.3	20155	PASS
68	69	0.00	2	1.3	574	PASS
69	198	0.00	100	33.9	44688	PASS
70	69	0.00	2	0.7	332	PASS
127	198	10	80	36.1	47528	PASS
197	198	0.00	2	0.5	721	PASS
198	198	100	100	100.0	131781	PASS
199	198	5	9	6.6	8650	PASS
275	198	10	60	33.5	44200	PASS
365	198	1	100	4.9	6436	PASS
441	442	0.01	24	14.7	16189	PASS
442	198	50	100	83.3	109786	PASS
443	442	15	24	19.8	21736	PASS