


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052317\
 Data File : BM010153.D
 Acq On : 23 May 2017 22:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

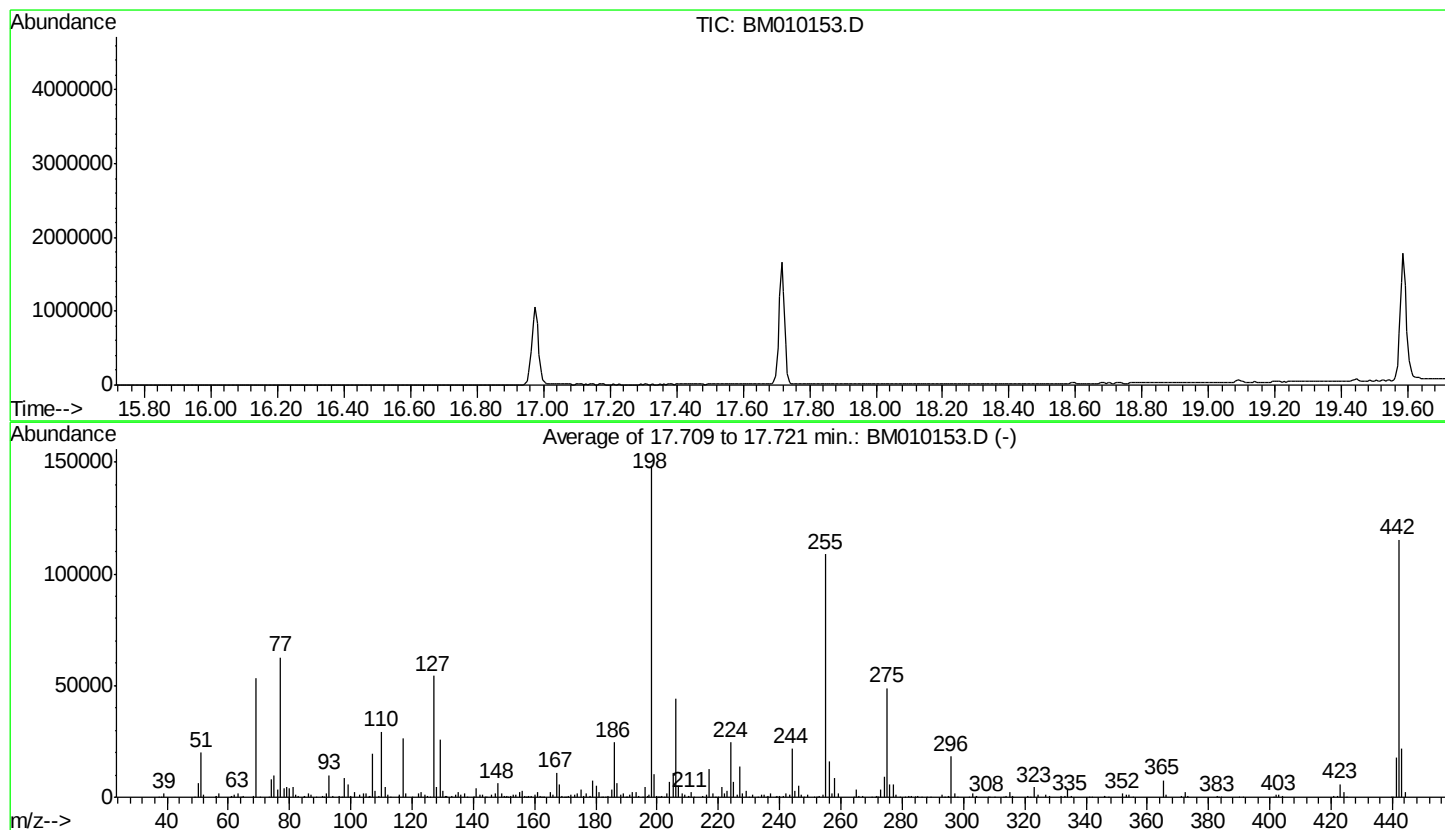

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.4	19940	PASS
68	69	0.00	2	1.6	854	PASS
69	198	0.00	100	35.8	53213	PASS
70	69	0.00	2	0.2	127	PASS
127	198	10	80	36.5	54245	PASS
197	198	0.00	2	0.8	1254	PASS
198	198	100	100	100.0	148514	PASS
199	198	5	9	7.0	10399	PASS
275	198	10	60	32.8	48760	PASS
365	198	1	100	5.0	7475	PASS
441	442	0.01	24	15.5	17829	PASS
442	198	50	100	77.6	115288	PASS
443	442	15	24	19.0	21928	PASS