
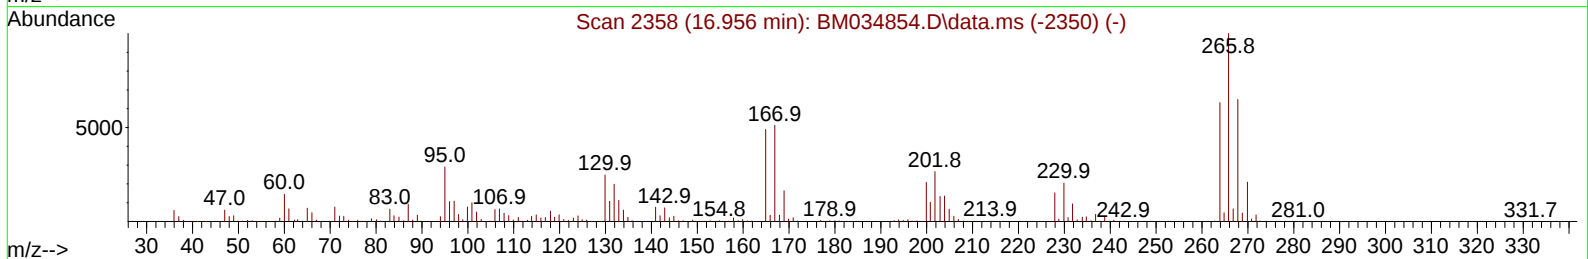
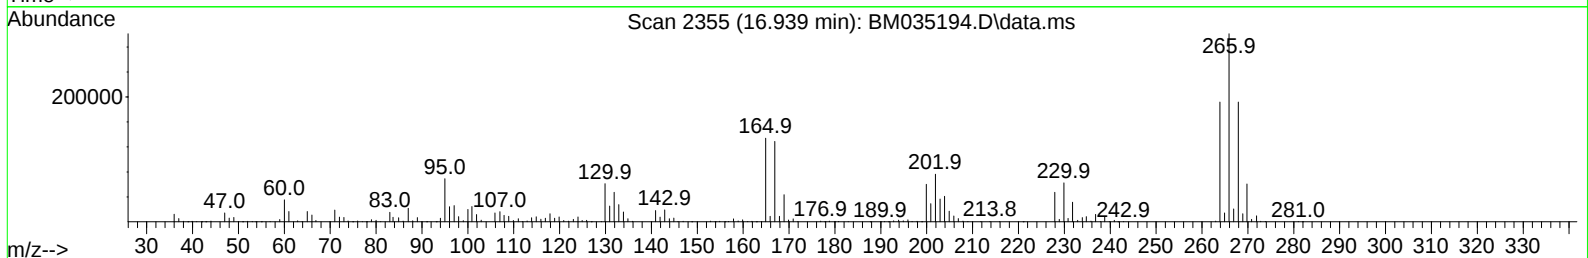


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035194.D
 Acq On : 23 May 2022 15:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 08:09:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

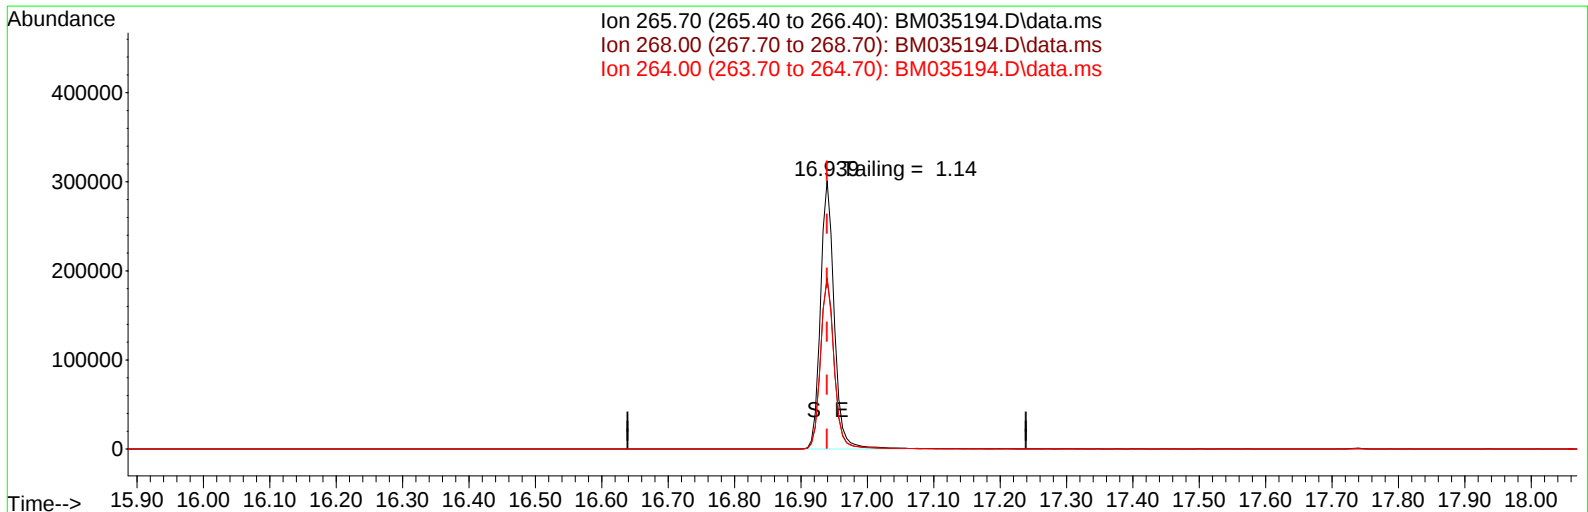

TIC: BM035194.D\data.ms

(70) Pentachlorophenol (C)




16.939min (+ 0.000) 378123.21 ng

response 435028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.68
264.00	63.30	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035194.D
Acq On : 23 May 2022 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 08:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

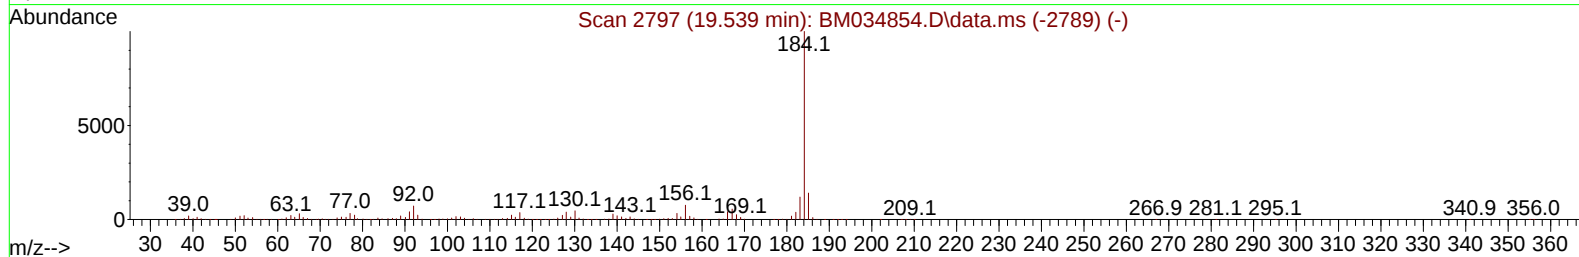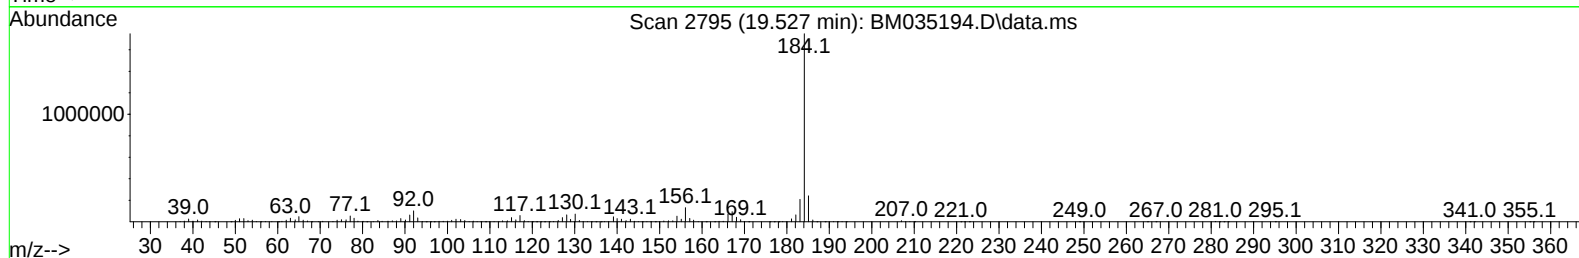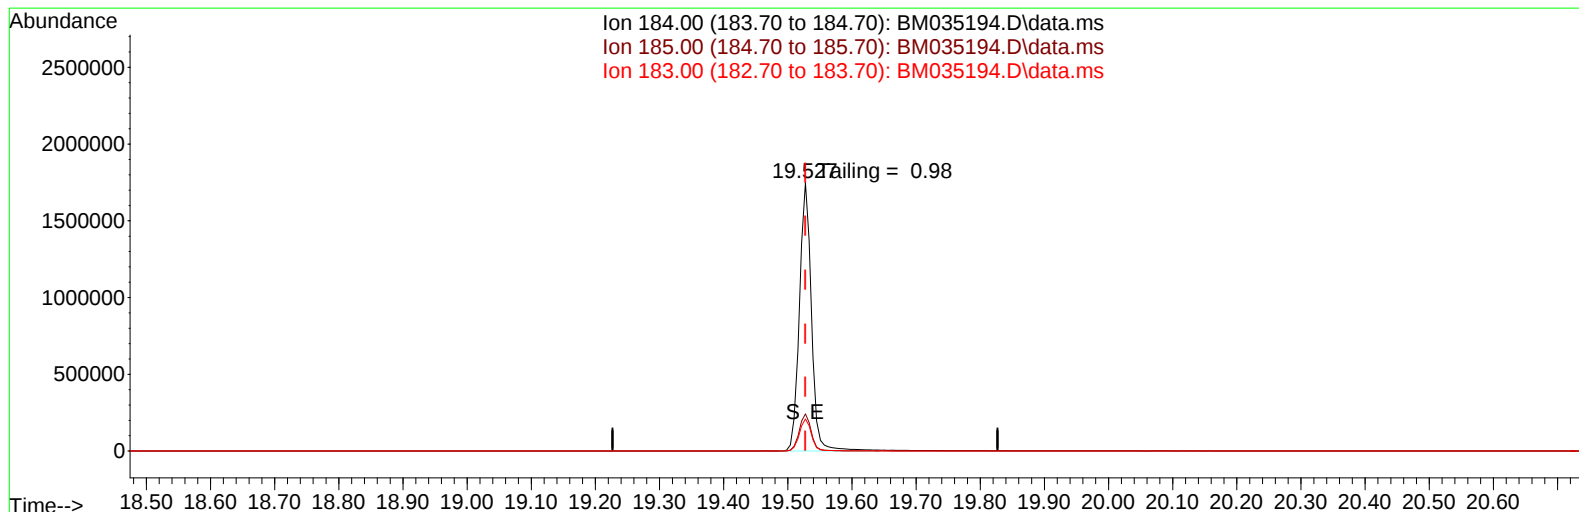

TIC: BM035194.D\data.ms

(77) Benzidine**19.527min (+ 0.000) 142627.95 ng****response 2313668**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.83
183.00	11.90	11.93
0.00	0.00	0.00