

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035206.D
 Acq On : 23 May 2022 22:25
 Operator : CG/JU
 Sample : N2979-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 NB-7-052022

Quant Time: May 24 03:18:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	161233	20.000	ng	0.00
21) Naphthalene-d8	10.704	136	594760	20.000	ng	0.00
39) Acenaphthene-d10	14.539	164	356135	20.000	ng	0.00
64) Phenanthrene-d10	17.280	188	746237	20.000	ng	0.00
76) Chrysene-d12	21.462	240	755369	20.000	ng	-0.01
86) Perylene-d12	23.844	264	810011	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	809265	88.550	ng	0.00
7) Phenol-d6	7.075	99	1006059	85.274	ng	0.00
23) Nitrobenzene-d5	9.057	82	653132	59.302	ng	0.00
42) 2,4,6-Tribromophenol	16.027	330	373888	96.511	ng	0.00
45) 2-Fluorobiphenyl	13.163	172	1370105	55.848	ng	0.00
79) Terphenyl-d14	19.903	244	2033091	52.113	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035206.D
Acq On : 23 May 2022 22:25
Operator : CG/JU
Sample : N2979-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NB-7-052022

Quant Time: May 24 03:18:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration




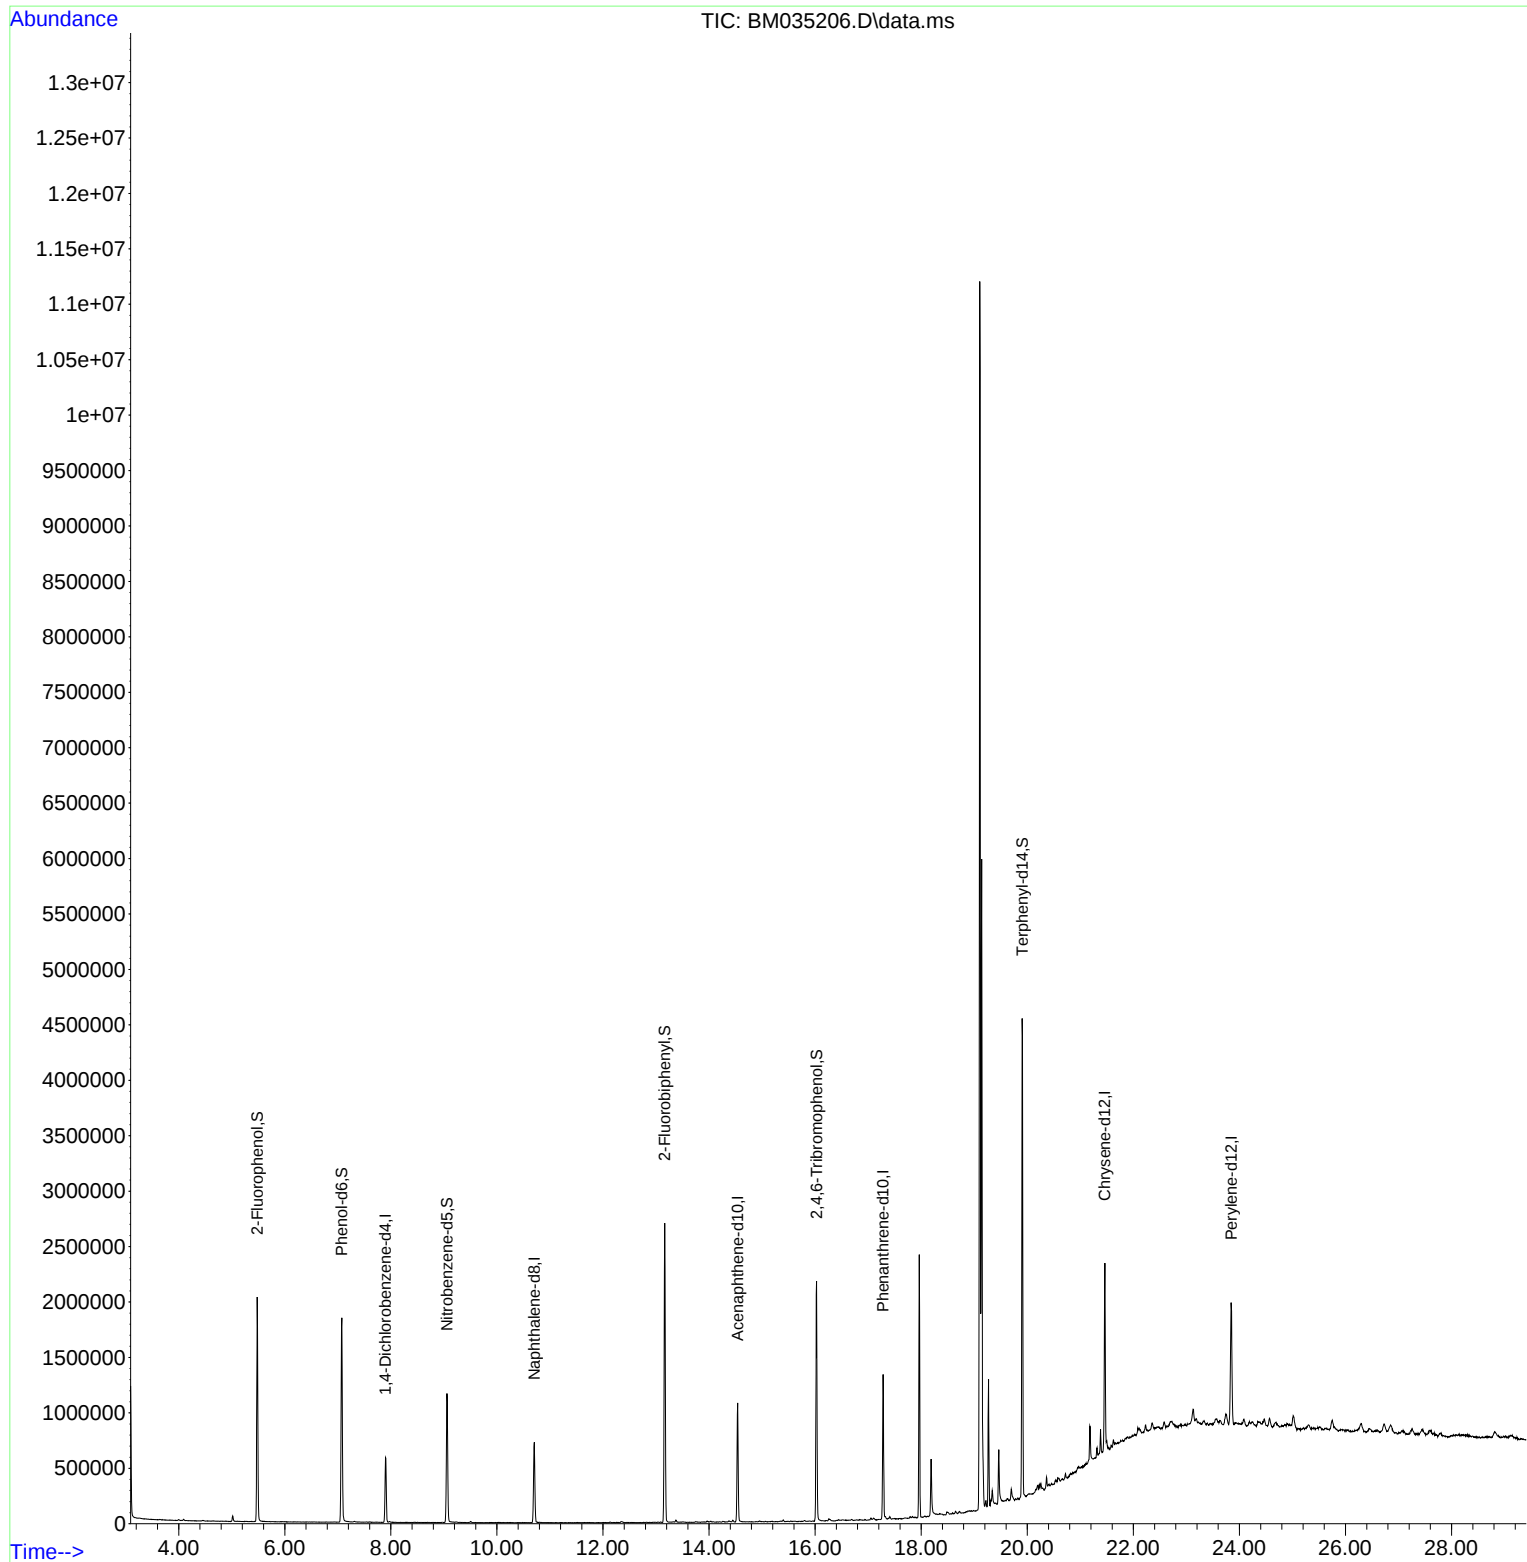




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.898 min Scan# 81
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25




Instrument :
BNA_M
ClientSampleId :
NB-7-052022

Tgt Ion:152 Resp: 161233
Ion Ratio Lower Upper
152 100
150 156.6 124.9 187.3
115 59.9 47.9 71.9

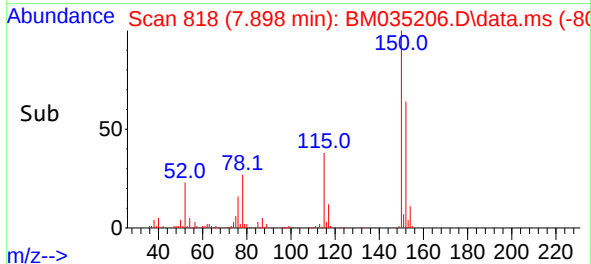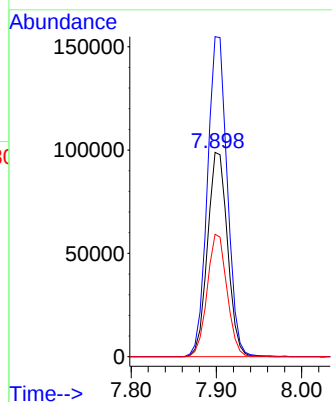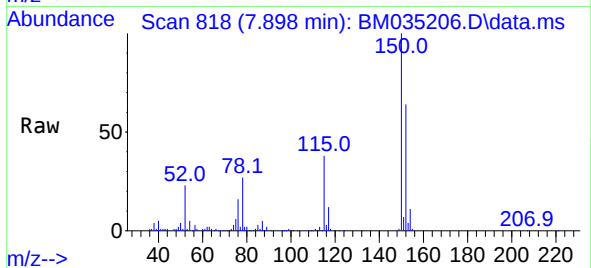

#5
2-Fluorophenol
Concen: 88.550 ng
RT: 5.481 min Scan# 407
Delta R.T. -0.000 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25

Tgt Ion:112 Resp: 809265
Ion Ratio Lower Upper
112 100
64 59.2 47.8 71.6
63 32.7 26.6 40.0


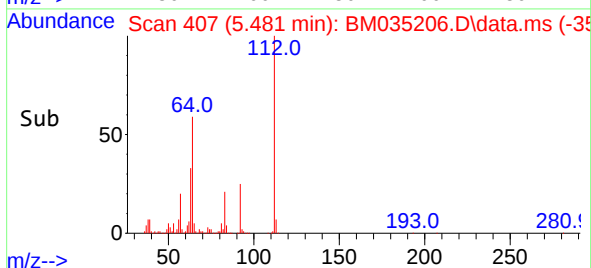
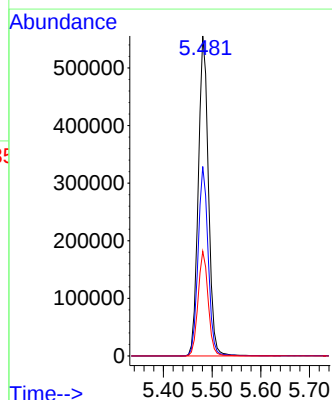
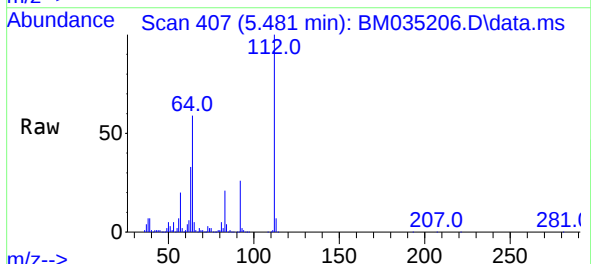




#7
Phenol-d6
Concen: 85.274 ng
RT: 7.075 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25




Instrument :
BNA_M
ClientSampleId :
NB-7-052022

Tgt Ion: 99 Resp: 1006059
Ion Ratio Lower Upper
99 100
42 21.7 18.8 28.2
71 37.2 30.2 45.2

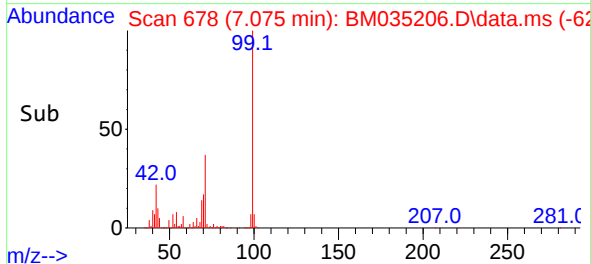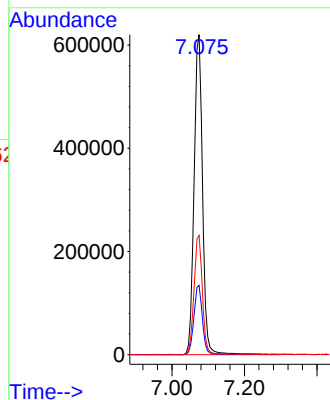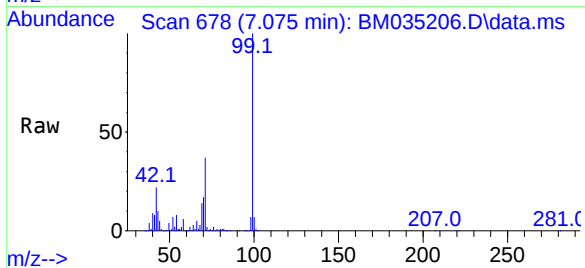

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.704 min Scan# 1295
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25

Tgt Ion: 136 Resp: 594760
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 7.5 7.0 10.4
68 5.2 4.3 6.5


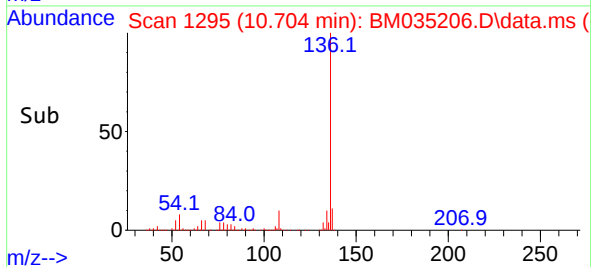
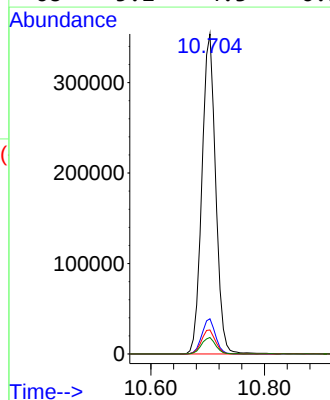
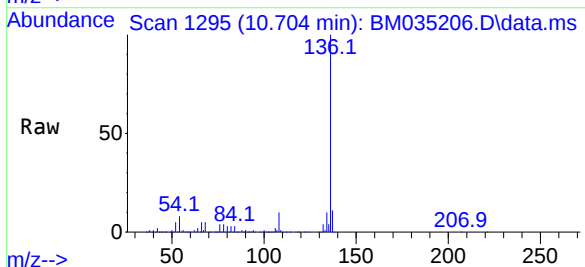




#23
Nitrobenzene-d5
Concen: 59.302 ng
RT: 9.057 min Scan# 1015
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25




Instrument :
BNA_M
ClientSampleId :
NB-7-052022


Tgt Ion: 82 Resp: 653132
Ion Ratio Lower Upper
82 100
128 42.0 33.7 50.5
54 52.8 43.2 64.8

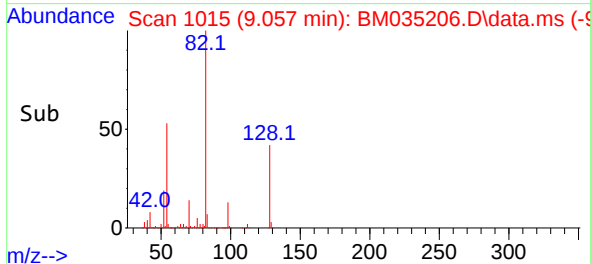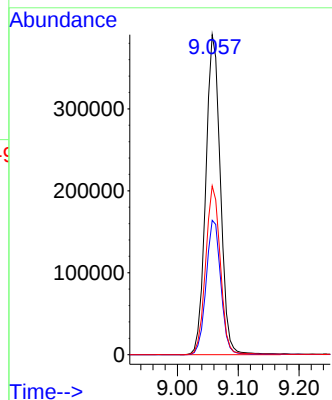

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.539 min Scan# 1947
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25


Tgt Ion:164 Resp: 356135
Ion Ratio Lower Upper
164 100
162 104.8 83.0 124.6
160 45.2 37.0 55.4

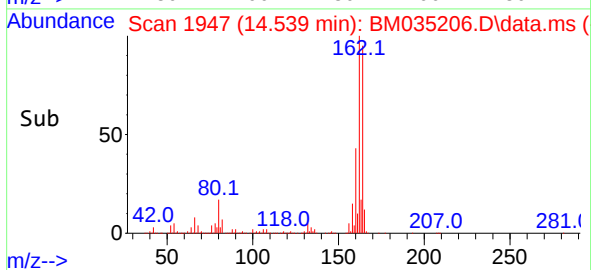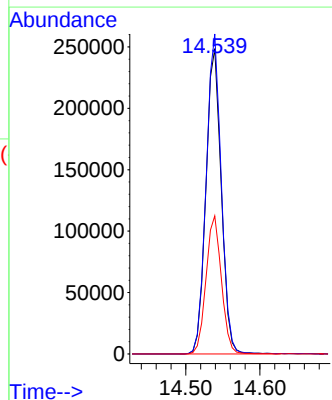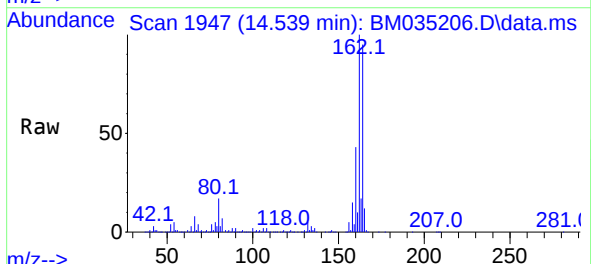






#42
2,4,6-Tribromophenol
Concen: 96.511 ng
RT: 16.027 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25


Instrument :
BNA_M
ClientSampleId :
NB-7-052022

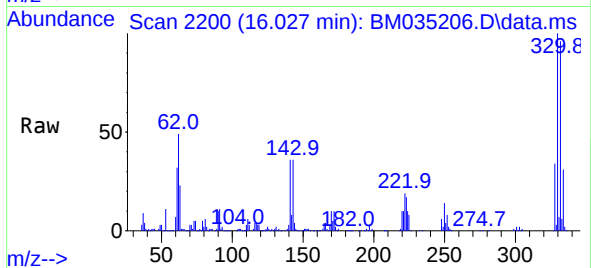



Tgt Ion:330 Resp: 373888
Ion Ratio Lower Upper
330 100
332 96.8 77.0 115.4
141 38.5 35.3 52.9

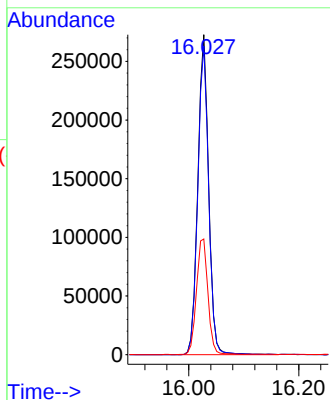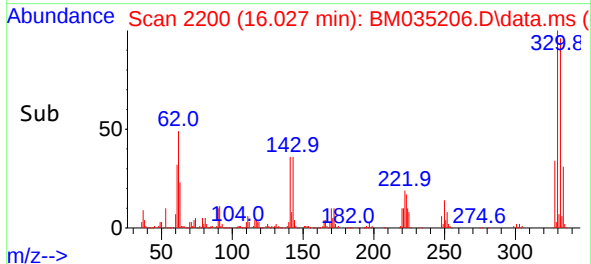


#45
2-Fluorobiphenyl
Concen: 55.848 ng
RT: 13.163 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25

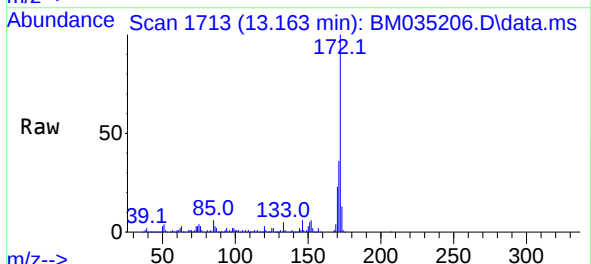

Tgt Ion:172 Resp: 1370105
Ion Ratio Lower Upper
172 100
171 35.6 28.5 42.7
170 23.4 18.7 28.1



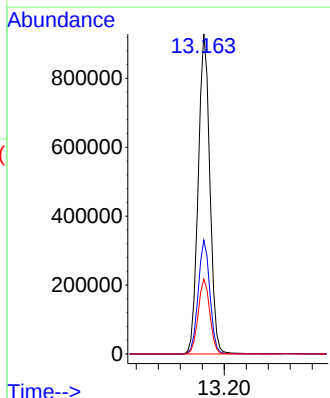
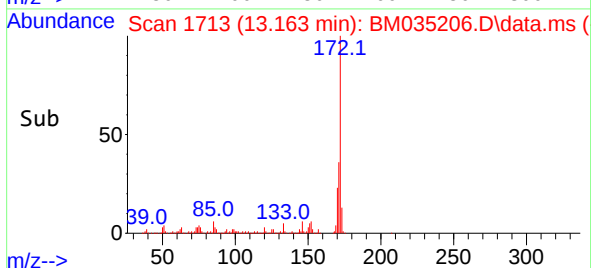




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.280 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25




Instrument :
BNA_M
ClientSampleId :
NB-7-052022


Tgt Ion:188 Resp: 746237
Ion Ratio Lower Upper
188 100
94 7.8 7.0 10.4
80 8.7 7.6 11.4

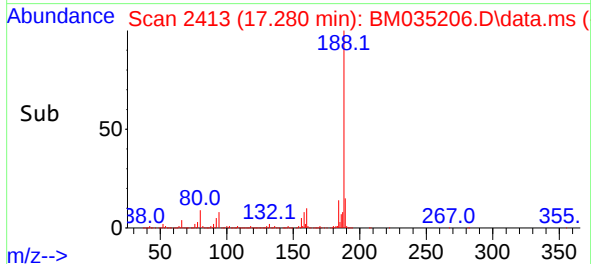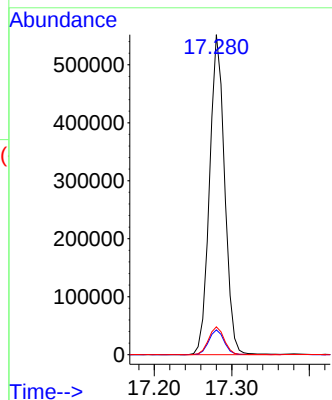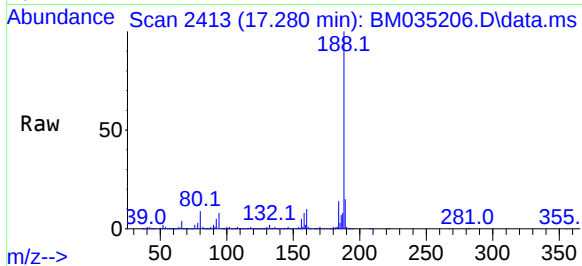

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.462 min Scan# 3124
Delta R.T. -0.012 min
Lab File: BM035206.D
Acq: 23 May 2022 22:25

Tgt Ion:240 Resp: 755369
Ion Ratio Lower Upper
240 100
120 10.1 9.4 14.0
236 25.6 20.6 30.8


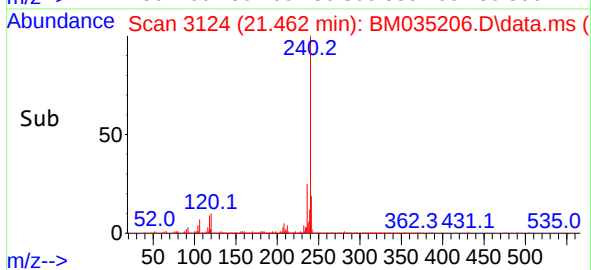
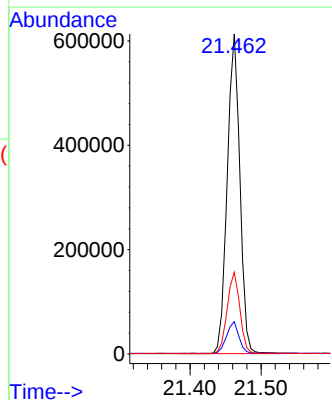
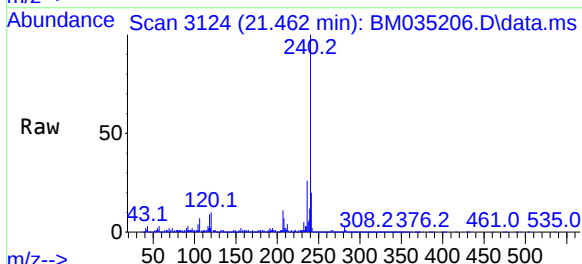




#79
 Terphenyl-d14
 Concen: 52.113 ng
 RT: 19.903 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BM035206.D
 Acq: 23 May 2022 22:25

Instrument :
 BNA_M
 ClientSampleId :
 NB-7-052022

Tgt Ion:244 Resp: 2033091
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.2 9.4
 122 9.8 8.3 12.5

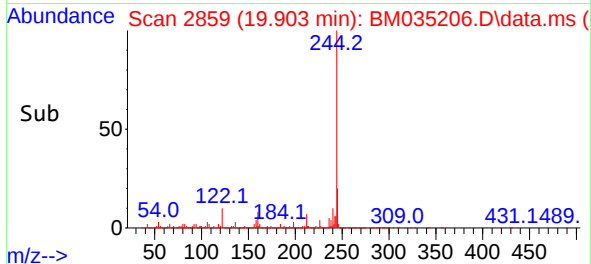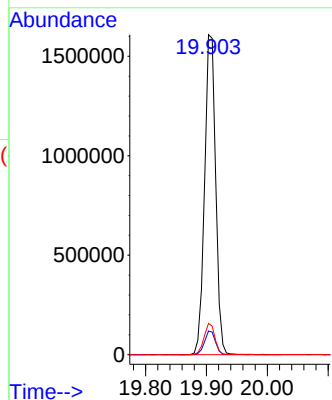

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.844 min Scan# 3529
 Delta R.T. -0.012 min
 Lab File: BM035206.D
 Acq: 23 May 2022 22:25

Tgt Ion:264 Resp: 810011
 Ion Ratio Lower Upper
 264 100
 260 23.5 18.9 28.3
 265 22.4 17.5 26.3

