

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035192.D
 Acq On : 23 May 2022 13:48
 Operator : CG/JU
 Sample : PB144968BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB144968BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	400	407	421	rBV	3357041	4862354	40.67%	9.594%
2	7.075	670	678	693	rBV	3156657	5073649	42.44%	10.011%
3	7.904	812	819	828	rBV	638782	1007307	8.43%	1.988%
4	9.063	1008	1016	1026	rBV	1997753	3283562	27.46%	6.479%
5	10.704	1288	1295	1307	rBV	826883	1412328	11.81%	2.787%
6	13.168	1706	1714	1729	rBV	5732881	8171324	68.35%	16.123%
7	14.539	1940	1947	1961	rBV	1337907	1991092	16.65%	3.929%
8	16.027	2193	2200	2218	rBV	4195293	6134582	51.31%	12.104%
9	17.286	2407	2414	2424	rBV	1605962	2322408	19.43%	4.582%
10	19.909	2854	2860	2870	rBV	9577905	11955528	100.00%	23.589%
11	21.468	3120	3125	3132	rBV	1828664	2367058	19.80%	4.670%
12	23.850	3524	3530	3541	rVB2	1039535	2100657	17.57%	4.145%




Sum of corrected areas: 50681849

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035192.D
Acq On : 23 May 2022 13:48
Operator : CG/JU
Sample : PB144968BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144968BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

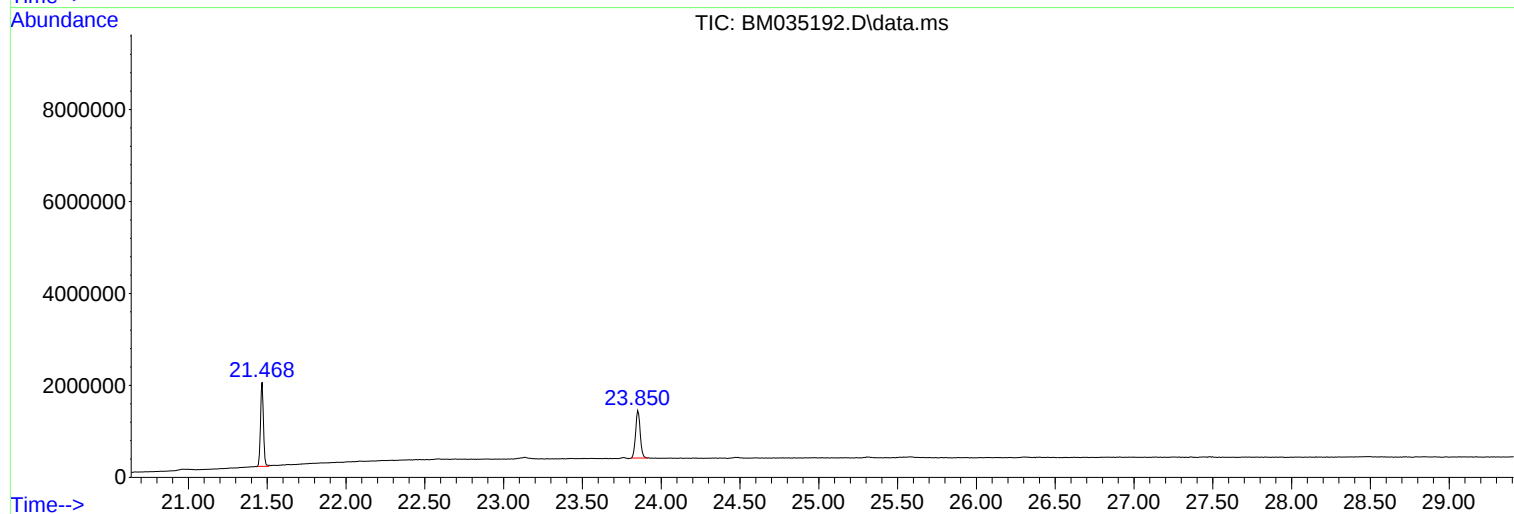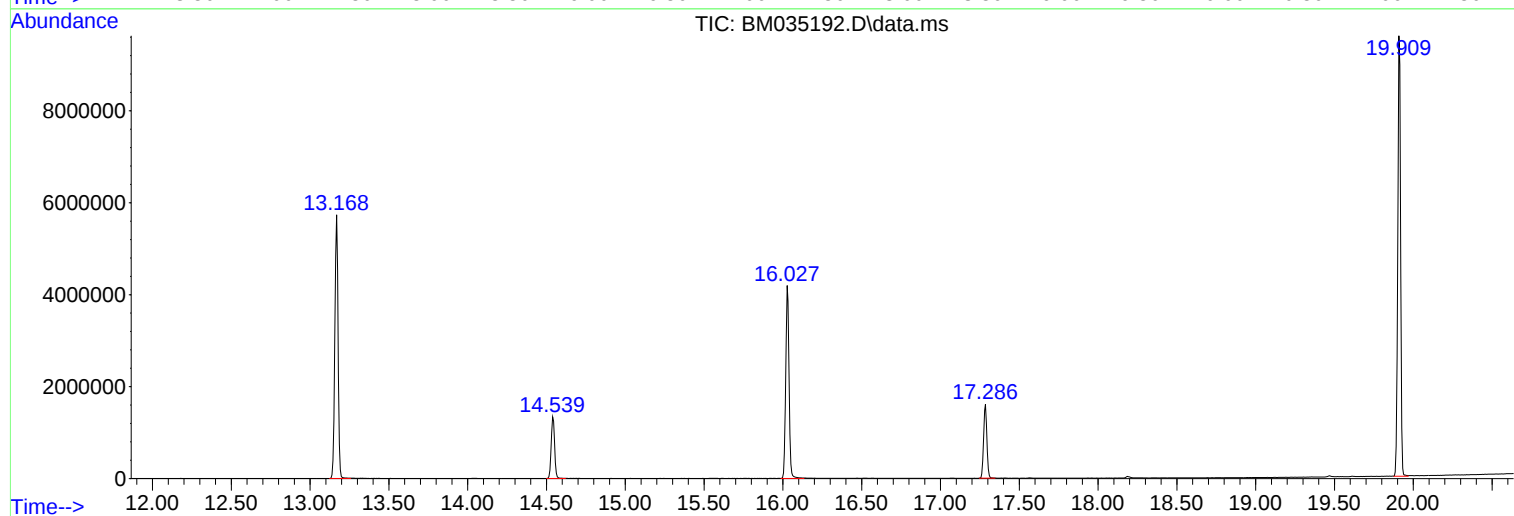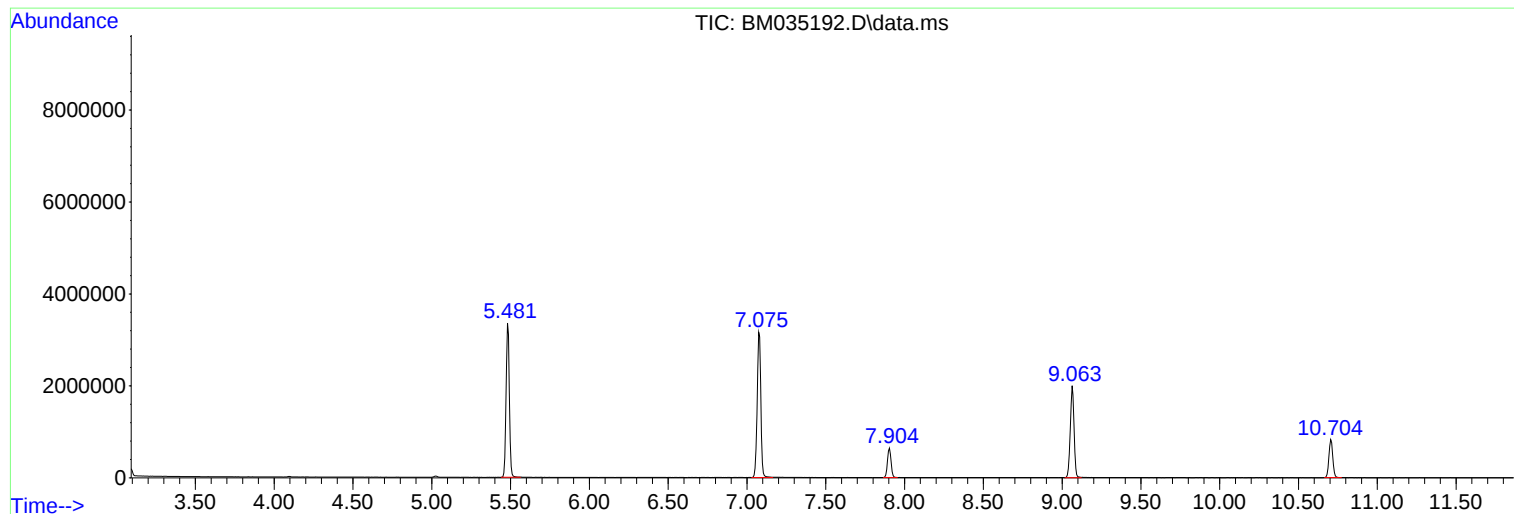

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035192.D
Acq On : 23 May 2022 13:48
Operator : CG/JU
Sample : PB144968BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144968BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035192.D
Acq On : 23 May 2022 13:48
Operator : CG/JU
Sample : PB144968BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144968BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------