

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035196.D
 Acq On : 23 May 2022 16:17
 Operator : CG/JU
 Sample : PB144970BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB144970BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	400	407	420	rBV	3217688	4571563	48.62%	10.333%
2	7.075	669	678	695	rBV	2958730	4747430	50.49%	10.731%
3	7.904	812	819	829	rBV	588255	947964	10.08%	2.143%
4	9.063	1008	1016	1032	rBV	1864219	3074555	32.70%	6.949%
5	10.704	1287	1295	1306	rBV	787381	1313927	13.97%	2.970%
6	13.169	1706	1714	1730	rBV	5065783	7491882	79.67%	16.934%
7	14.539	1940	1947	1961	rBV	1209851	1803162	19.18%	4.076%
8	16.027	2193	2200	2221	rBV	3672645	5390332	57.32%	12.184%
9	17.286	2407	2414	2426	rBV	1379762	2027851	21.56%	4.584%
10	19.909	2854	2860	2870	rBV	7881850	9403575	100.00%	21.255%
11	21.462	3120	3124	3136	rBV	1359362	1811916	19.27%	4.096%
12	23.850	3524	3530	3540	rVB2	811623	1657312	17.62%	3.746%




Sum of corrected areas: 44241469

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035196.D
Acq On : 23 May 2022 16:17
Operator : CG/JU
Sample : PB144970BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144970BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

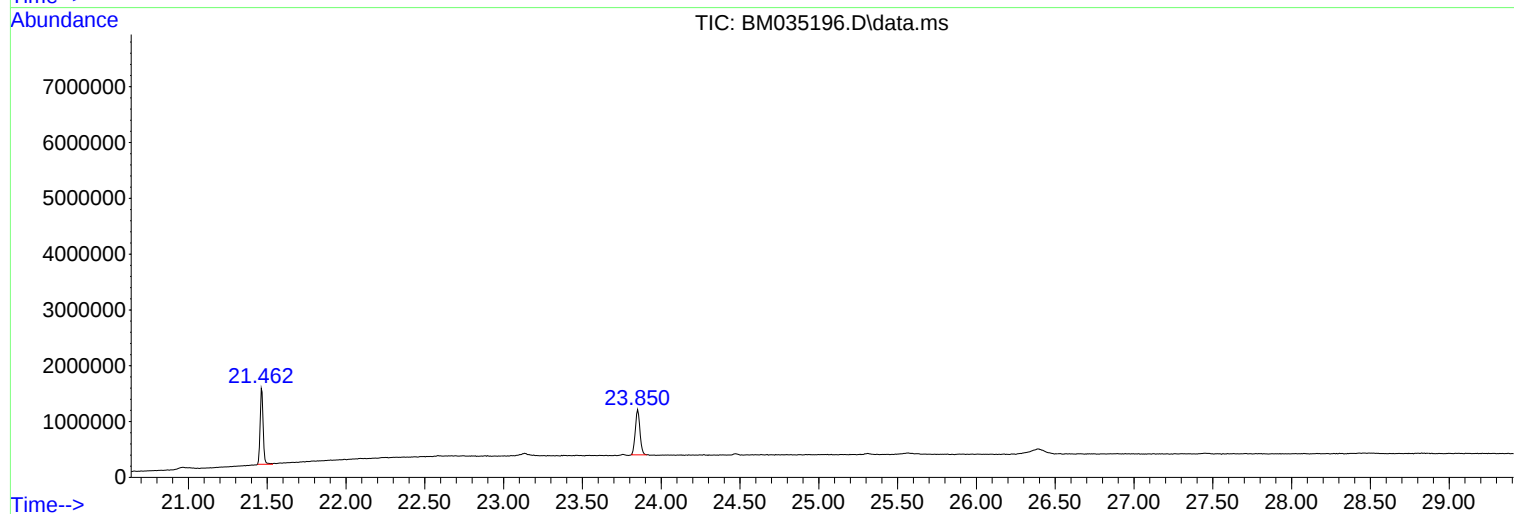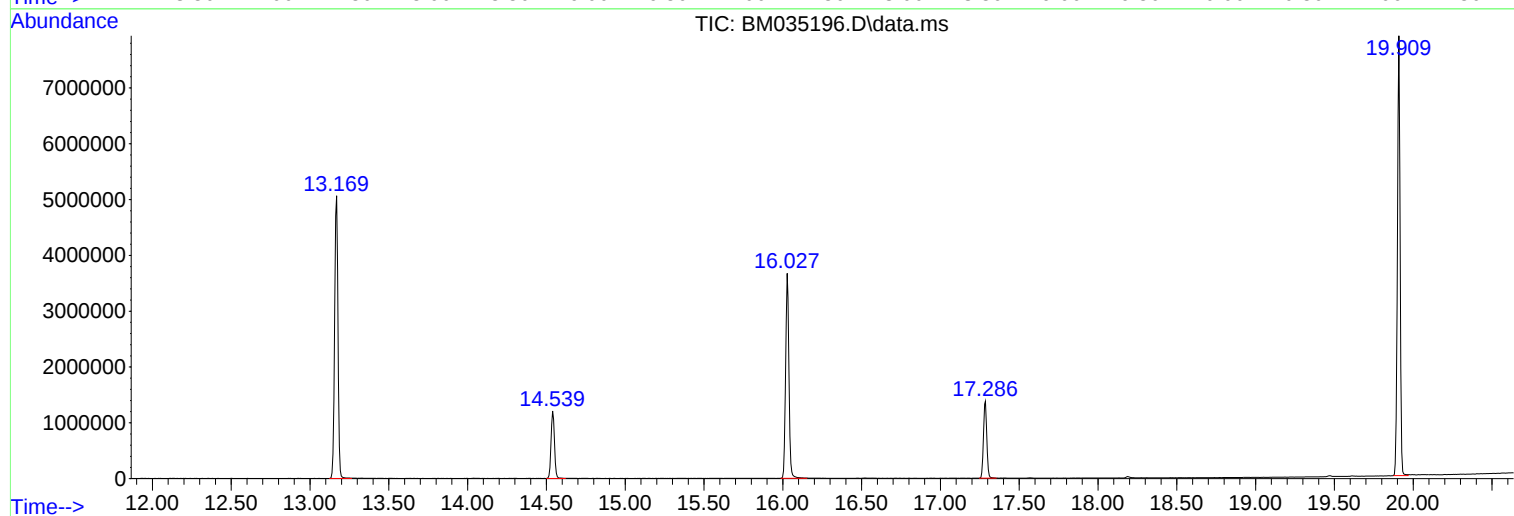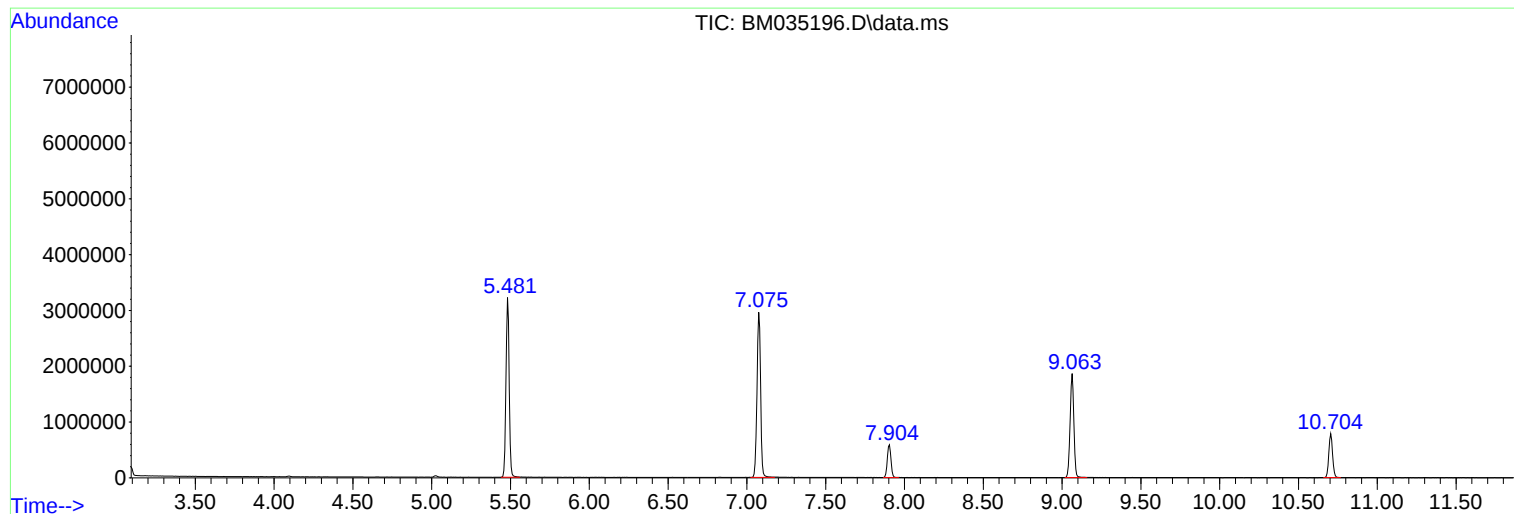

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035196.D
Acq On : 23 May 2022 16:17
Operator : CG/JU
Sample : PB144970BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144970BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035196.D
Acq On : 23 May 2022 16:17
Operator : CG/JU
Sample : PB144970BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144970BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------