

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035206.D
 Acq On : 23 May 2022 22:25
 Operator : CG/JU
 Sample : N2979-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 NB-7-052022

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	401	407	423	rBV	2025312	2940001	22.09%	5.108%
2	7.075	670	678	697	rBV	1844027	3016389	22.66%	5.241%
3	7.898	810	818	827	rBV	585385	955895	7.18%	1.661%
4	9.057	1007	1015	1028	rBV	1163016	1952977	14.67%	3.393%
5	10.704	1287	1295	1304	rBV	724910	1227622	9.22%	2.133%
6	13.163	1706	1713	1725	rBV	2700944	3994737	30.02%	6.941%
7	14.539	1940	1947	1961	rBV	1072668	1572454	11.82%	2.732%
8	16.027	2193	2200	2212	rBV	2167948	3134284	23.55%	5.446%
9	17.280	2407	2413	2419	rBV	1306395	1791094	13.46%	3.112%
10	17.962	2524	2529	2535	rBV	2372579	2736066	20.56%	4.754%
11	18.186	2562	2567	2581	rBV	512732	777382	5.84%	1.351%
12	19.103	2718	2723	2726	rBV	11069798	13308736	100.00%	23.123%
13	19.139	2726	2729	2739	rVB2	5844601	7546196	56.70%	13.111%
14	19.268	2747	2751	2756	rBV	1145235	1208847	9.08%	2.100%
15	19.339	2760	2763	2771	rVB	120504	182199	1.37%	0.317%
16	19.462	2780	2784	2794	rBV	489090	711271	5.34%	1.236%
17	19.698	2821	2824	2835	rVB2	103823	192843	1.45%	0.335%
18	19.903	2854	2859	2865	rBV	4316971	5401788	40.59%	9.385%
19	21.180	3073	3076	3087	rBV	303058	397010	2.98%	0.690%
20	21.380	3108	3110	3115	rVB	208356	197595	1.48%	0.343%
21	21.462	3119	3124	3128	rBV	1675350	2136835	16.06%	3.713%
22	23.844	3524	3529	3537	rVB2	1098718	2174624	16.34%	3.778%




Sum of corrected areas: 57556845

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035206.D
Acq On : 23 May 2022 22:25
Operator : CG/JU
Sample : N2979-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NB-7-052022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

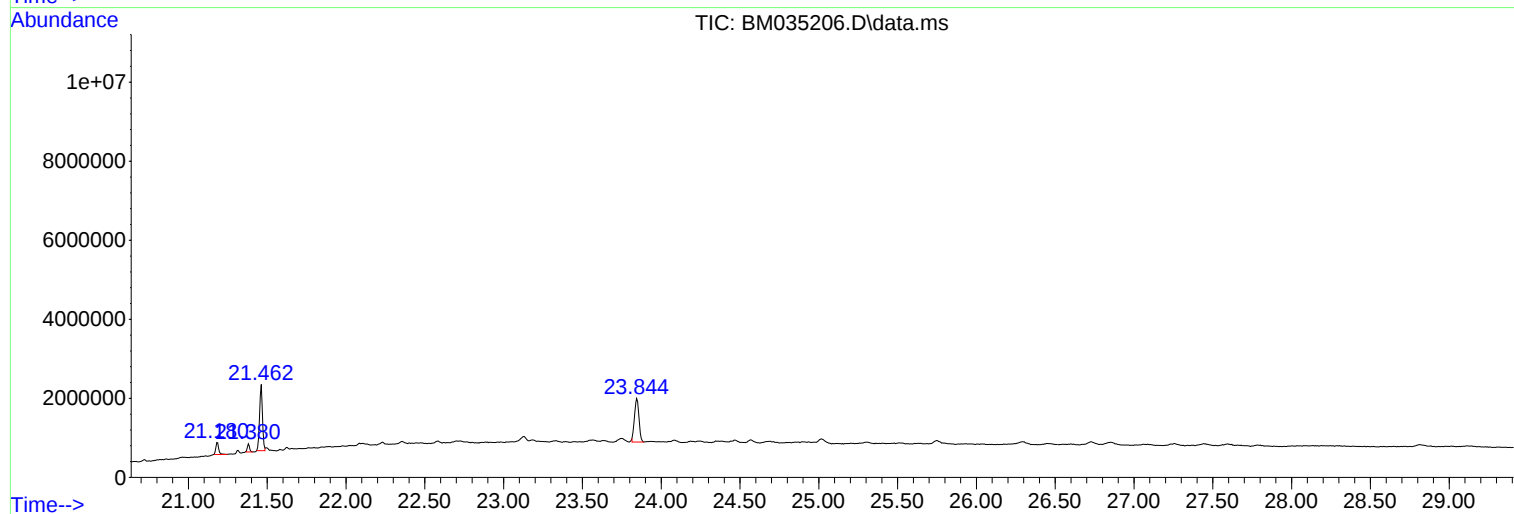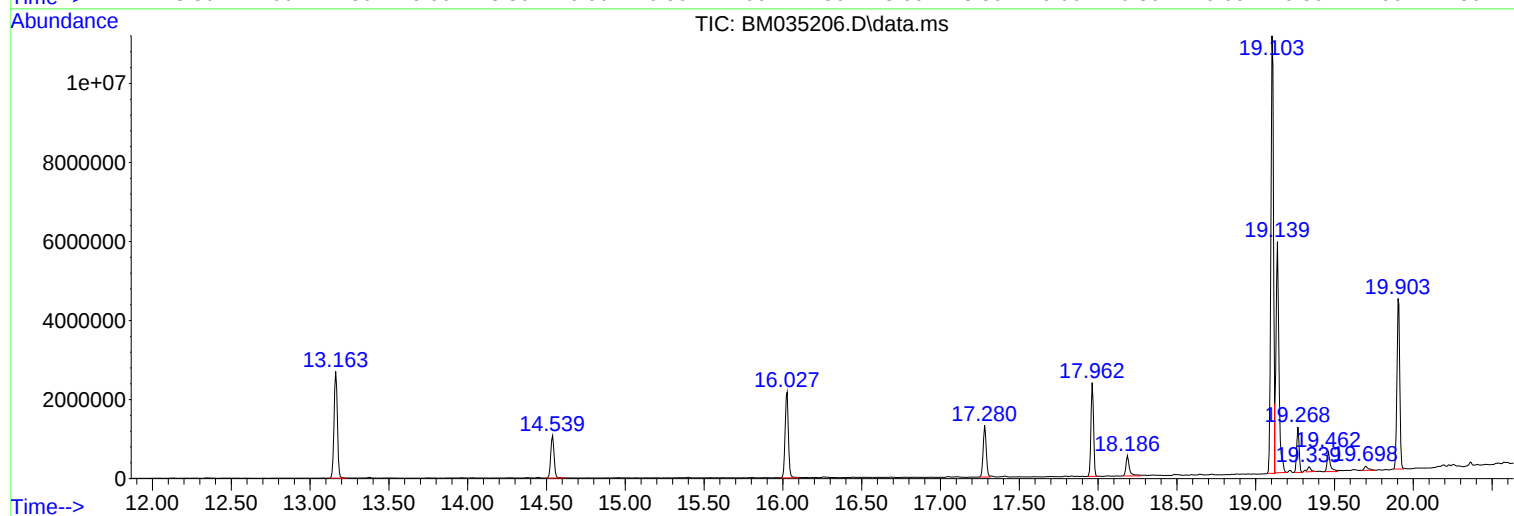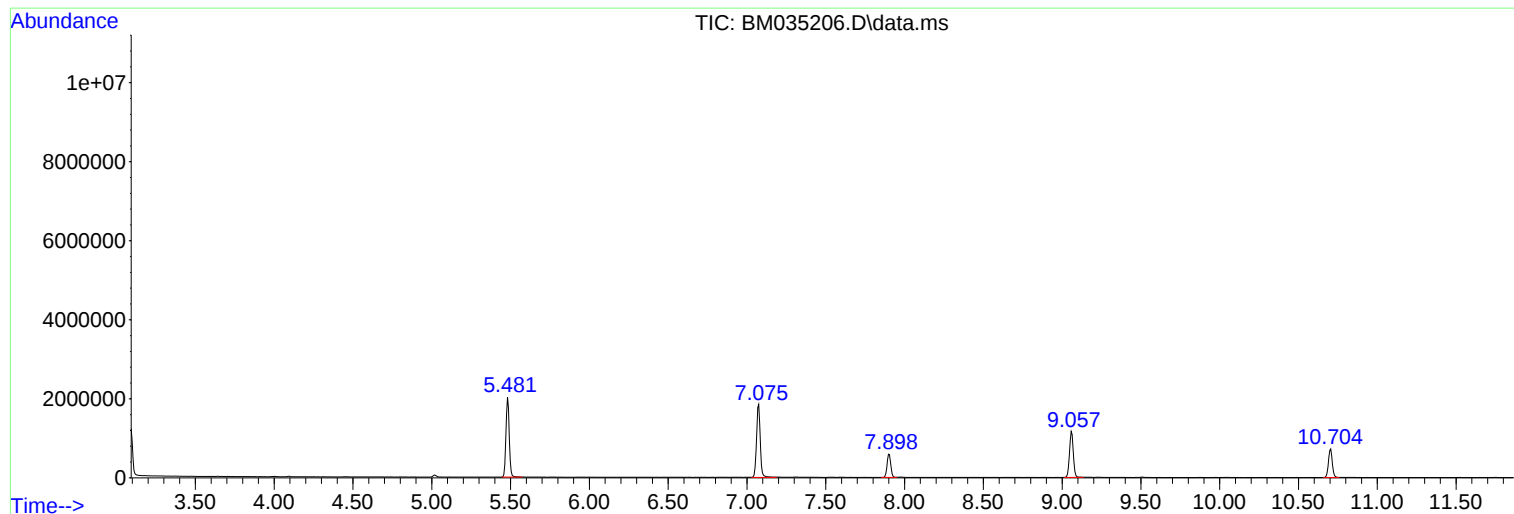

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035206.D
Acq On : 23 May 2022 22:25
Operator : CG/JU
Sample : N2979-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NB-7-052022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035206.D
Acq On : 23 May 2022 22:25
Operator : CG/JU
Sample : N2979-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NB-7-052022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------