

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035207.D
 Acq On : 23 May 2022 23:02
 Operator : CG/JU
 Sample : N2874-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P007-SS002-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	400	407	421	rBV	2467003	3611176	46.87%	9.314%
2	7.075	670	678	691	rBV	2380529	3723669	48.33%	9.604%
3	7.899	811	818	828	rBV	569490	925985	12.02%	2.388%
4	9.057	1007	1015	1030	rBV	1441554	2480044	32.19%	6.397%
5	10.487	1250	1258	1274	rBV	150862	295133	3.83%	0.761%
6	10.704	1287	1295	1305	rBV	719308	1220348	15.84%	3.148%
7	13.163	1706	1713	1729	rBV	3812735	5497893	71.36%	14.180%
8	14.539	1940	1947	1957	rBV	1042958	1543954	20.04%	3.982%
9	16.027	2193	2200	2214	rBV	2777525	4038128	52.41%	10.415%
10	17.280	2407	2413	2420	rBV	1239630	1765235	22.91%	4.553%
11	18.186	2562	2567	2579	rBV	510096	758727	9.85%	1.957%
12	19.462	2780	2784	2797	rBV	391202	602852	7.82%	1.555%
13	19.910	2854	2860	2865	rBV	6203989	7704843	100.00%	19.873%
14	21.186	3073	3077	3082	rBV	327261	438480	5.69%	1.131%
15	21.462	3120	3124	3134	rVB	1574343	1980918	25.71%	5.109%
16	23.845	3524	3529	3539	rVB2	1084123	2183425	28.34%	5.632%




Sum of corrected areas: 38770810

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035207.D
Acq On : 23 May 2022 23:02
Operator : CG/JU
Sample : N2874-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

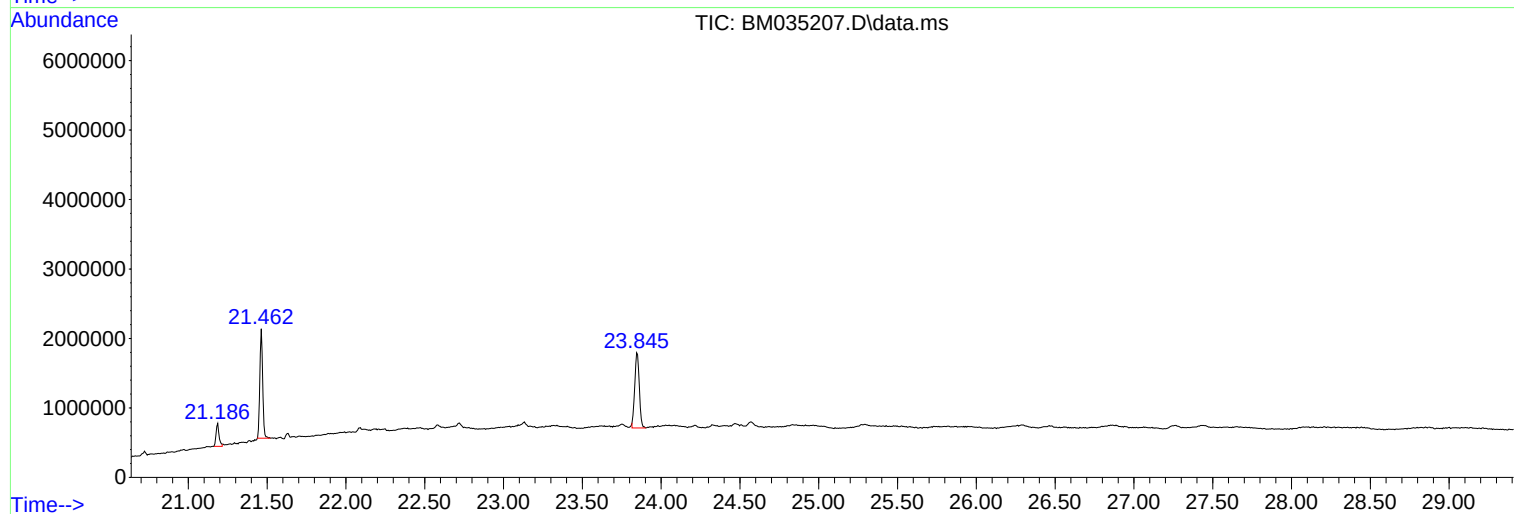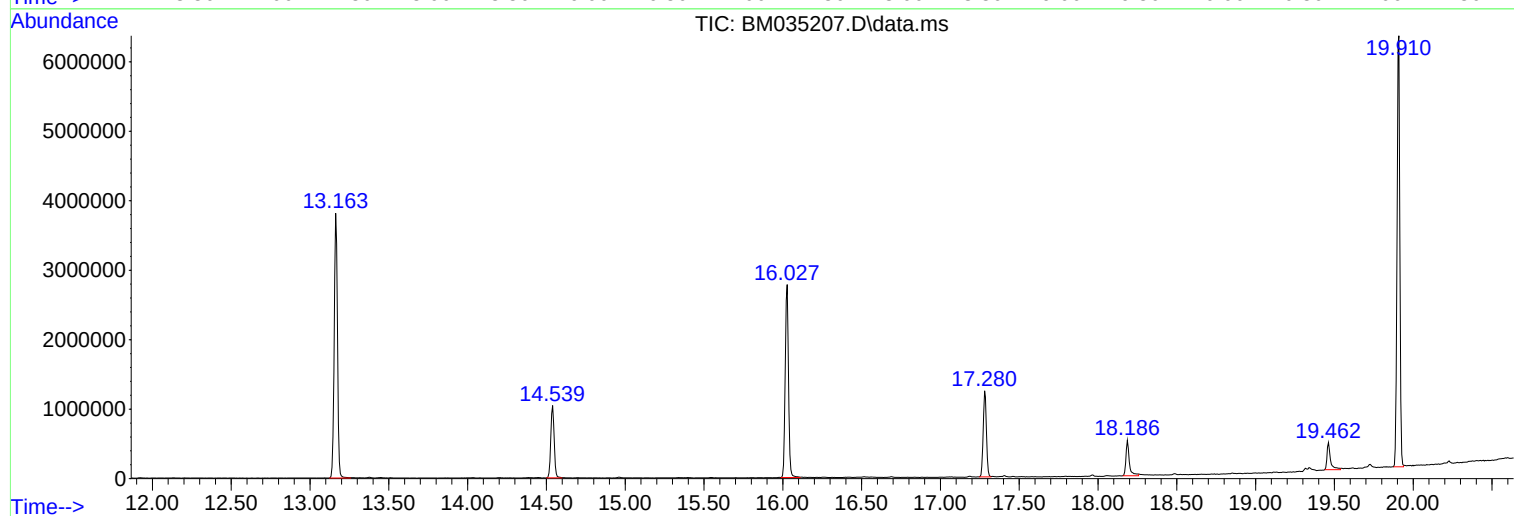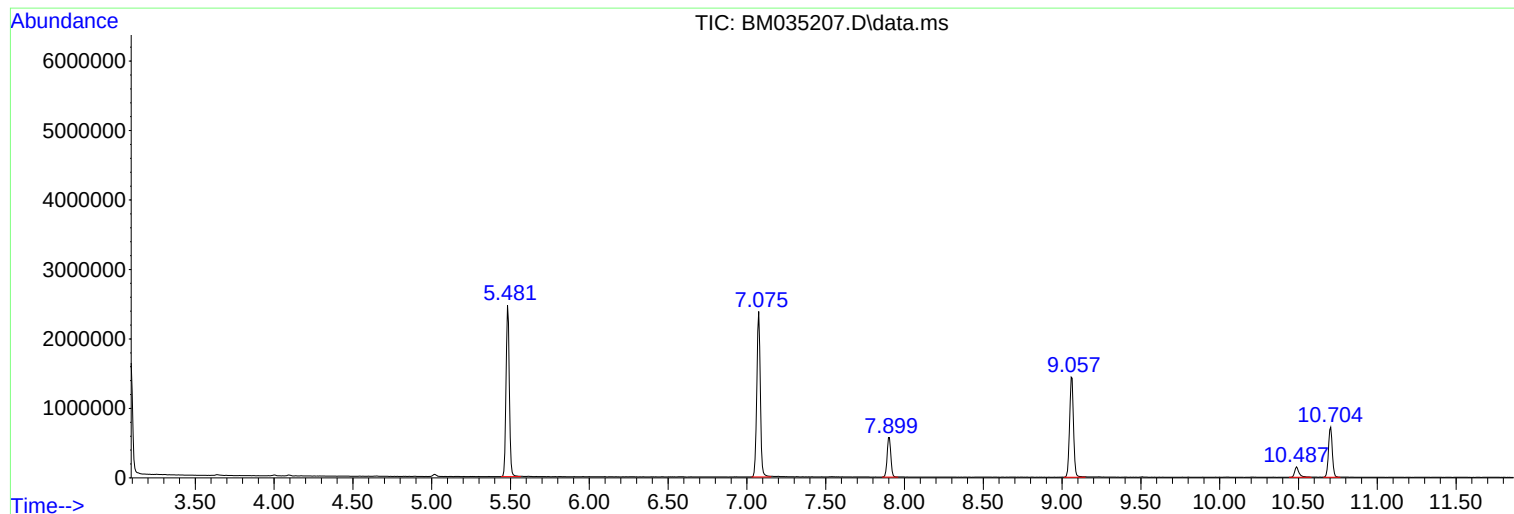

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035207.D
Acq On : 23 May 2022 23:02
Operator : CG/JU
Sample : N2874-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035207.D
Acq On : 23 May 2022 23:02
Operator : CG/JU
Sample : N2874-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------