

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035208.D
 Acq On : 23 May 2022 23:38
 Operator : CG/JU
 Sample : N2876-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P007-SS012-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	323	328	336	rVB2	59001	87799	1.33%	0.254%
2	5.481	400	407	422	rBV	2198914	3189119	48.45%	9.236%
3	7.075	670	678	693	rBV	1991214	3232102	49.10%	9.361%
4	7.898	811	818	827	rBV	573221	913535	13.88%	2.646%
5	9.057	1007	1015	1031	rBV	1249715	2121171	32.23%	6.143%
6	10.486	1252	1258	1271	rBV	143512	282199	4.29%	0.817%
7	10.704	1288	1295	1303	rBV	681864	1157629	17.59%	3.353%
8	13.163	1706	1713	1726	rBV	3145901	4645598	70.58%	13.454%
9	14.539	1940	1947	1958	rBV	976017	1446109	21.97%	4.188%
10	16.027	2194	2200	2216	rBV	2364688	3463554	52.62%	10.031%
11	17.280	2406	2413	2420	rBV	1145277	1666266	25.32%	4.826%
12	18.186	2562	2567	2577	rBV	332596	508592	7.73%	1.473%
13	19.462	2779	2784	2795	rBV	219073	374307	5.69%	1.084%
14	19.903	2854	2859	2867	rBV	5318875	6582117	100.00%	19.063%
15	21.180	3073	3076	3086	rBV	420490	598113	9.09%	1.732%
16	21.462	3119	3124	3133	rBV	1641008	2123148	32.26%	6.149%
17	23.844	3523	3529	3537	rVB2	1075697	2137164	32.47%	6.190%


Sum of corrected areas: 34528522

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035208.D
Acq On : 23 May 2022 23:38
Operator : CG/JU
Sample : N2876-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS012-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

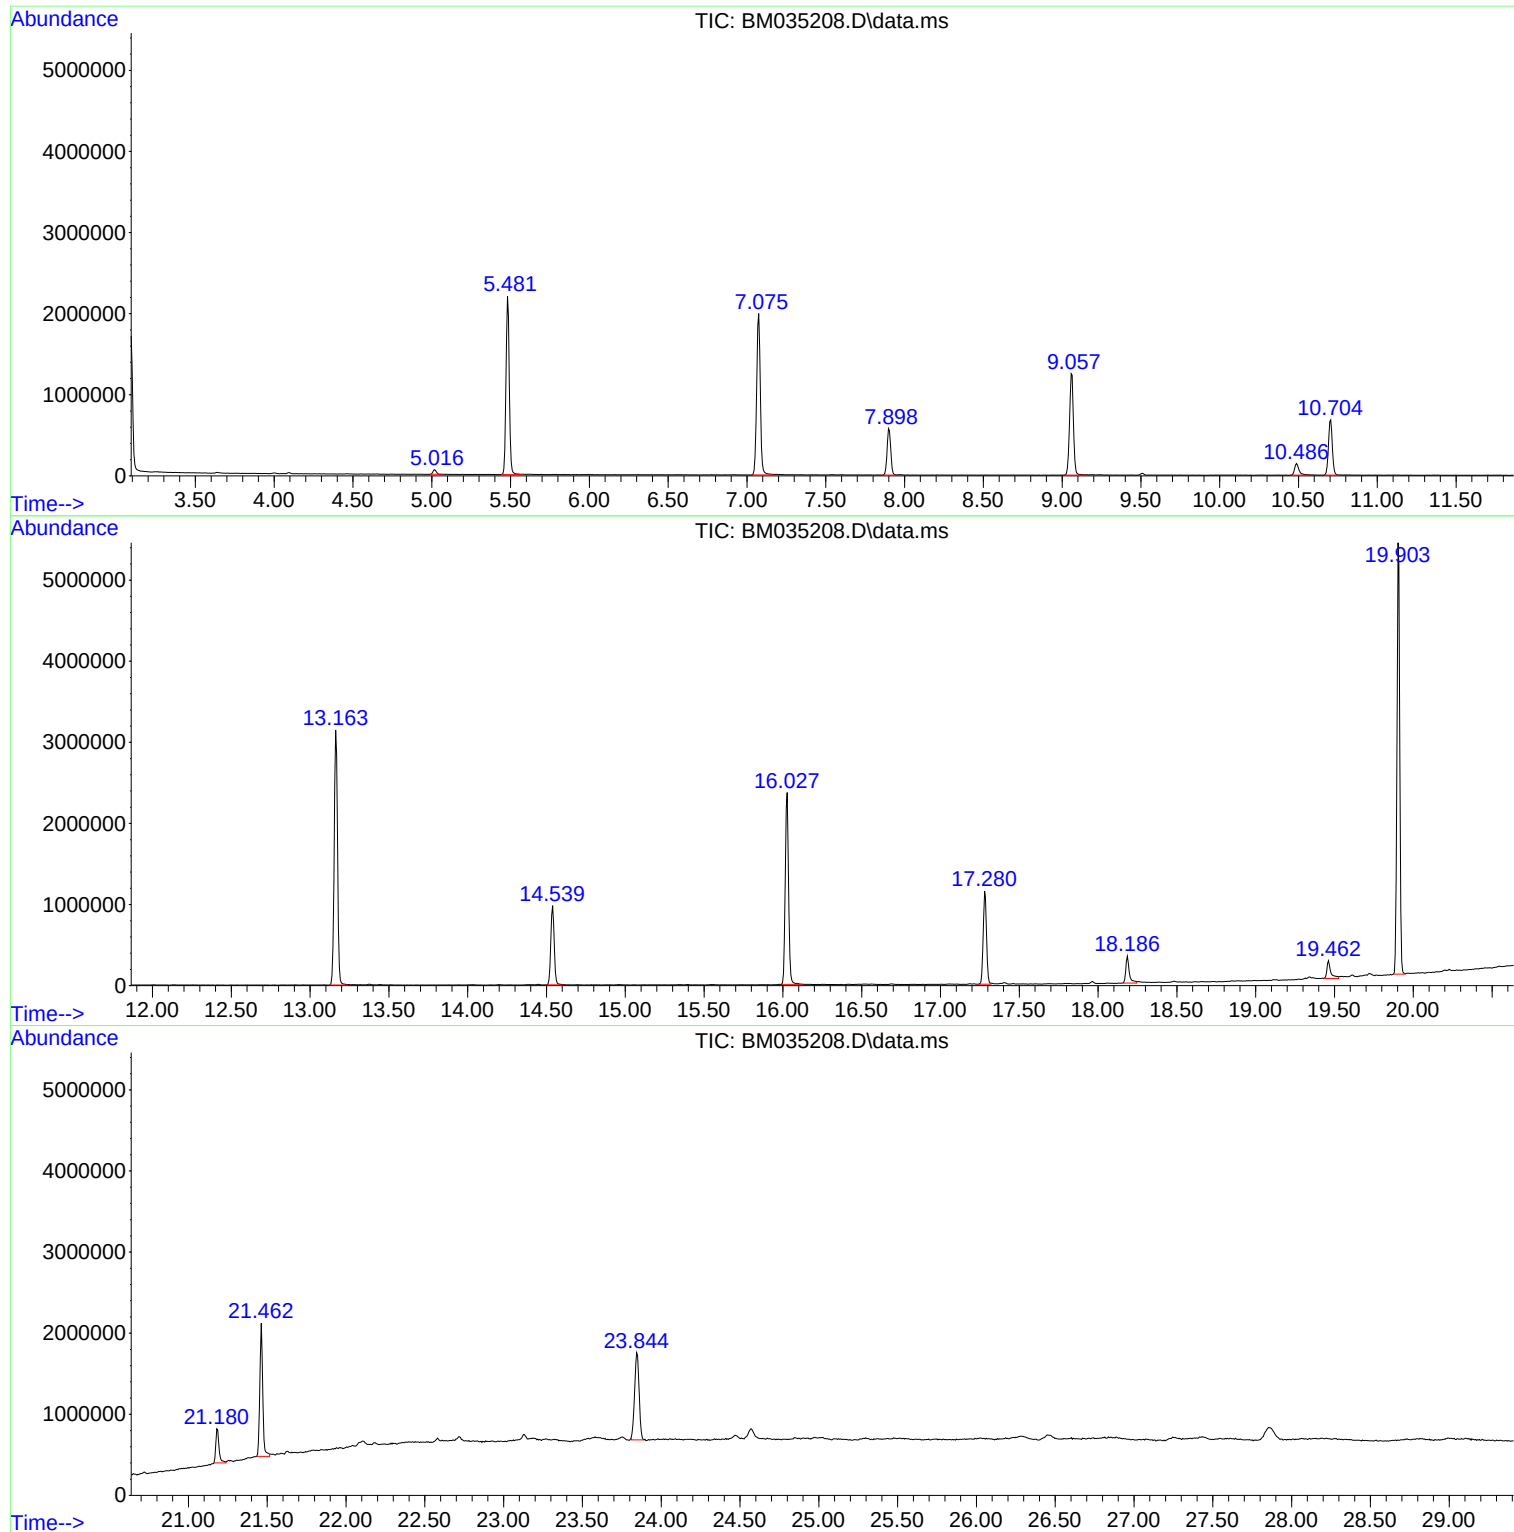

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035208.D
Acq On : 23 May 2022 23:38
Operator : CG/JU
Sample : N2876-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS012-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035208.D
Acq On : 23 May 2022 23:38
Operator : CG/JU
Sample : N2876-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS012-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------