

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035210.D
 Acq On : 24 May 2022 00:50
 Operator : CG/JU
 Sample : N2874-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P007-SS003-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	401	407	421	rBV	2214116	3320381	49.43%	8.928%
2	7.075	670	678	694	rBV	2106280	3362244	50.06%	9.041%
3	7.904	811	819	826	rBV	585018	932607	13.88%	2.508%
4	9.063	1008	1016	1028	rBV	1291088	2164471	32.22%	5.820%
5	10.704	1287	1295	1305	rBV	731171	1238145	18.43%	3.329%
6	13.163	1706	1713	1728	rBV	3257911	4810478	71.62%	12.935%
7	14.539	1939	1947	1963	rBV	1062680	1610561	23.98%	4.331%
8	16.027	2193	2200	2209	rBV	2684876	3748701	55.81%	10.080%
9	17.186	2392	2397	2400	rBV	76652	100139	1.49%	0.269%
10	17.280	2405	2413	2420	rBV	1282857	1883333	28.04%	5.064%
11	18.062	2541	2546	2553	rBV7	33748	72462	1.08%	0.195%
12	18.186	2562	2567	2578	rBV	718300	1069241	15.92%	2.875%
13	18.480	2613	2617	2622	rBV4	69791	113327	1.69%	0.305%
14	19.315	2756	2759	2761	rBV2	55237	73694	1.10%	0.198%
15	19.345	2761	2764	2766	rVV2	54568	67510	1.01%	0.182%
16	19.462	2780	2784	2796	rBV	495963	752433	11.20%	2.023%
17	19.909	2854	2860	2866	rBV	5373689	6716895	100.00%	18.061%
18	21.186	3073	3077	3085	rVB	436842	572293	8.52%	1.539%
19	21.380	3108	3110	3114	rVB	208485	214897	3.20%	0.578%
20	21.462	3120	3124	3135	rVB	1696899	2158899	32.14%	5.805%
21	23.850	3524	3530	3538	rVB2	1108142	2207565	32.87%	5.936%




Sum of corrected areas: 37190276

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035210.D
Acq On : 24 May 2022 00:50
Operator : CG/JU
Sample : N2874-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

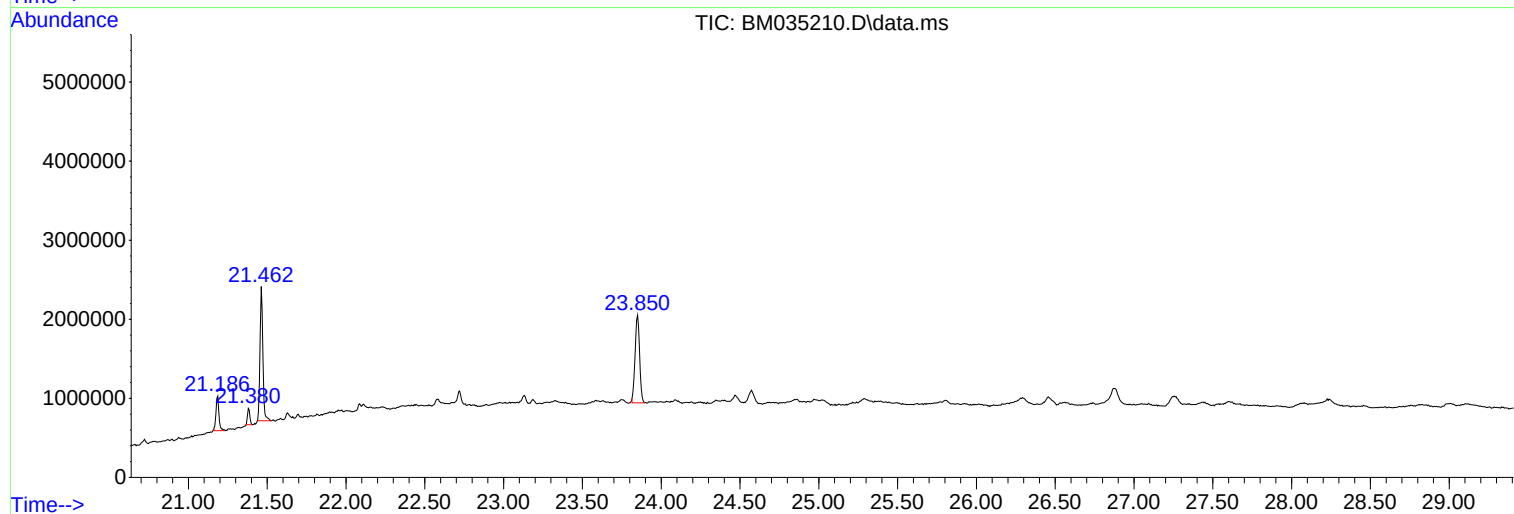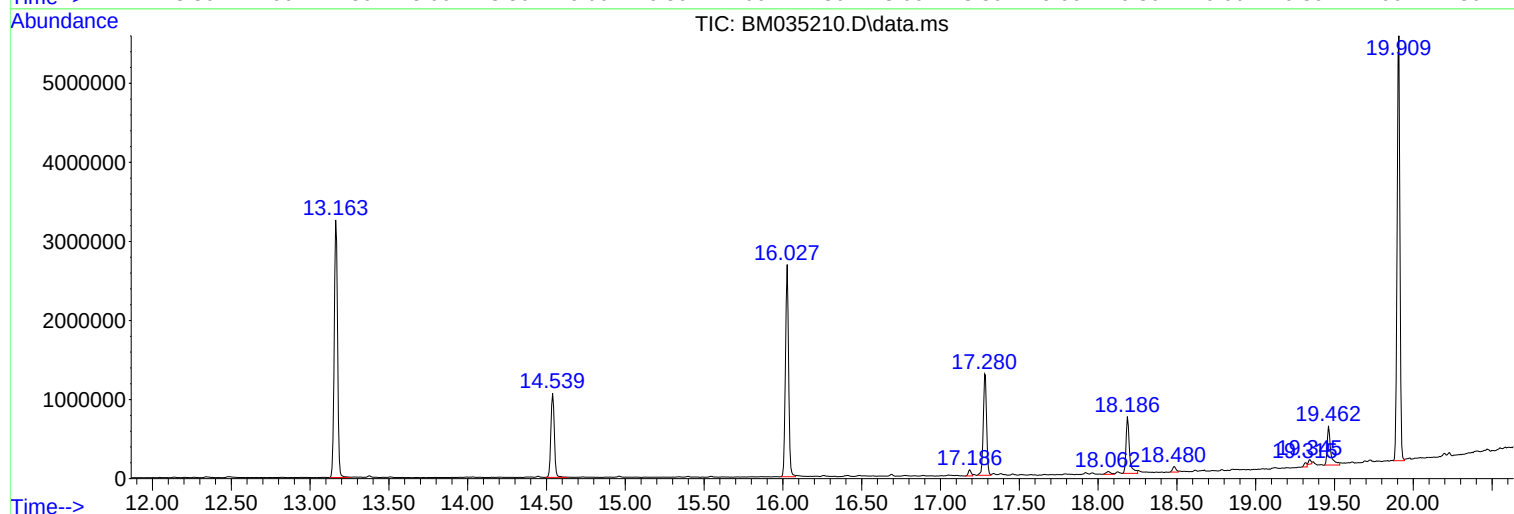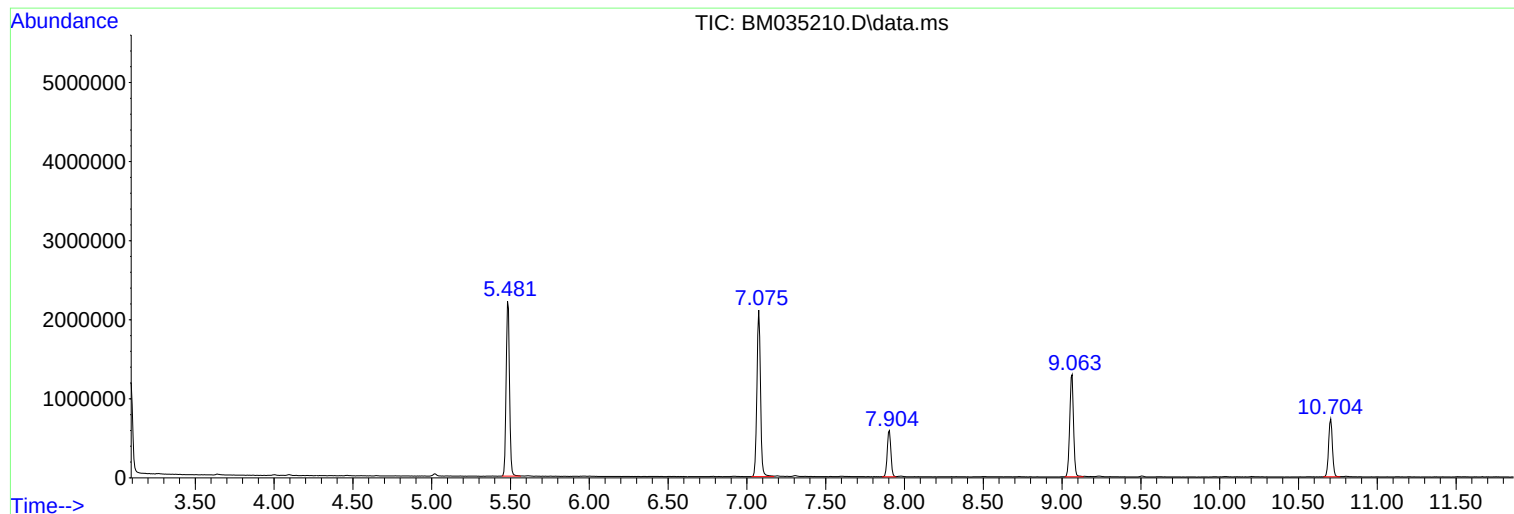

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035210.D
Acq On : 24 May 2022 00:50
Operator : CG/JU
Sample : N2874-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035210.D
Acq On : 24 May 2022 00:50
Operator : CG/JU
Sample : N2874-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------