

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035213.D
 Acq On : 24 May 2022 02:38
 Operator : CG/JU
 Sample : N2876-14 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P007-SS013-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	401	407	414	rBV	156013	242896	9.62%	1.788%
2	7.075	671	678	687	rBV	136846	241997	9.59%	1.782%
3	7.904	812	819	827	rBV	643436	1029629	40.80%	7.581%
4	9.063	1010	1016	1026	rBV	86394	159705	6.33%	1.176%
5	10.704	1287	1295	1307	rBV	817619	1373902	54.44%	10.116%
6	13.163	1707	1713	1723	rBV	267488	411621	16.31%	3.031%
7	14.539	1940	1947	1965	rBV	1206065	1798352	71.25%	13.241%
8	16.027	2195	2200	2210	rBV	181356	283598	11.24%	2.088%
9	17.286	2408	2414	2425	rBV	1457431	2064310	81.79%	15.199%
10	18.186	2563	2567	2576	rBV2	102740	171286	6.79%	1.261%
11	19.462	2781	2784	2794	rBV2	135604	235167	9.32%	1.732%
12	19.904	2855	2859	2865	rBV	492835	614070	24.33%	4.521%
13	21.468	3120	3125	3131	rBV	1876564	2431245	96.33%	17.901%
14	23.850	3525	3530	3539	rVB2	1278416	2523877	100.00%	18.583%




Sum of corrected areas: 13581655

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035213.D
Acq On : 24 May 2022 02:38
Operator : CG/JU
Sample : N2876-14 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS013-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

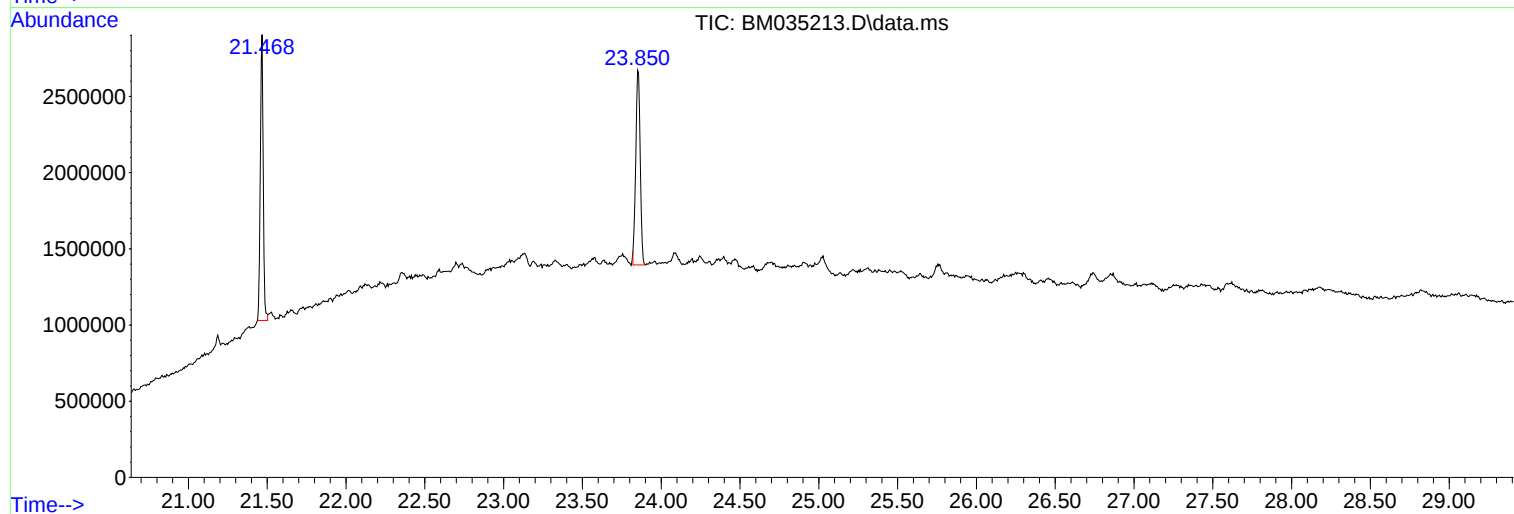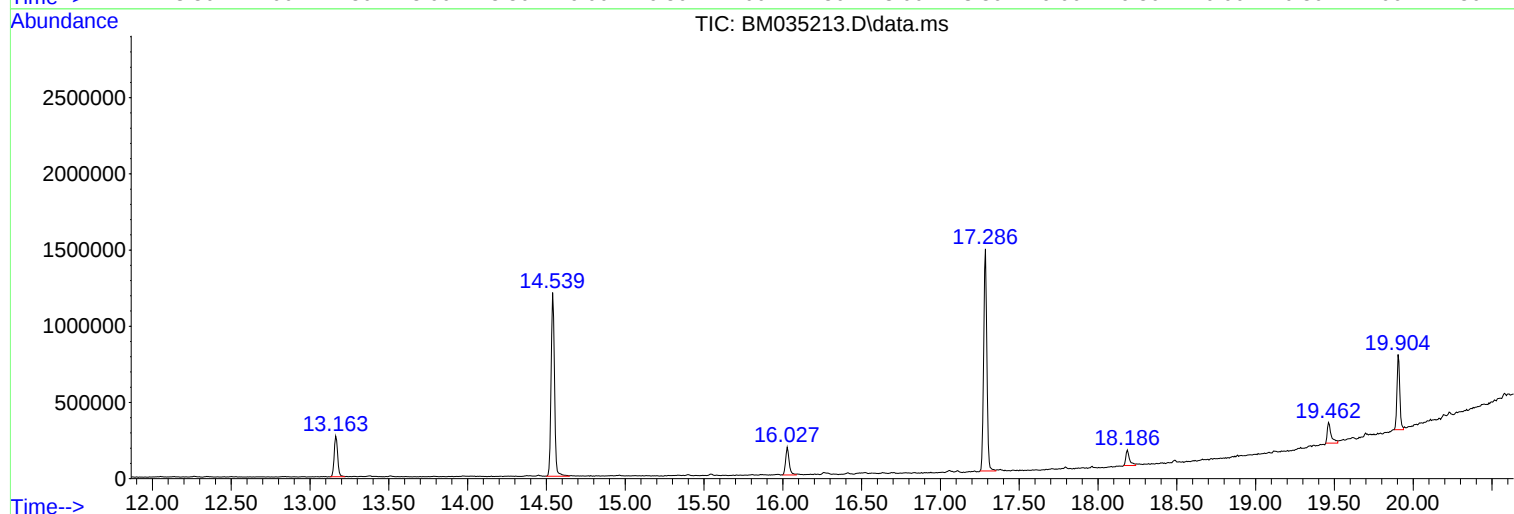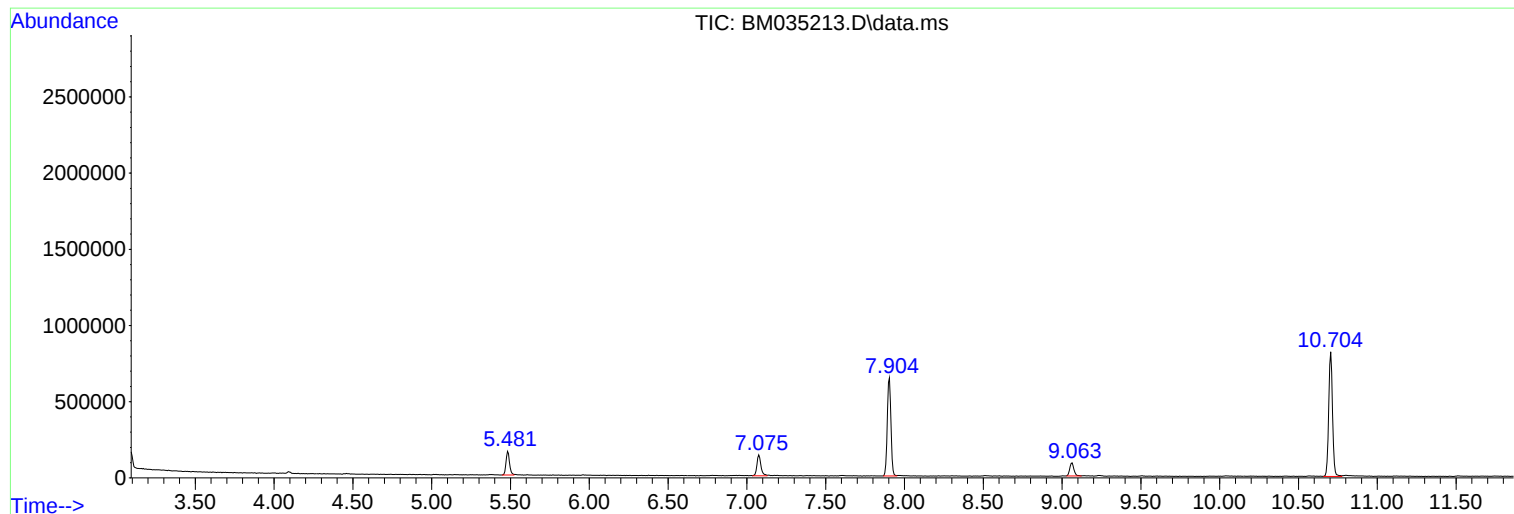

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035213.D
Acq On : 24 May 2022 02:38
Operator : CG/JU
Sample : N2876-14 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS013-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035213.D
Acq On : 24 May 2022 02:38
Operator : CG/JU
Sample : N2876-14 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P007-SS013-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------