
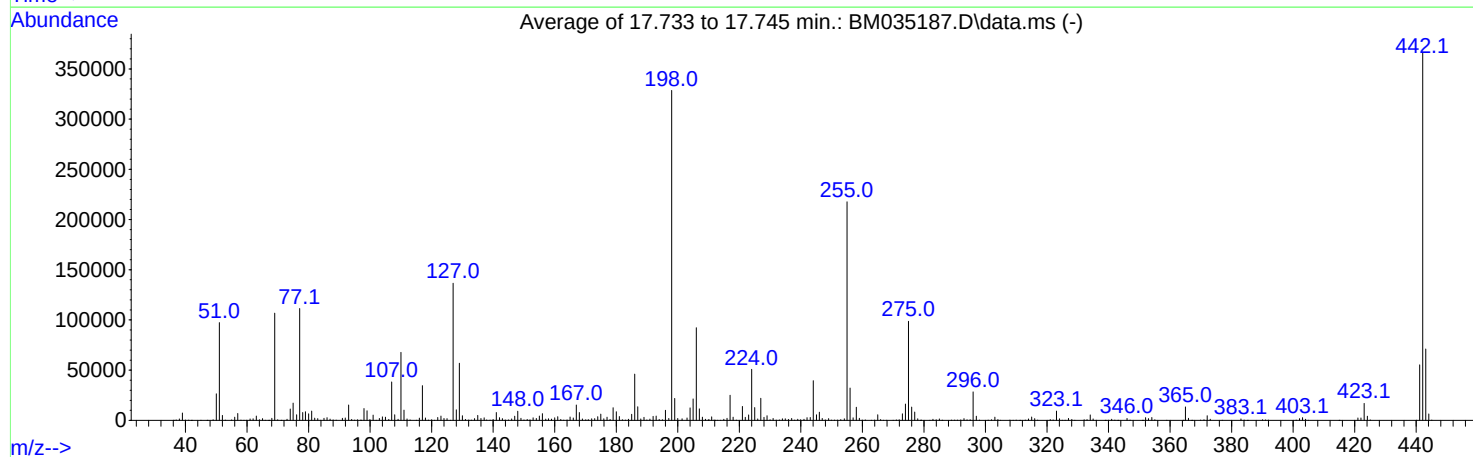


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035187.D
 Acq On : 23 May 2022 10:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 04:53:59 2022

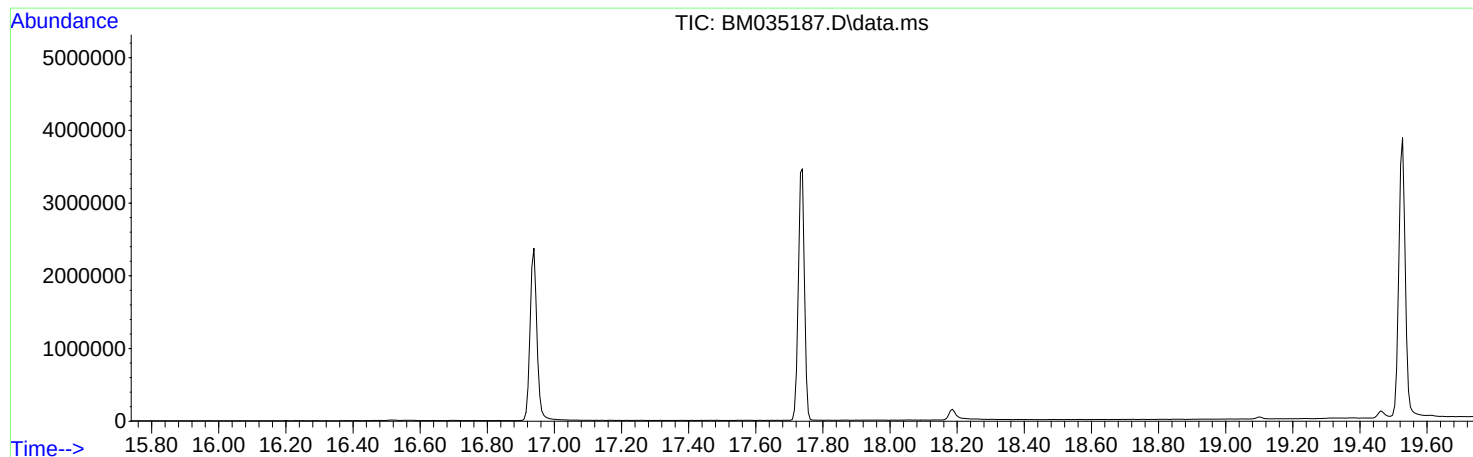




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	97392	PASS
68	69	0.00	2	2.0	2085	PASS
69	198	0.00	100	32.5	106764	PASS
70	69	0.00	2	0.6	652	PASS
127	198	10	80	41.6	136595	PASS
197	198	0.00	2	0.6	1985	PASS
198	198	100	100	100.0	328576	PASS
199	198	5	9	6.6	21760	PASS
275	198	10	60	30.0	98677	PASS
365	198	1	100	4.1	13420	PASS
441	198	0.01	100	16.9	55381	PASS
442	442	50	100	100.0	366357	PASS
443	442	15	24	19.4	71165	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035187.D
 Acq On : 23 May 2022 10:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 24 08:07:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

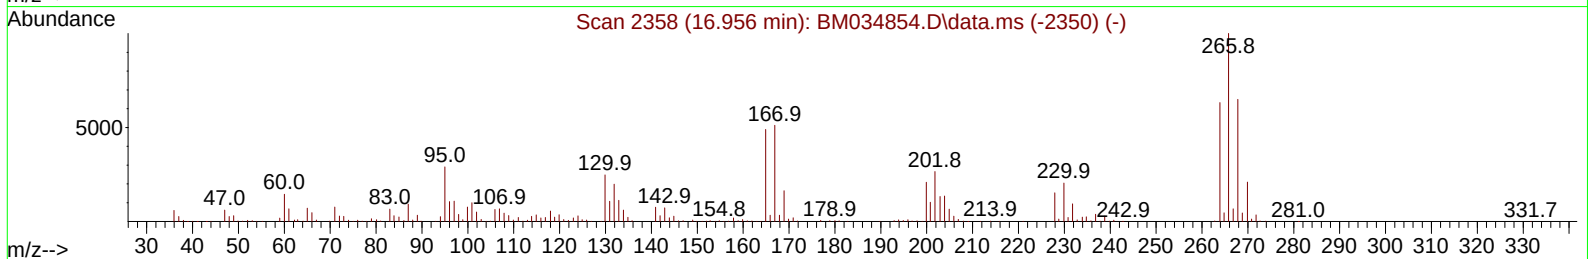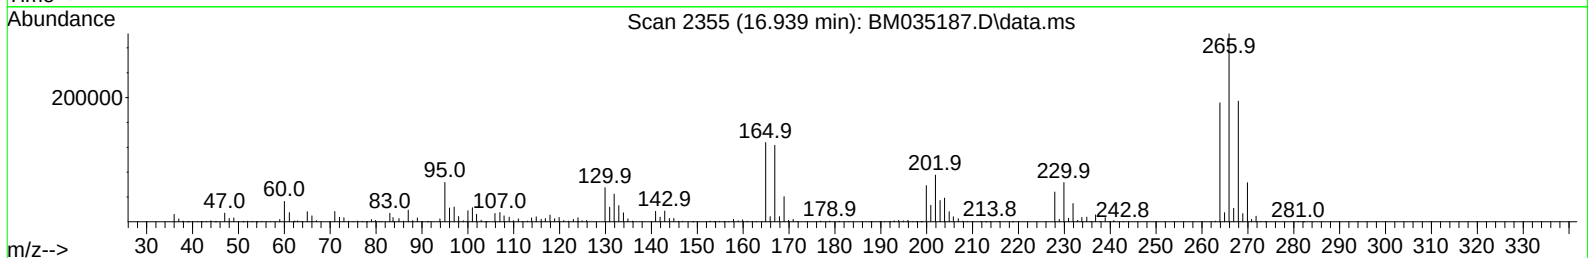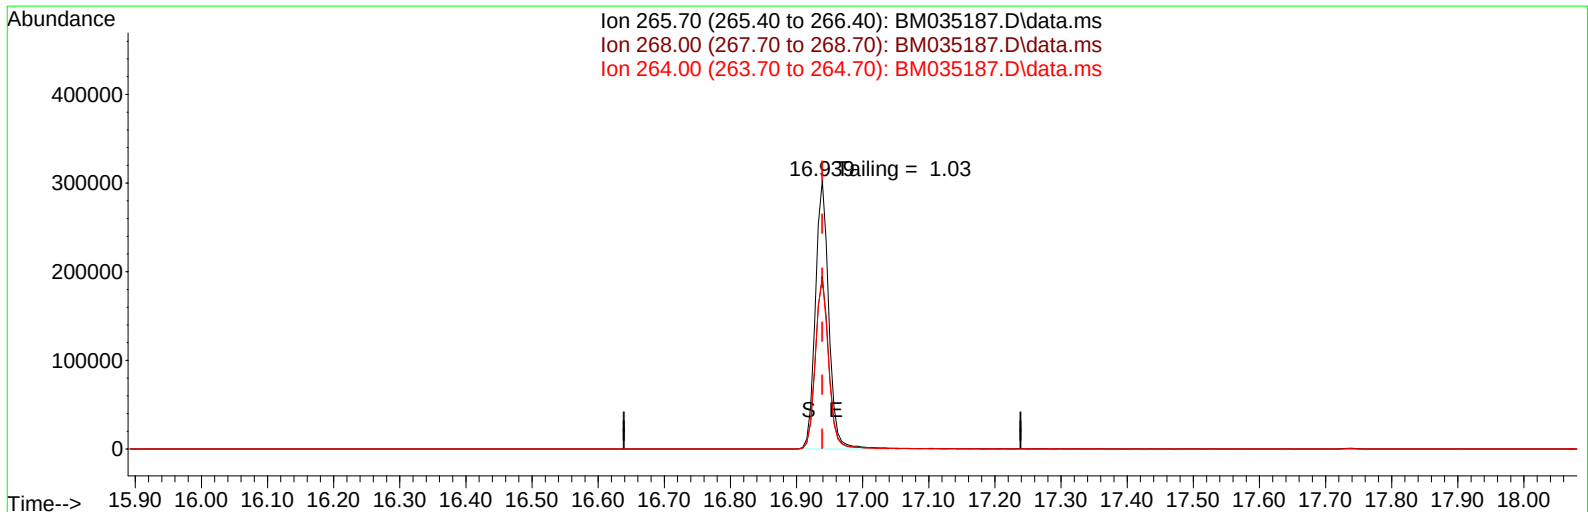

TIC: BM035187.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.000) 891350.75 ng




response 429425

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.19
264.00	63.30	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035187.D
Acq On : 23 May 2022 10:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 24 08:07:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

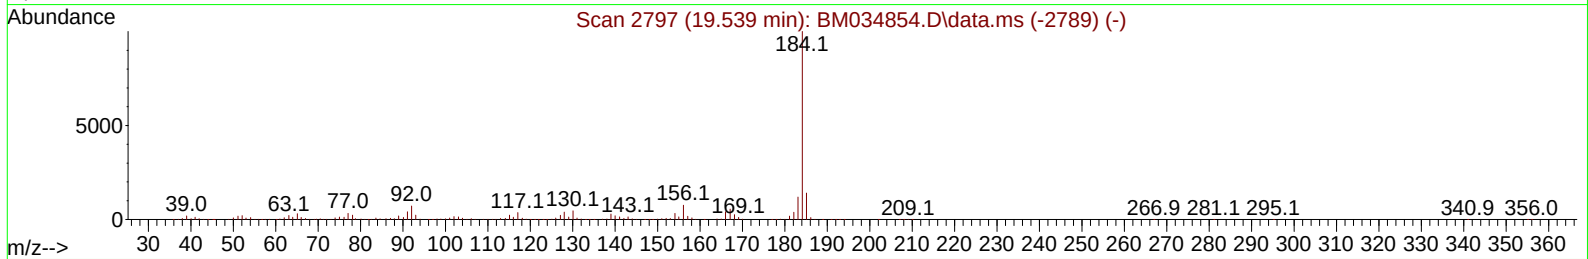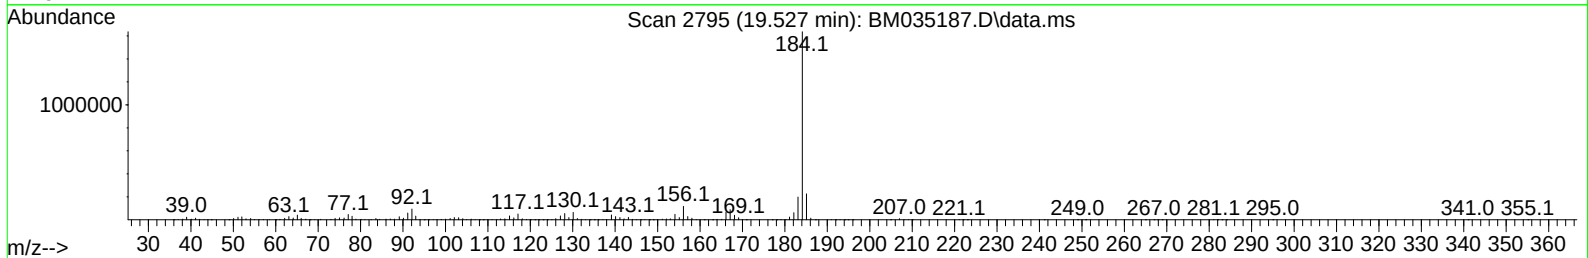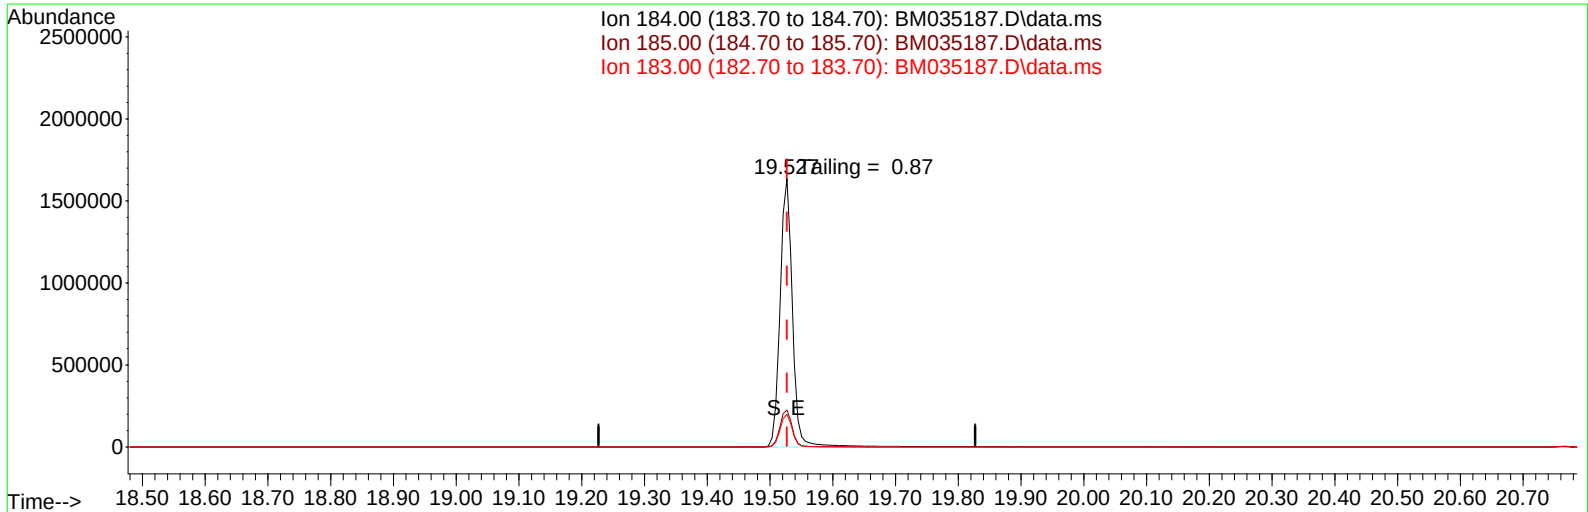

TIC: BM035187.D\data.ms

(77) Benzidine

19.527min (-0.000) 108137.78 ng

response 2239799

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.78
183.00	11.90	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2022	BNA_M	<u>BM035187.D</u>
Compound Name	Response	Retention Time
DDT	1273804	20.768
DDD	18122	20.327
DDE	1852	19.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19974	1293778	1.54

Instrument :
BNA_M
ClientSampleId :
DFTPP