
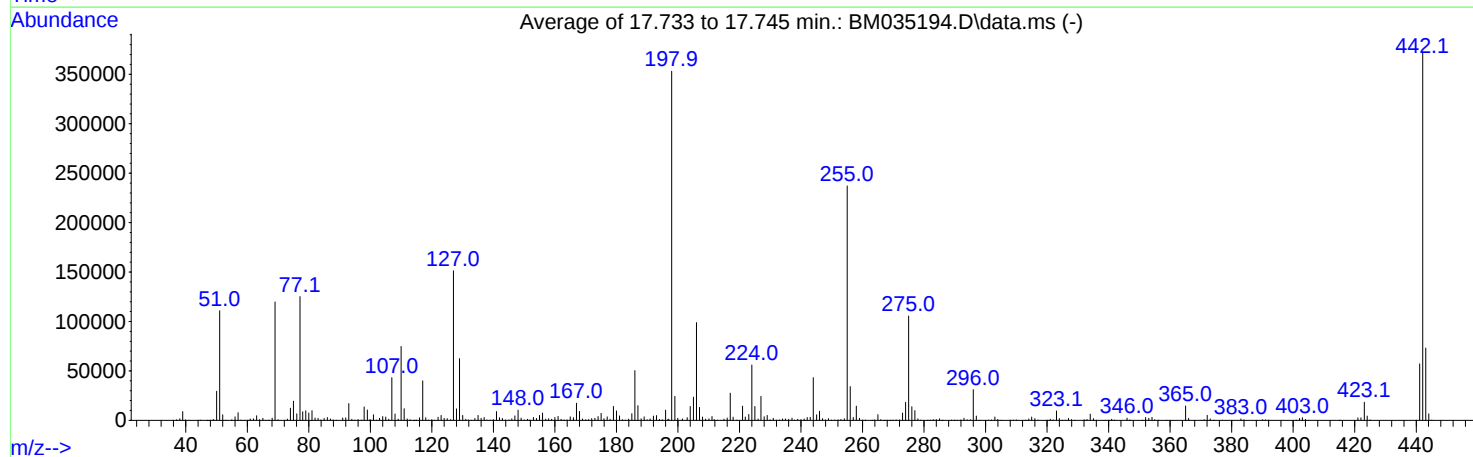


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035194.D
 Acq On : 23 May 2022 15:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 04:53:59 2022

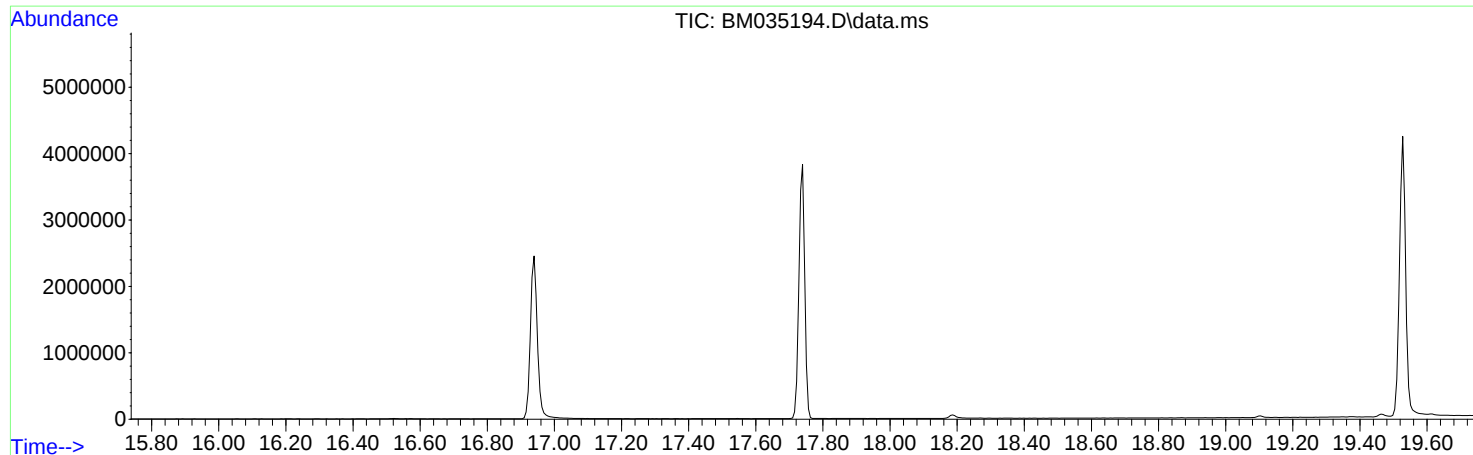




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	110904	PASS
68	69	0.00	2	1.9	2256	PASS
69	198	0.00	100	33.9	119760	PASS
70	69	0.00	2	0.6	664	PASS
127	198	10	80	42.9	151363	PASS
197	198	0.00	2	0.4	1253	PASS
198	198	100	100	100.0	353067	PASS
199	198	5	9	6.9	24301	PASS
275	198	10	60	29.9	105445	PASS
365	198	1	100	4.1	14572	PASS
441	198	0.01	100	16.2	57088	PASS
442	442	50	100	100.0	372053	PASS
443	442	15	24	19.6	73096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
 Data File : BM035194.D
 Acq On : 23 May 2022 15:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 24 08:09:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

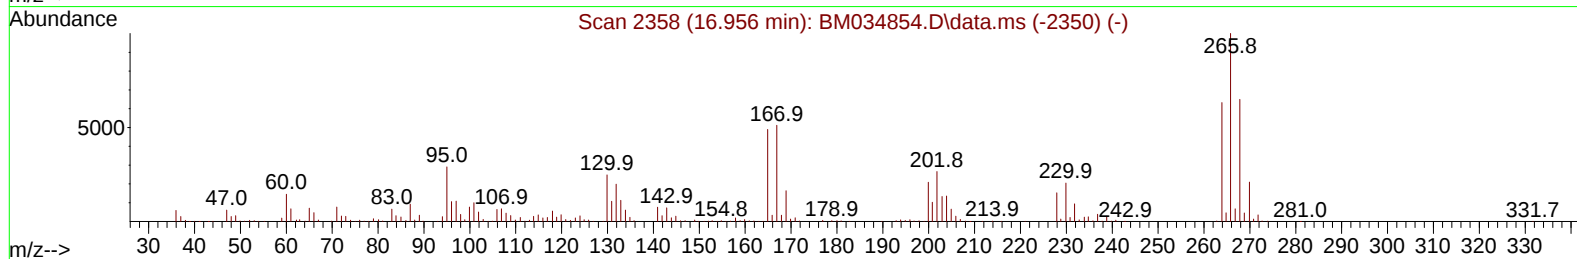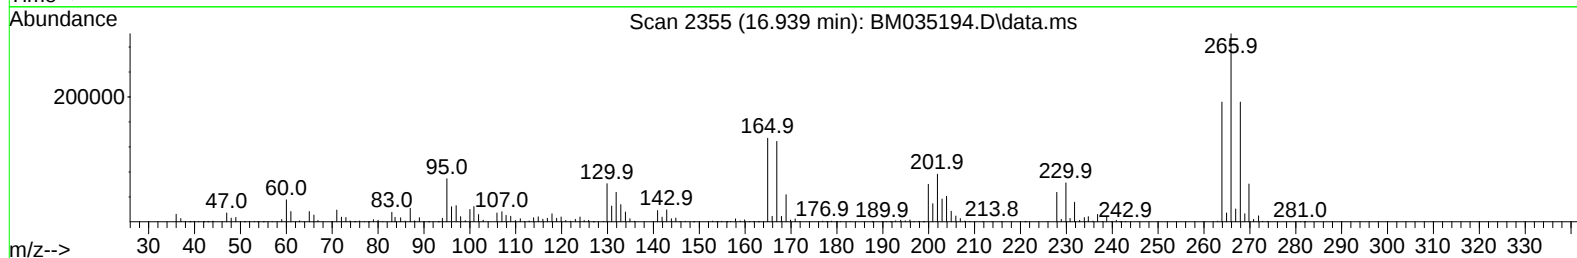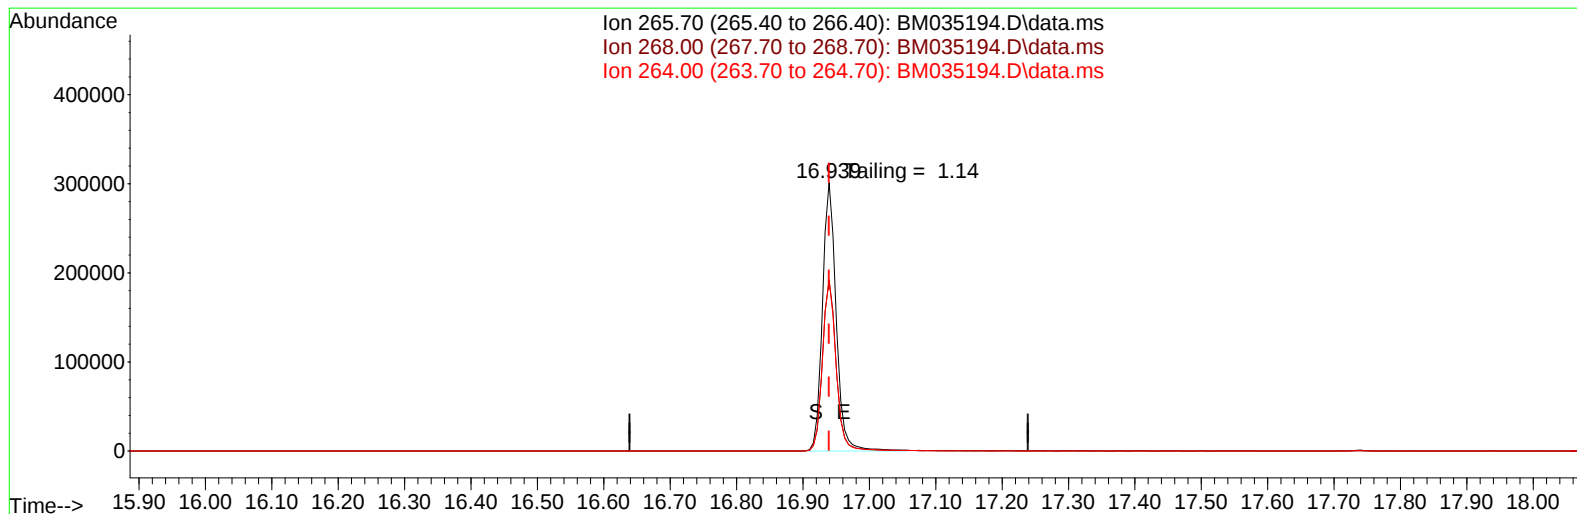

TIC: BM035194.D\data.ms

(70) Pentachlorophenol (C)

16.939min (+ 0.000) 378123.21 ng




response 435028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.68
264.00	63.30	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052322\
Data File : BM035194.D
Acq On : 23 May 2022 15:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 24 08:09:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

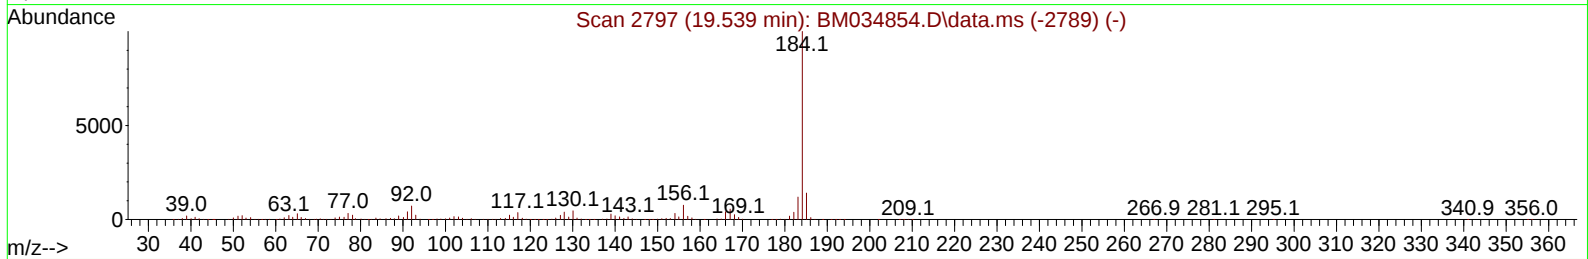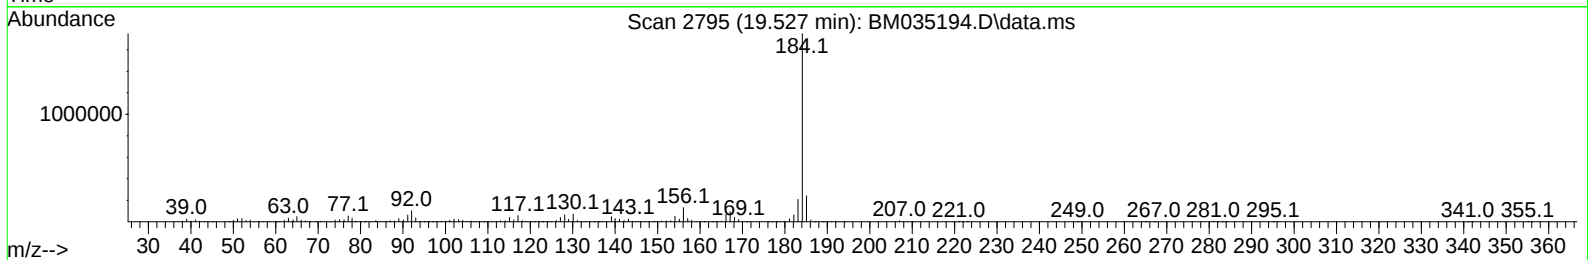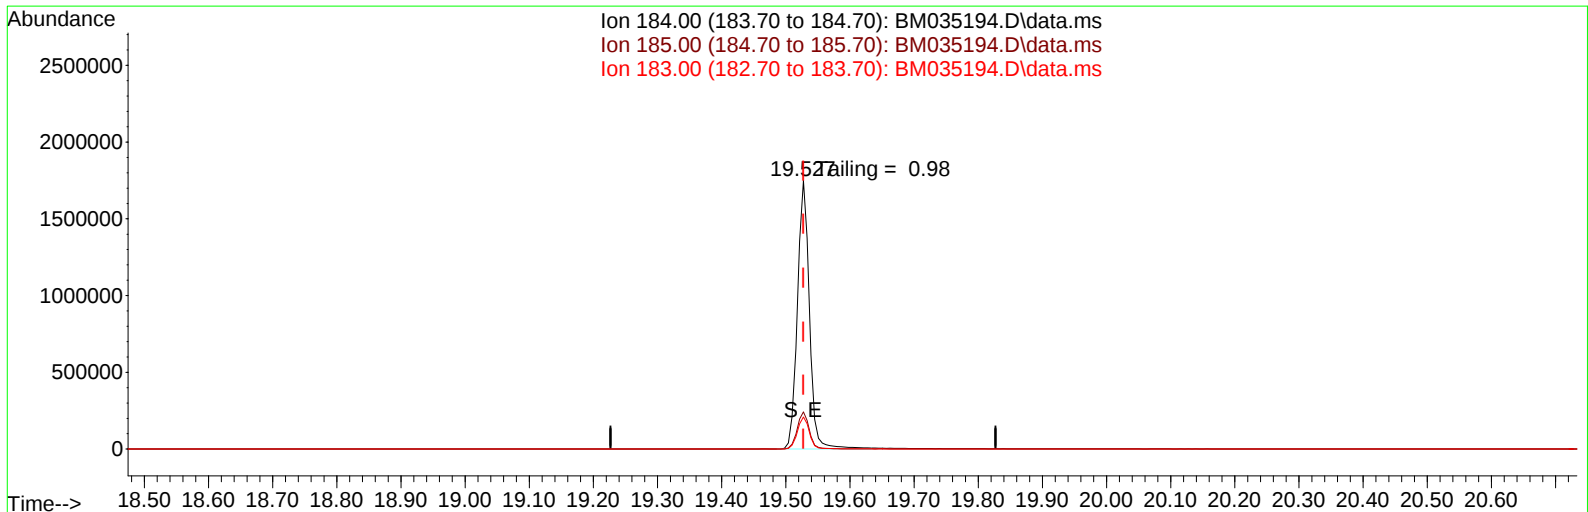

TIC: BM035194.D\data.ms

(77) Benzidine

19.527min (+ 0.000) 142627.95 ng

response 2313668

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.83
183.00	11.90	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2022	BNA_M	<u>BM035194.D</u>
Compound Name	Response	Retention Time
DDT	1342913	20.762
DDD	19338	20.327
DDE	2576	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21914	1364827	1.61

Instrument :
BNA_M
ClientSampleId :
DFTPP