
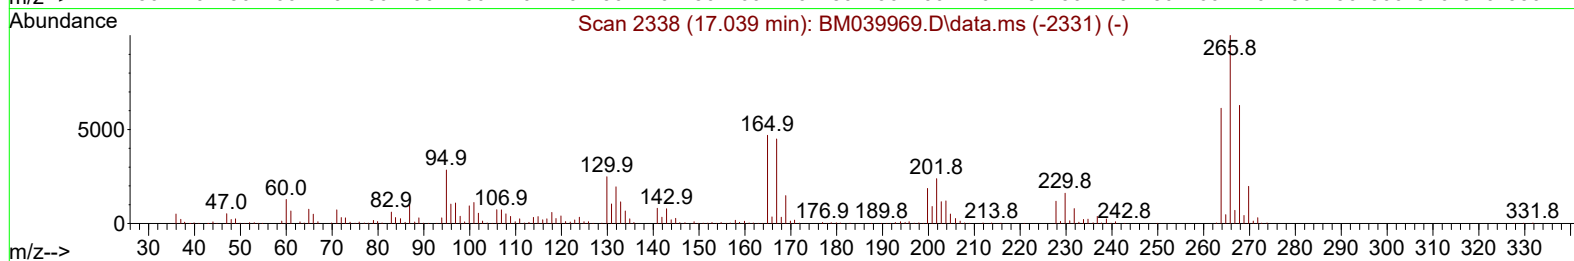
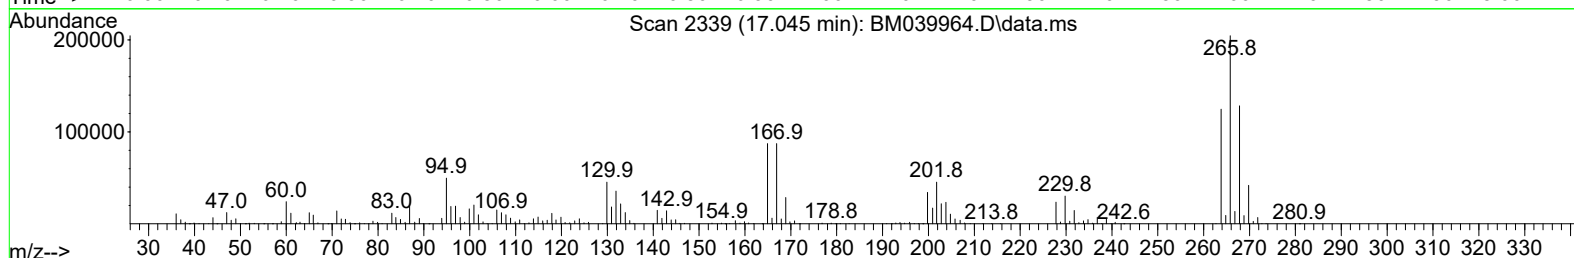


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052323\
 Data File : BM039964.D
 Acq On : 23 May 2023 09:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 06:46:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 01:06:13 2023
 Response via : Initial Calibration

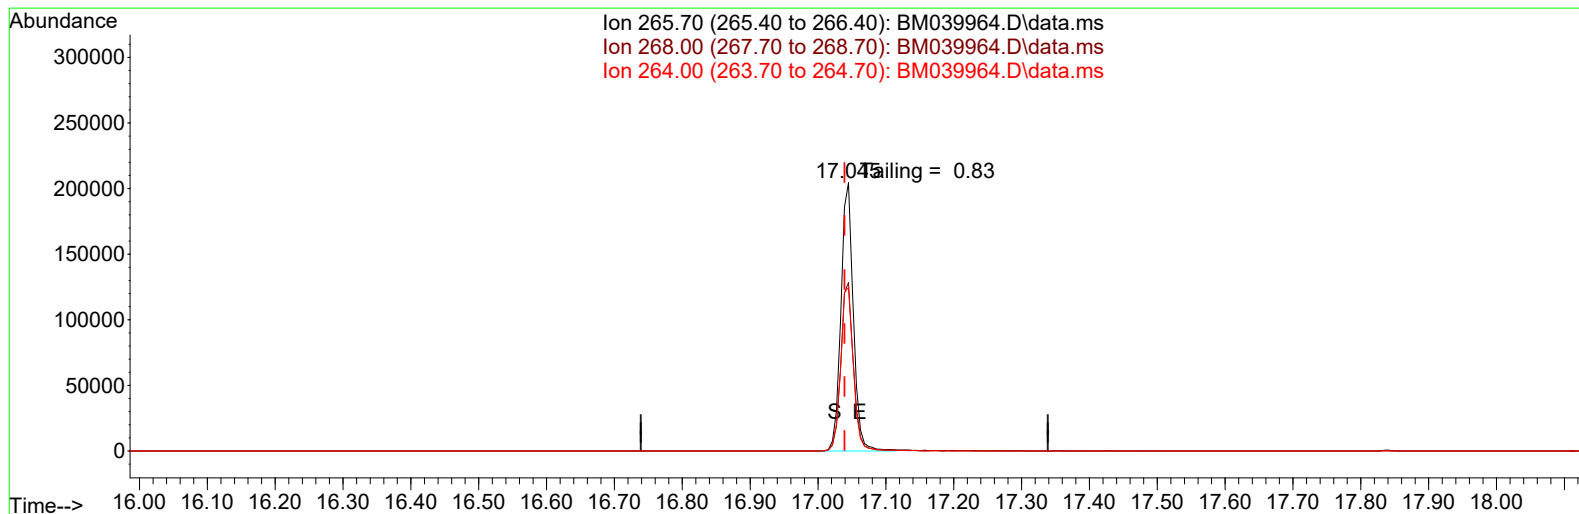

TIC: BM039964.D\data.ms

(70) Pentachlorophenol (C)




17.045min (+ 0.006) 0.00 ng

response 259356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.76
264.00	61.30	60.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052323\
 Data File : BM039964.D
 Acq On : 23 May 2023 09:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 06:46:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 01:06:13 2023
 Response via : Initial Calibration

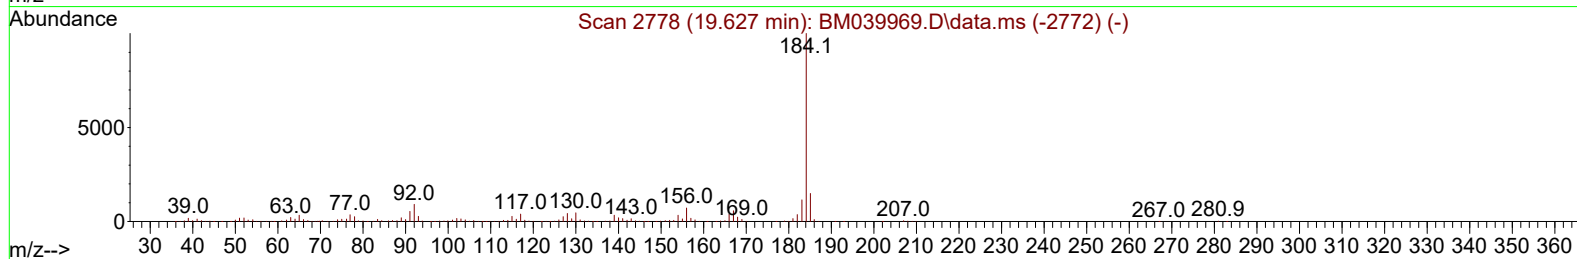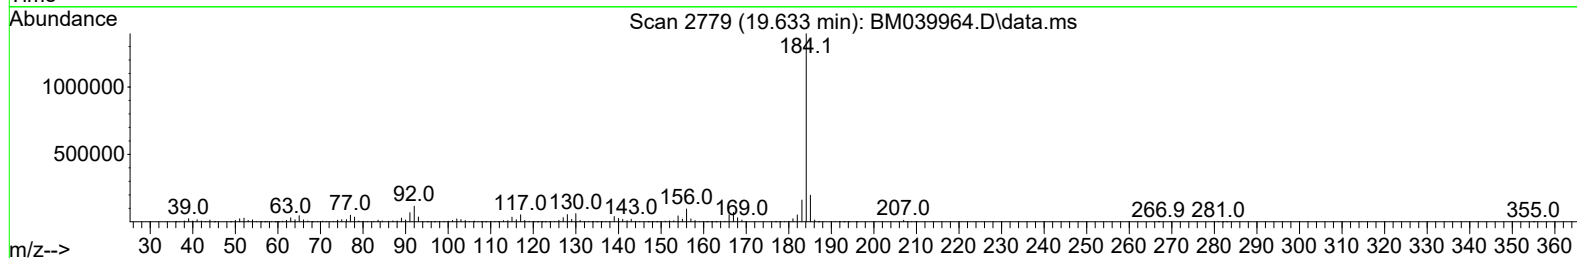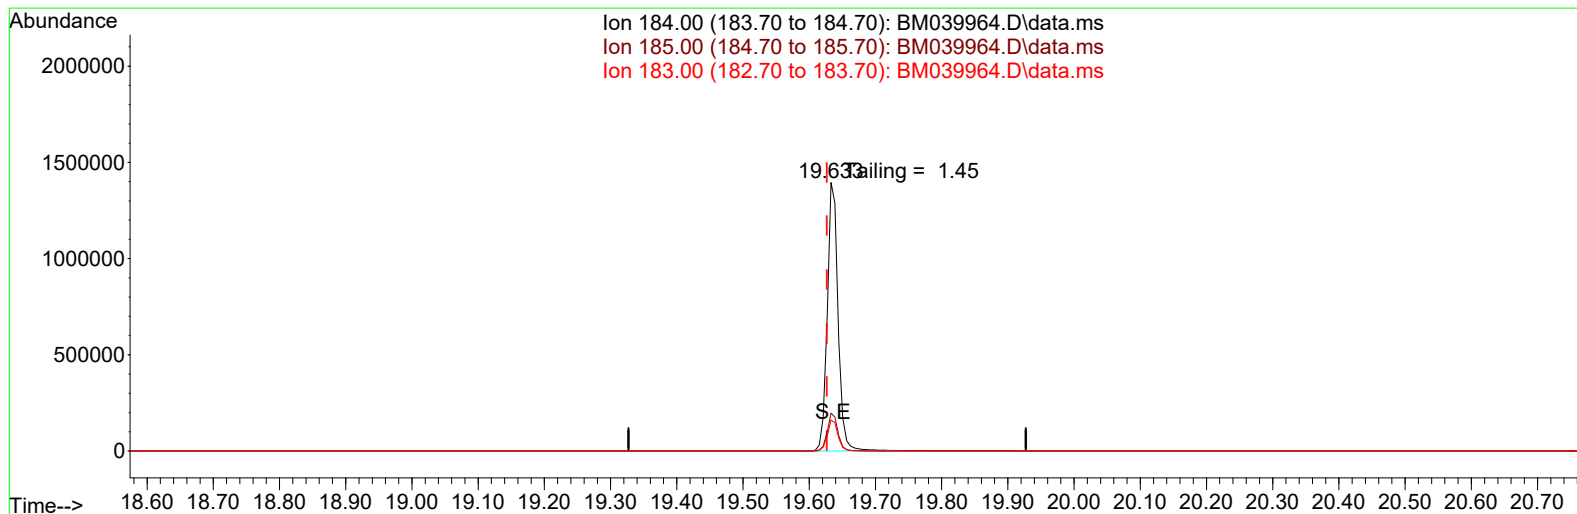

TIC: BM039964.D\data.ms

(77) Benzidine**19.633min (+ 0.006) 0.00 ng****response 1587306**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.16
183.00	11.50	11.60
0.00	0.00	0.00