


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052323\
Data File : BM039964.D
Acq On : 23 May 2023 09:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 24 01:06:13 2023

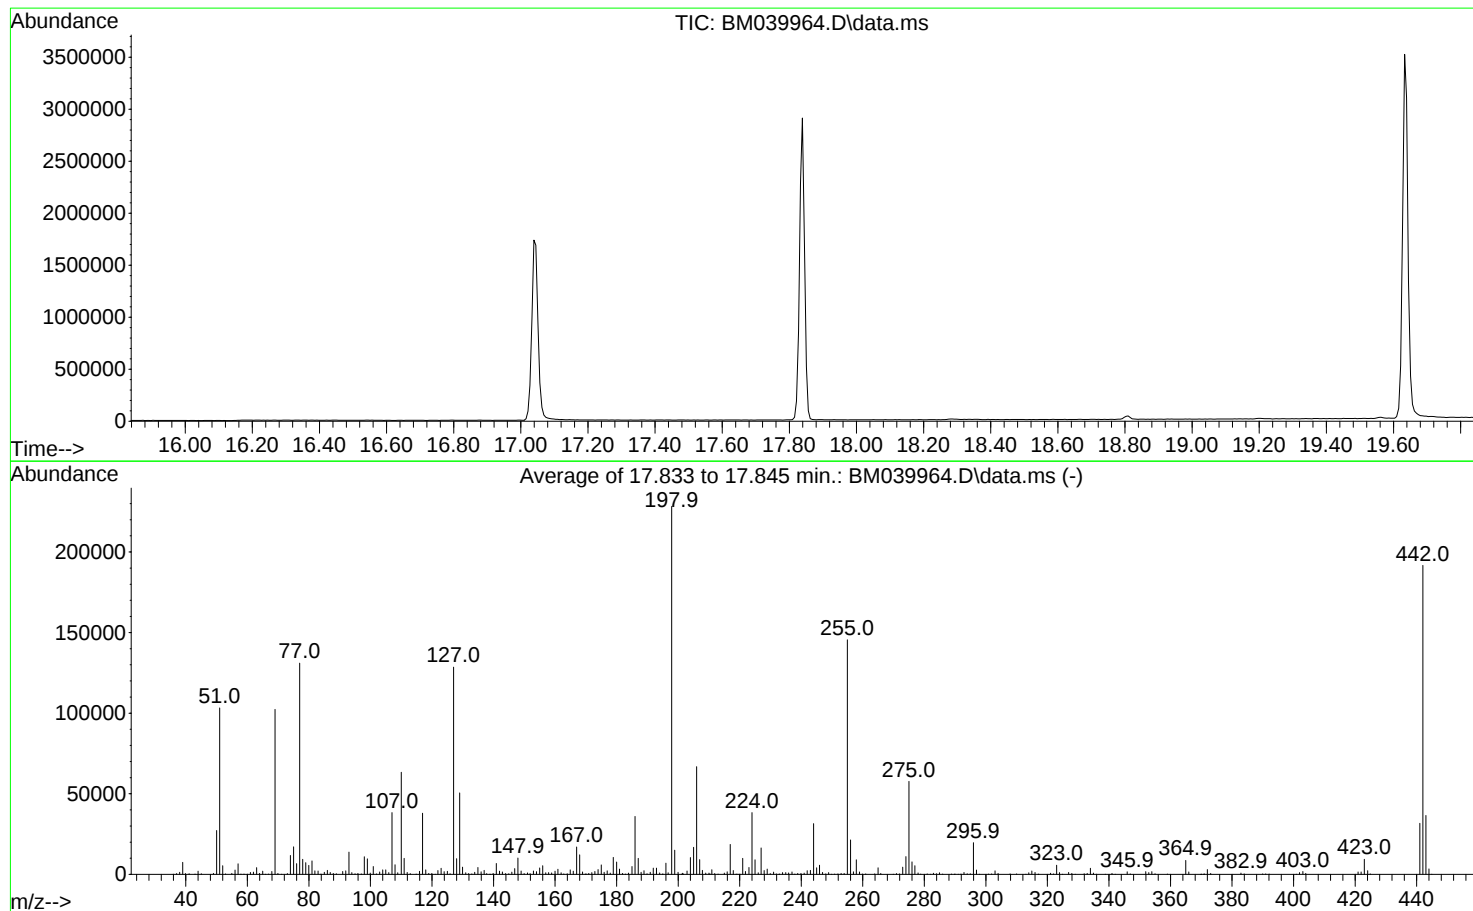




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	103210	PASS
68	69	0.00	2	1.7	1752	PASS
69	198	0.00	100	44.8	102339	PASS
70	69	0.00	2	0.6	648	PASS
127	198	10	80	56.3	128499	PASS
197	198	0.00	2	0.4	1003	PASS
198	198	100	100	100.0	228203	PASS
199	198	5	9	6.6	14961	PASS
275	198	10	60	25.3	57648	PASS
365	198	1	100	3.8	8673	PASS
441	198	0.01	100	13.9	31645	PASS
442	442	50	100	100.0	191659	PASS
443	442	15	24	19.1	36544	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052323\
 Data File : BM039964.D
 Acq On : 23 May 2023 09:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 24 06:46:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 01:06:13 2023
 Response via : Initial Calibration

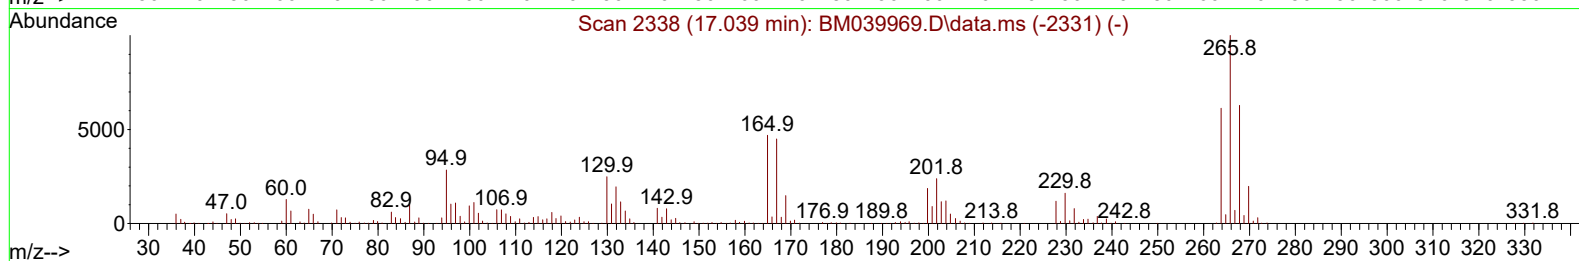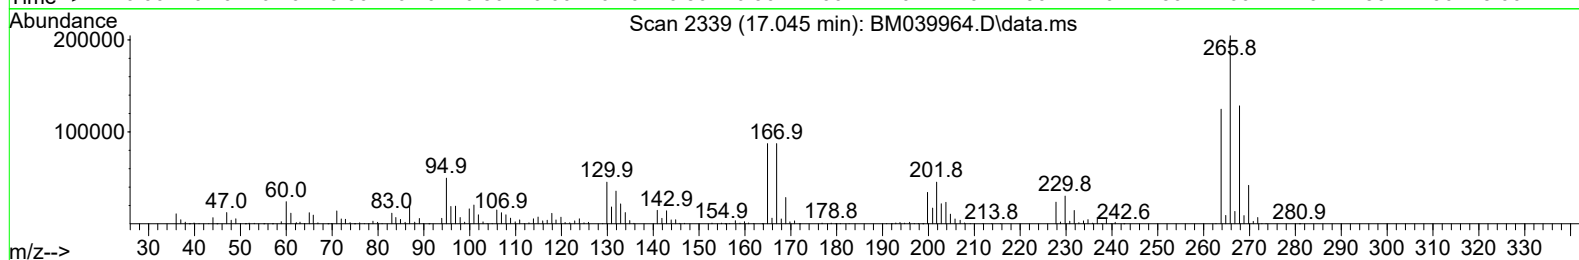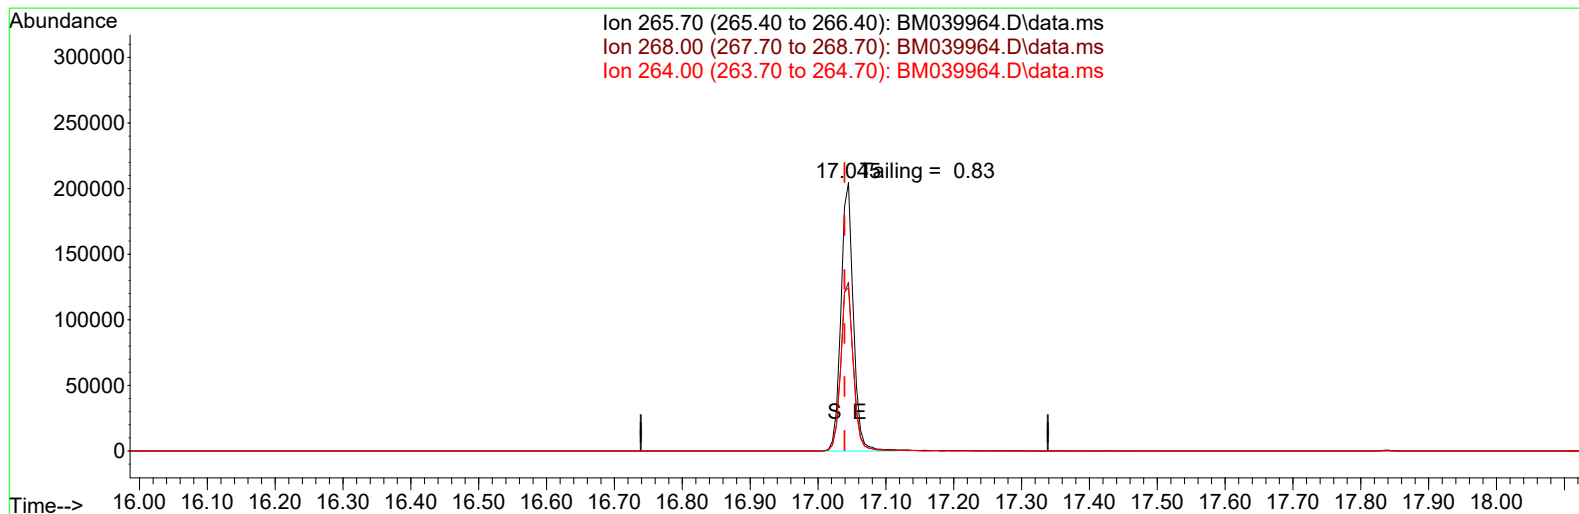

TIC: BM039964.D\data.ms

(70) Pentachlorophenol (C)

17.045min (+ 0.006) 0.00 ng




response 259356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.76
264.00	61.30	60.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052323\
Data File : BM039964.D
Acq On : 23 May 2023 09:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 24 06:46:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 01:06:13 2023
Response via : Initial Calibration

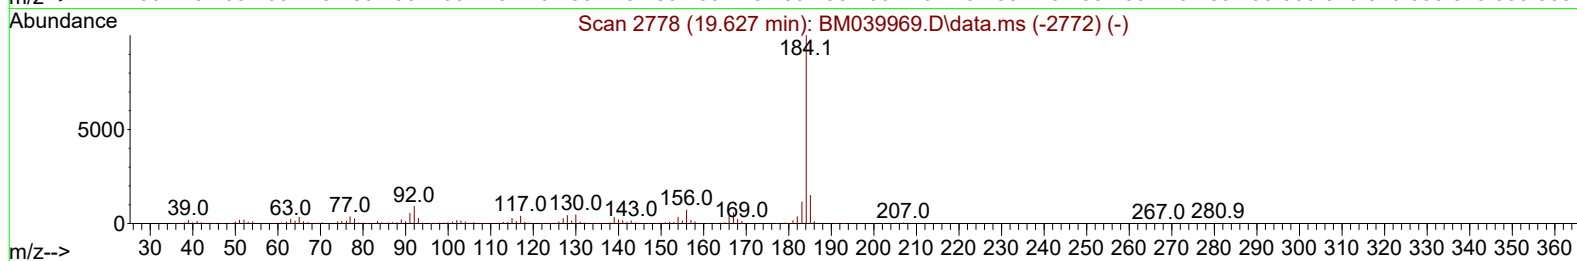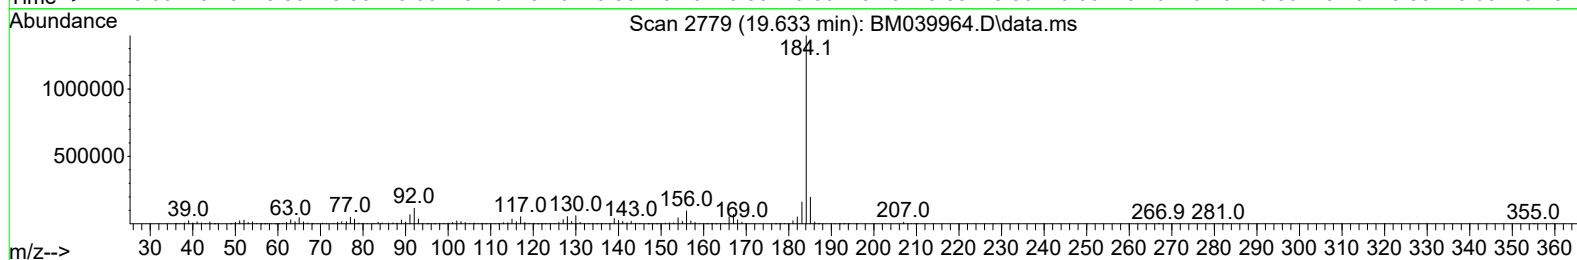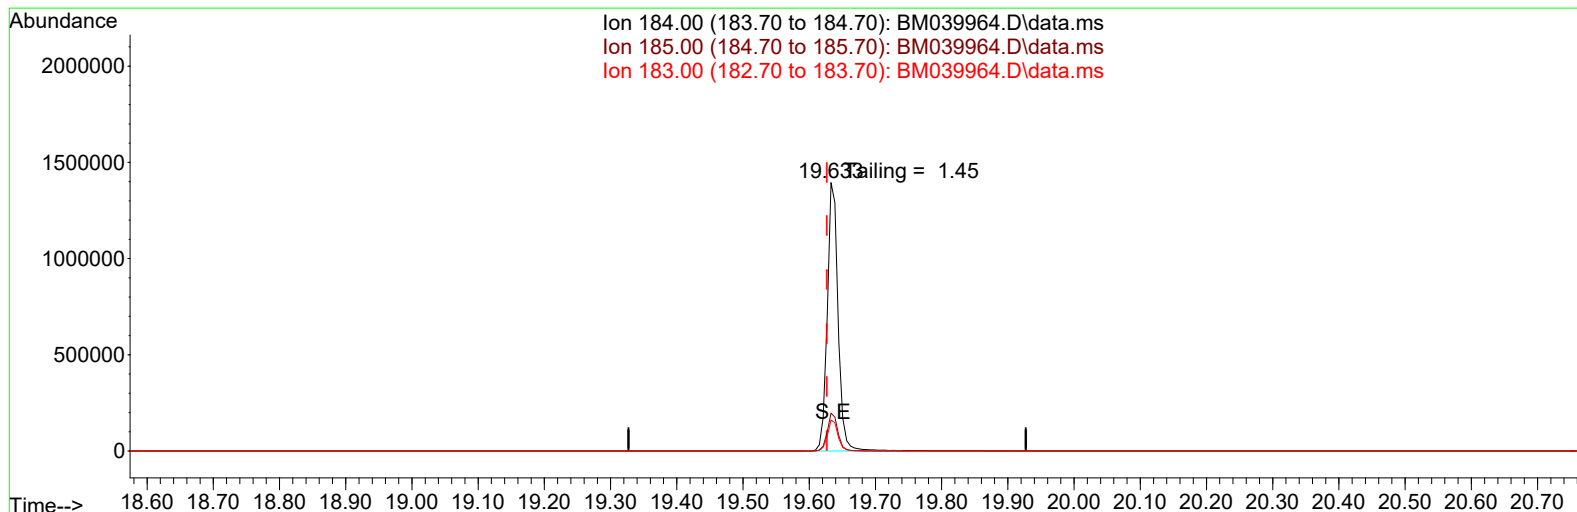

TIC: BM039964.D\data.ms

(77) Benzidine

19.633min (+ 0.006) 0.00 ng

response 1587306

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.16
183.00	11.50	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/23/2023	BNA_M	<u>BM039964.D</u>
Compound Name	Response	Retention Time
DDT	632995	20.868
DDD	3146	20.486
DDE	0	19.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3146	636141	0.49

Instrument :
BNA_M
ClientSampleId :
DFTPP