
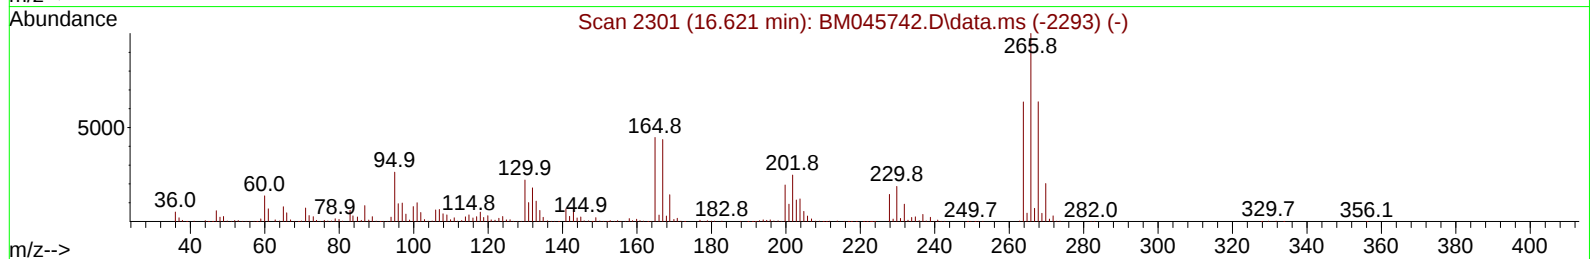
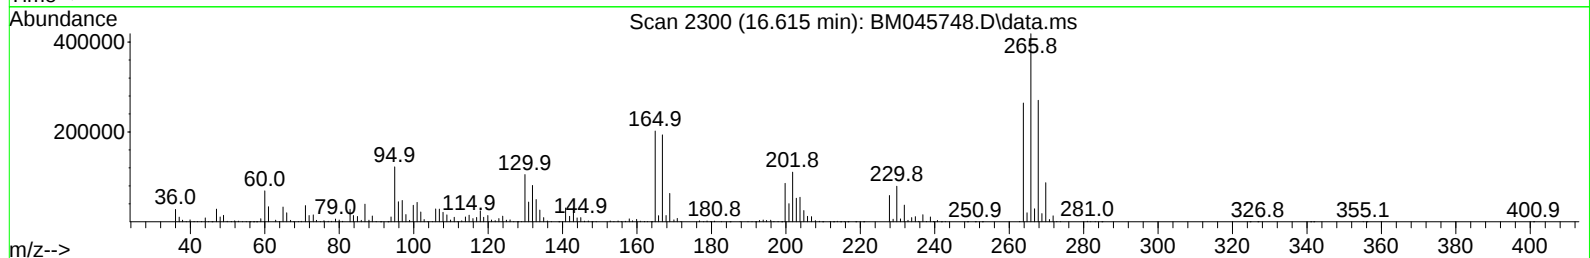


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045748.D
Acq On : 23 May 2024 09:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 04:16:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

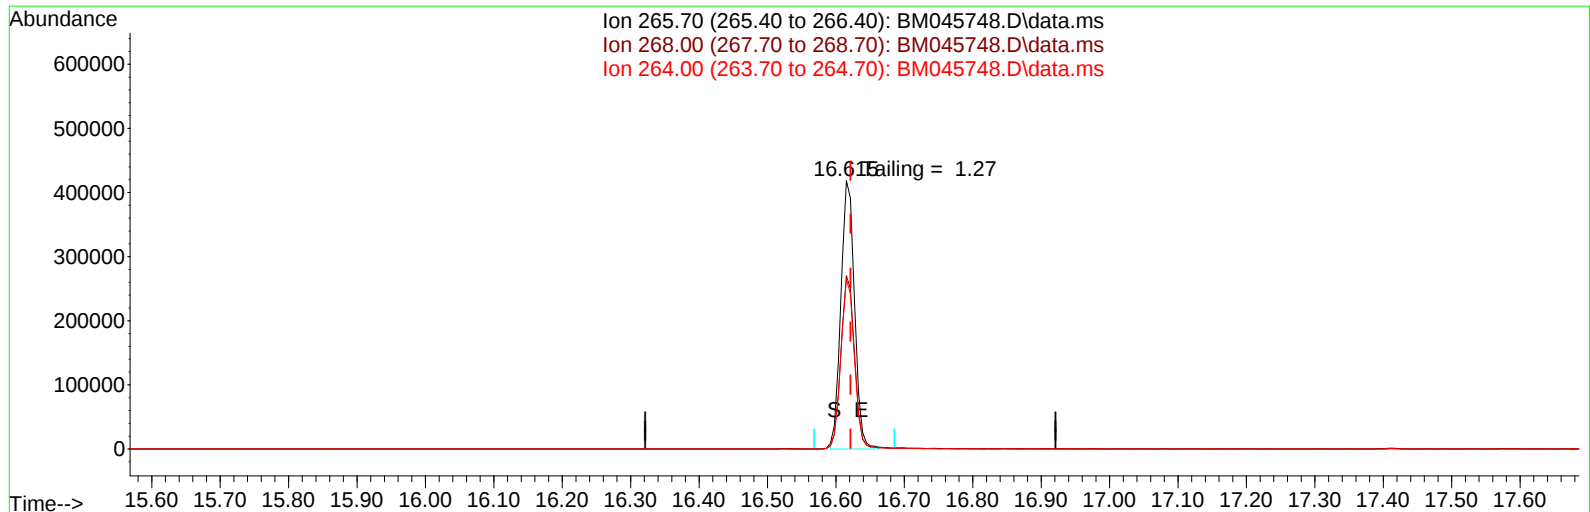

TIC: BM045748.D\data.ms

(70) Pentachlorophenol (C)




16.615min (-0.006) 183203.12 ng

response 585654

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.60
264.00	63.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045748.D
Acq On : 23 May 2024 09:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 04:16:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

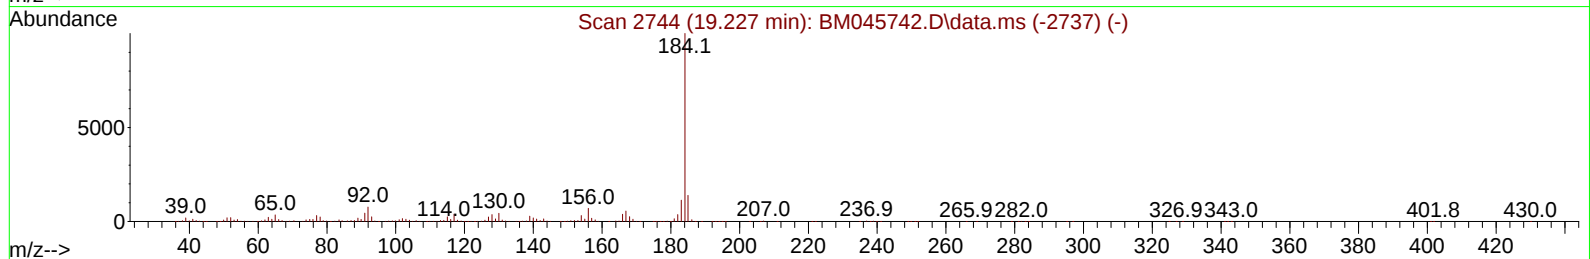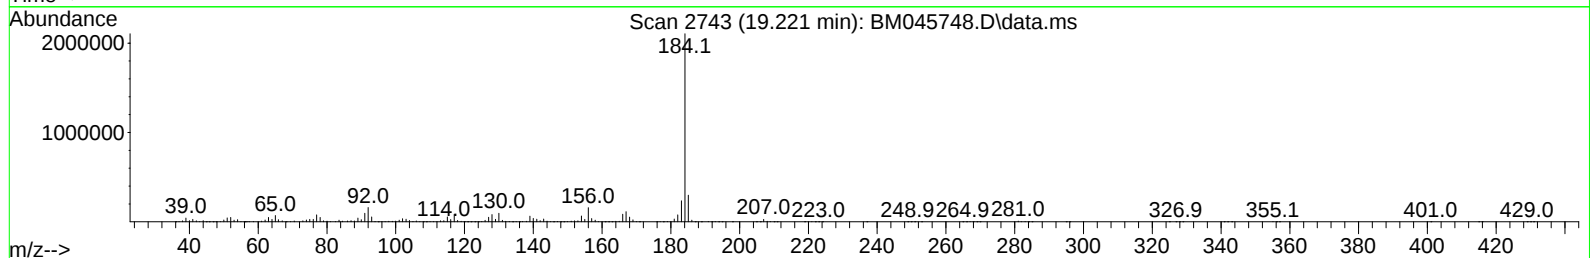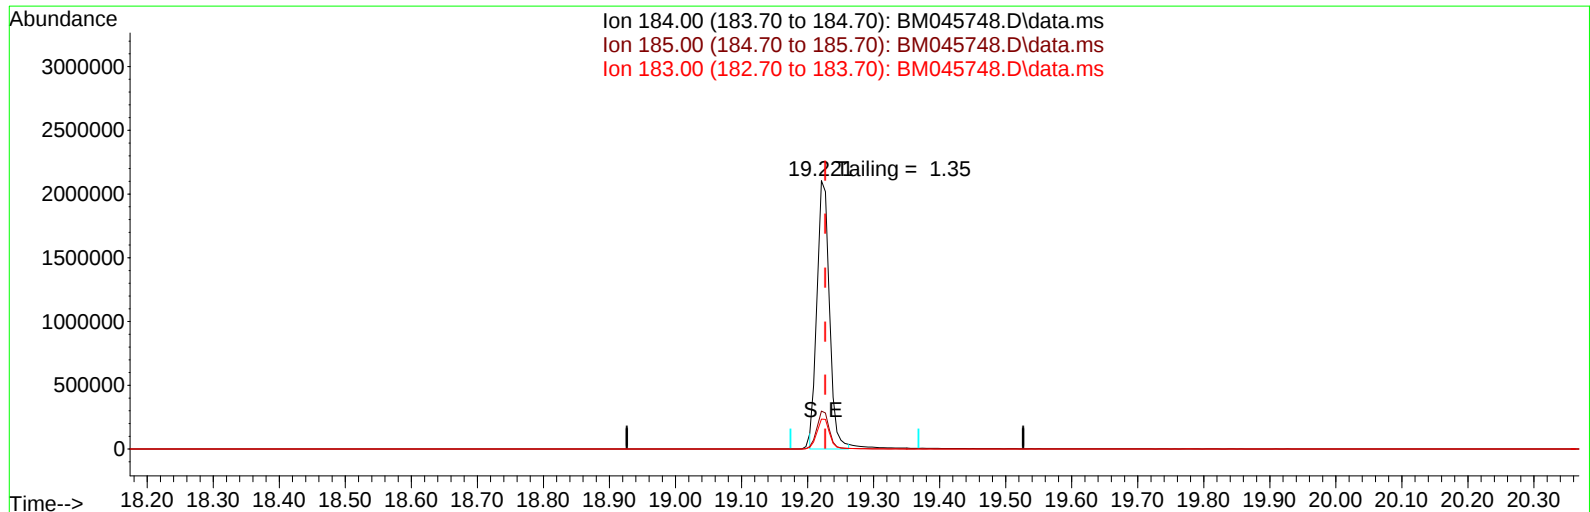

TIC: BM045748.D\data.ms

(77) Benzidine**19.221min (-0.006) 10005.33 ng****response 2874943**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.14
183.00	11.30	11.14
0.00	0.00	0.00