

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
 Data File : BM045757.D
 Acq On : 23 May 2024 17:33
 Operator : MA/JU
 Sample : P2464-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EFF-WW

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM045757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.781	282	288	305	rBV	2545701	4073691	3.21%	0.424%
2	5.246	362	367	379	rVB	2099715	3103837	2.45%	0.323%
3	6.846	631	639	648	rBV	1633758	2540120	2.00%	0.264%
4	7.563	754	761	769	rBV	1038876	1592673	1.26%	0.166%
5	7.681	769	781	822	rBV	24222086	53593446	42.23%	5.578%
6	8.728	945	959	974	rBV	3468694	6152108	4.85%	0.640%
7	9.145	995	1030	1033	rBV	3769237	21667242	17.07%	2.255%
8	10.334	1225	1232	1239	rVB	1437396	2391831	1.88%	0.249%
9	12.822	1647	1655	1668	rVB	8604142	12923984	10.18%	1.345%
10	13.904	1829	1839	1843	rBV2	1021691	1567540	1.24%	0.163%
11	14.192	1879	1888	1898	rVV	2018774	3420334	2.70%	0.356%
12	14.345	1910	1914	1920	rVB	1418125	1834340	1.45%	0.191%
13	14.698	1968	1974	1990	rBV	1060750	2122194	1.67%	0.221%
14	15.698	2138	2144	2152	rVB	5084085	7323519	5.77%	0.762%
15	16.139	2212	2219	2222	rBV	26949429	44558012	35.11%	4.638%
16	16.192	2222	2228	2232	rVV2	37193093	75880449	59.80%	7.898%
17	16.239	2232	2236	2247	rVB	32357914	49887034	39.31%	5.192%
18	16.451	2268	2272	2275	rBV	1907993	2858692	2.25%	0.298%
19	16.733	2317	2320	2326	rVB2	960909	1377995	1.09%	0.143%
20	16.939	2350	2355	2361	rBV	2297621	3205367	2.53%	0.334%
21	17.627	2467	2472	2478	rVB	2262263	2825346	2.23%	0.294%
22	17.804	2494	2502	2504	rVV	3428872	6206425	4.89%	0.646%
23	17.827	2504	2506	2510	rVV	2285659	2501940	1.97%	0.260%
24	17.880	2510	2515	2520	rVV	1683072	2844929	2.24%	0.296%
25	17.927	2520	2523	2538	rVB	850357	1751414	1.38%	0.182%
26	18.086	2545	2550	2555	rBV	13673762	17655145	13.91%	1.838%
27	18.239	2571	2576	2579	rBV2	1218595	1612468	1.27%	0.168%
28	18.280	2579	2583	2588	rVB	6131713	7034763	5.54%	0.732%
29	18.339	2588	2593	2598	rBV	3729458	5443699	4.29%	0.567%
30	18.809	2663	2673	2676	rVV2	18808659	29876150	23.54%	3.110%
31	18.833	2676	2677	2686	rVB2	1758707	2197151	1.73%	0.229%
32	18.945	2691	2696	2700	rVB	19968758	25269112	19.91%	2.630%
33	19.062	2710	2716	2722	rBV2	834601	1539948	1.21%	0.160%
34	19.127	2722	2727	2730	rVV	1494290	2757778	2.17%	0.287%
35	19.168	2730	2734	2735	rVV	10383869	12734758	10.04%	1.325%
36	19.209	2735	2741	2756	rVV3	36631518	106955260	84.29%	11.132%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045757.D
Acq On : 23 May 2024 17:33
Operator : MA/JU
Sample : P2464-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EFF-WW

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.345	2756	2764	2777	rVV4	36504269	126896366	100.00%	13.208%
38	19.486	2777	2788	2792	rVV3	31311573	50152461	39.52%	5.220%
39	19.521	2792	2794	2798	rVV	1629138	1700033	1.34%	0.177%
40	19.586	2800	2805	2813	rVV2	12189362	19127507	15.07%	1.991%
41	19.692	2819	2823	2826	rVV	2153693	2634554	2.08%	0.274%
42	19.733	2826	2830	2837	rVB2	1682654	2203947	1.74%	0.229%
43	19.845	2846	2849	2855	rBV3	1526630	2393983	1.89%	0.249%
44	19.903	2855	2859	2862	rVB	3556625	3879113	3.06%	0.404%
45	20.033	2877	2881	2886	rBV	8522380	10006587	7.89%	1.042%
46	20.156	2897	2902	2904	rBV3	1024312	1560409	1.23%	0.162%
47	20.262	2913	2920	2922	rBV2	3505383	5830294	4.59%	0.607%
48	20.362	2933	2937	2940	rBV	7458865	8403694	6.62%	0.875%
49	20.392	2940	2942	2949	rVB	1783527	1963775	1.55%	0.204%
50	20.492	2955	2959	2962	rBV	2612663	3397983	2.68%	0.354%
51	20.545	2962	2968	2972	rVV	7272516	10474030	8.25%	1.090%
52	20.586	2972	2975	2982	rVV	6472318	8126890	6.40%	0.846%
53	20.680	2984	2991	3007	rVB	11069556	19162715	15.10%	1.994%
54	20.868	3018	3023	3031	rVB	12399318	14675824	11.57%	1.527%
55	21.039	3048	3052	3057	rBV	6168432	7294886	5.75%	0.759%
56	21.156	3068	3072	3076	rVB2	2218178	3043024	2.40%	0.317%
57	21.315	3095	3099	3108	rVB4	1117130	2118693	1.67%	0.221%
58	21.633	3149	3153	3163	rVB	1009156	1761829	1.39%	0.183%
59	21.774	3172	3177	3182	rVV	6799867	9411081	7.42%	0.980%
60	21.821	3182	3185	3191	rVV2	924018	1585707	1.25%	0.165%
61	21.892	3191	3197	3204	rVB	12855246	19318247	15.22%	2.011%
62	22.286	3260	3264	3269	rBV2	975329	1728682	1.36%	0.180%
63	23.115	3400	3405	3411	rBV2	1639574	2820040	2.22%	0.294%
64	23.239	3418	3426	3447	rVB	20241469	47709244	37.60%	4.966%
65	23.691	3496	3503	3511	rBV	4292815	8709129	6.86%	0.906%
66	23.950	3540	3547	3556	rVB	1766235	3964026	3.12%	0.413%
67	25.856	3863	3871	3883	rVB2	2588159	7760685	6.12%	0.808%
68	32.350	4962	4975	4999	rVB2	3327167	19687934	15.51%	2.049%


Sum of corrected areas: 960784066

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045757.D
Acq On : 23 May 2024 17:33
Operator : MA/JU
Sample : P2464-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EFF-WW

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

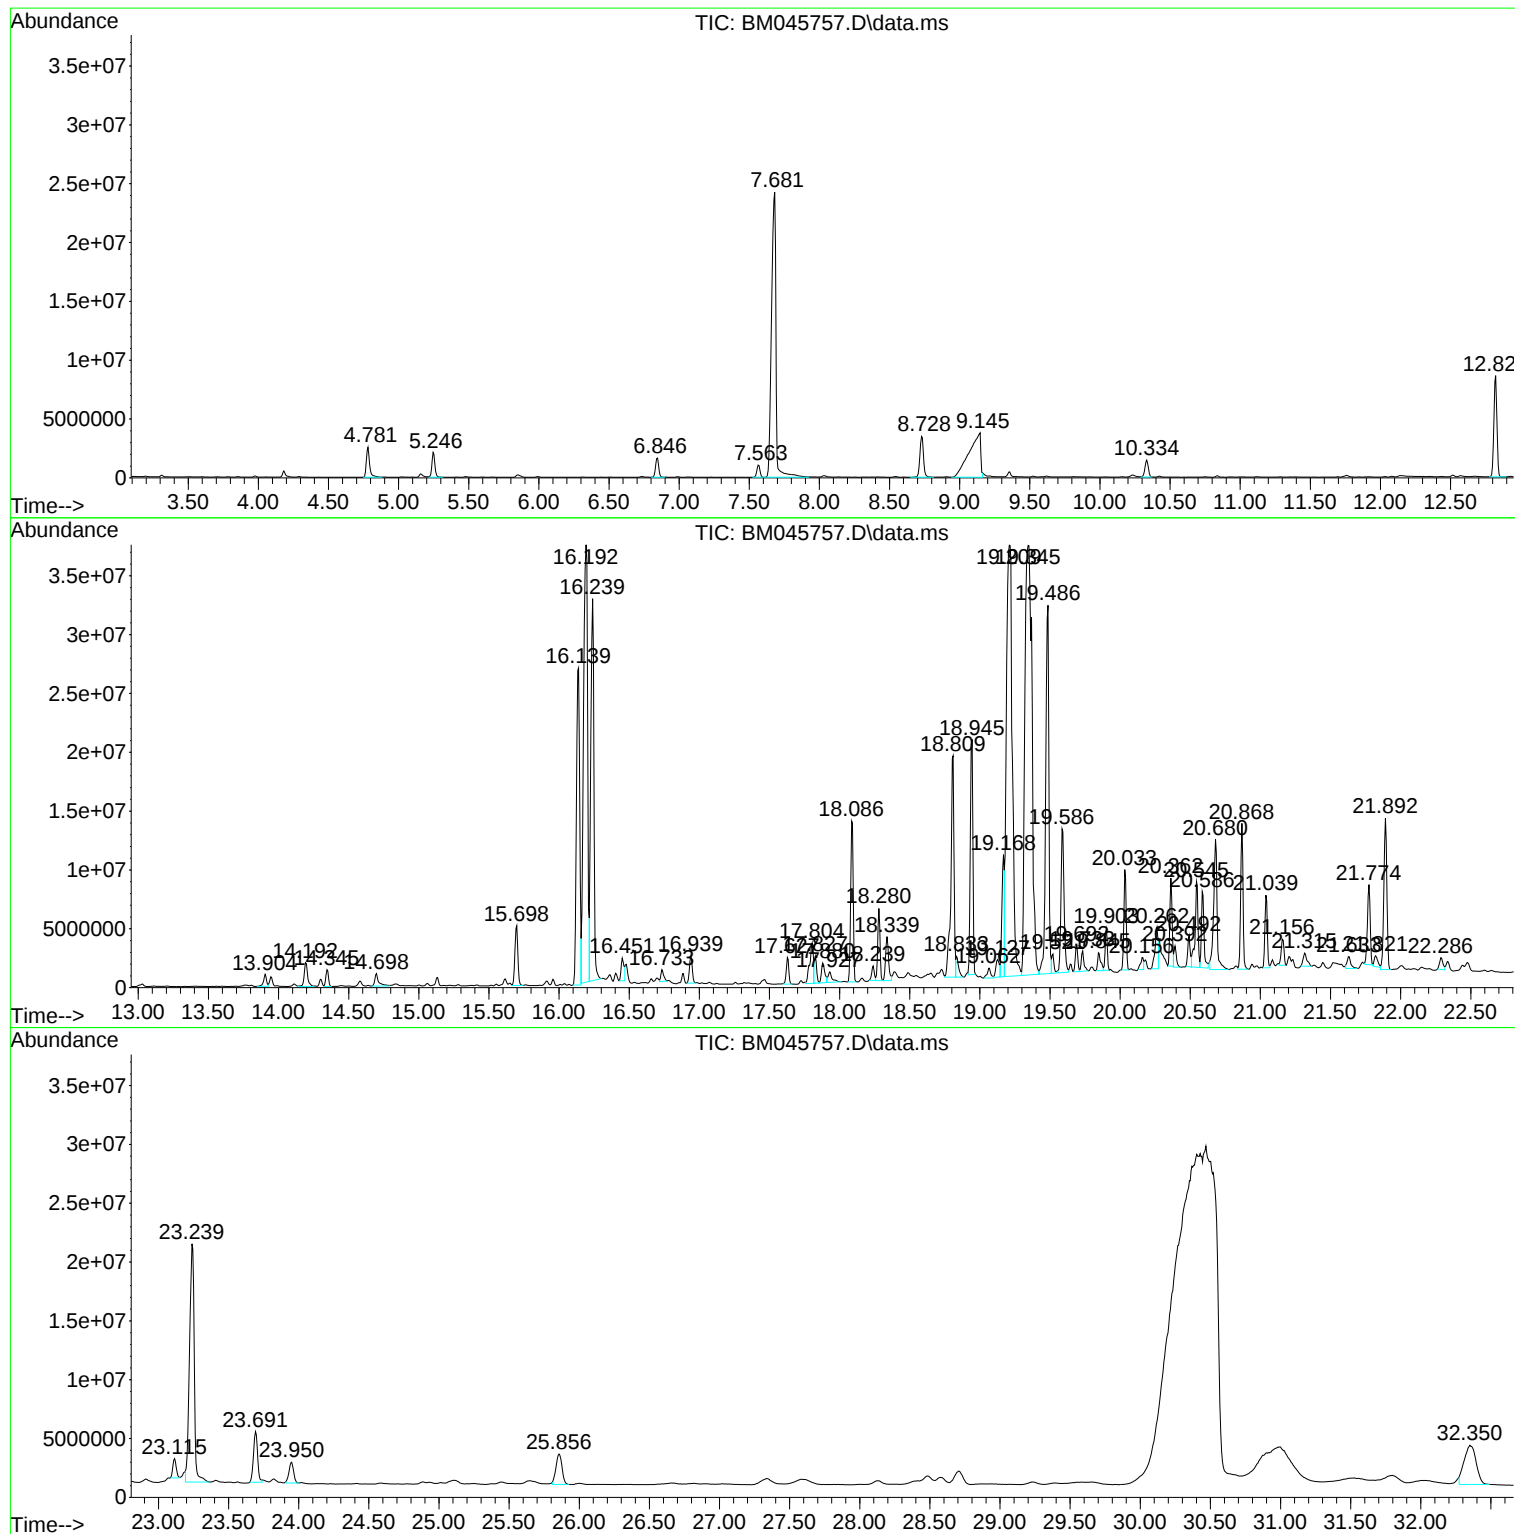

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045757.D
Acq On : 23 May 2024 17:33
Operator : MA/JU
Sample : P2464-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EFF-WW

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045757.D
Acq On : 23 May 2024 17:33
Operator : MA/JU
Sample : P2464-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EFF-WW

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------