


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045748.D
Acq On : 23 May 2024 09:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 23 04:12:56 2024

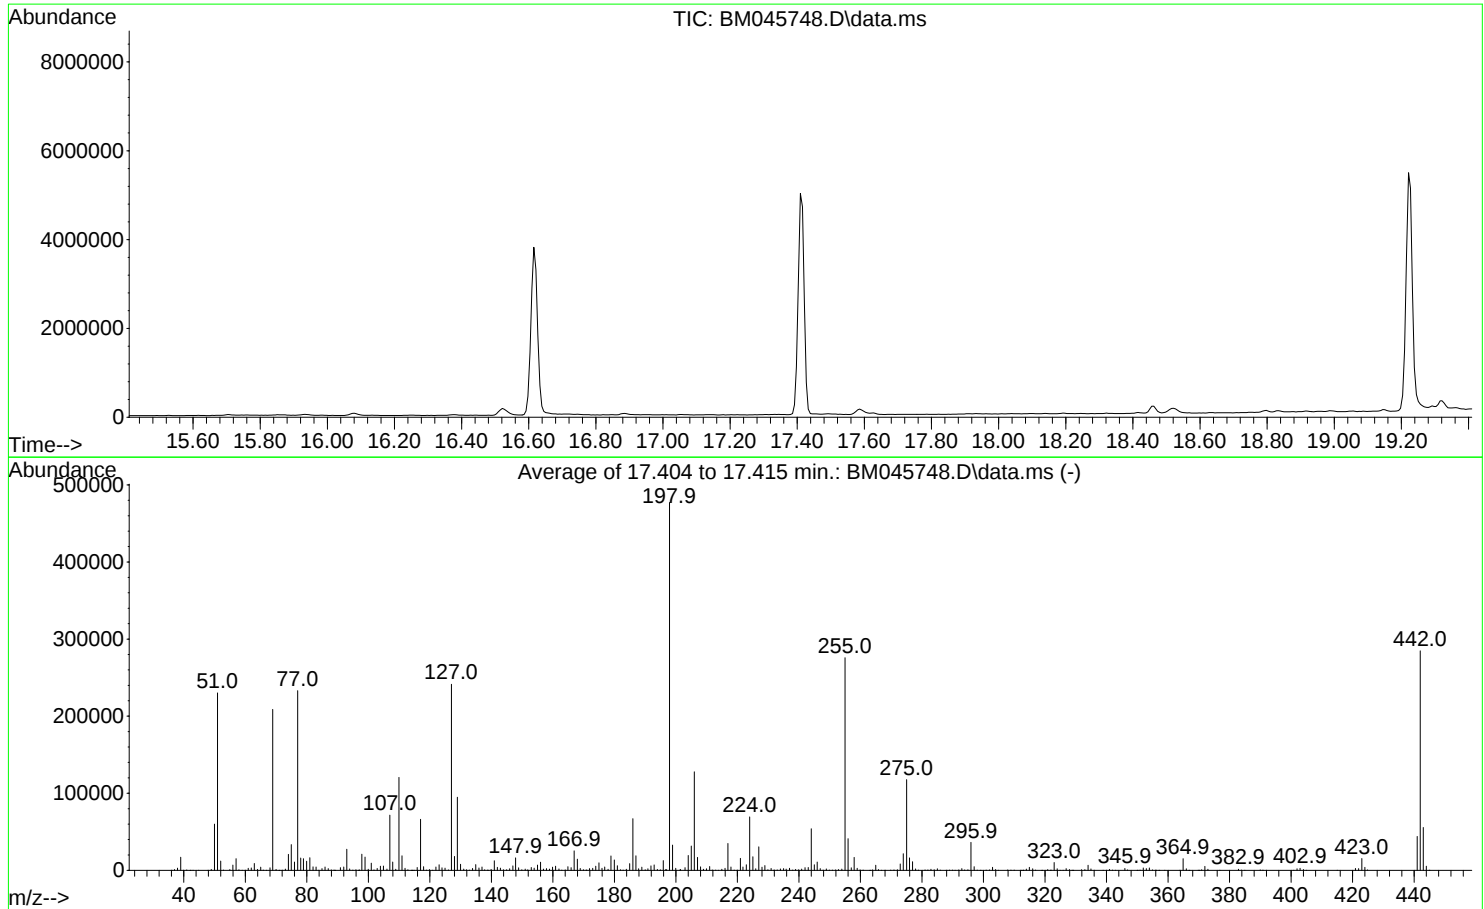

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2427

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	230210	PASS
68	69	0.00	2	1.5	3234	PASS
69	198	0.00	100	43.7	208756	PASS
70	69	0.00	2	0.6	1244	PASS
127	198	10	80	50.6	241323	PASS
197	198	0.00	2	0.3	1222	PASS
198	198	100	100	100.0	477163	PASS
199	198	5	9	6.9	32731	PASS
275	198	10	60	24.7	117651	PASS
365	198	1	100	3.2	15100	PASS
441	198	0.01	100	9.2	44107	PASS
442	442	50	100	100.0	284779	PASS
443	442	15	24	19.5	55643	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/23/2024	BNA_M	<u>BM045748.D</u>
Compound Name	Response	Retention Time
DDT	1809142	20.439
DDD	29046	20.056
DDE	2737	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31783	1840925	1.73

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
 Data File : BM045748.D
 Acq On : 23 May 2024 09:50
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 24 04:16:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 23 04:12:56 2024
 Response via : Initial Calibration

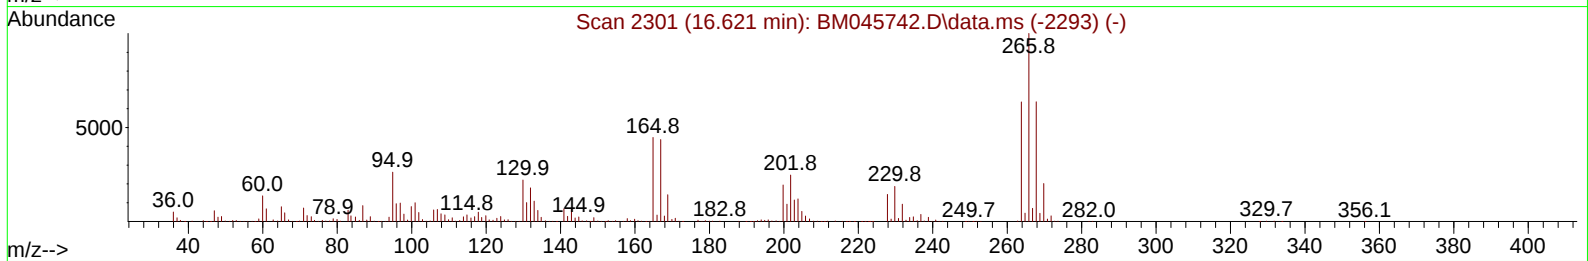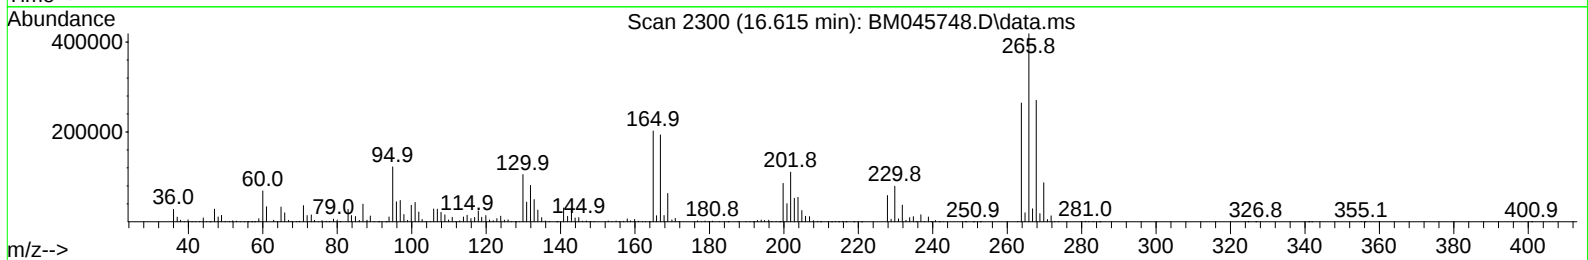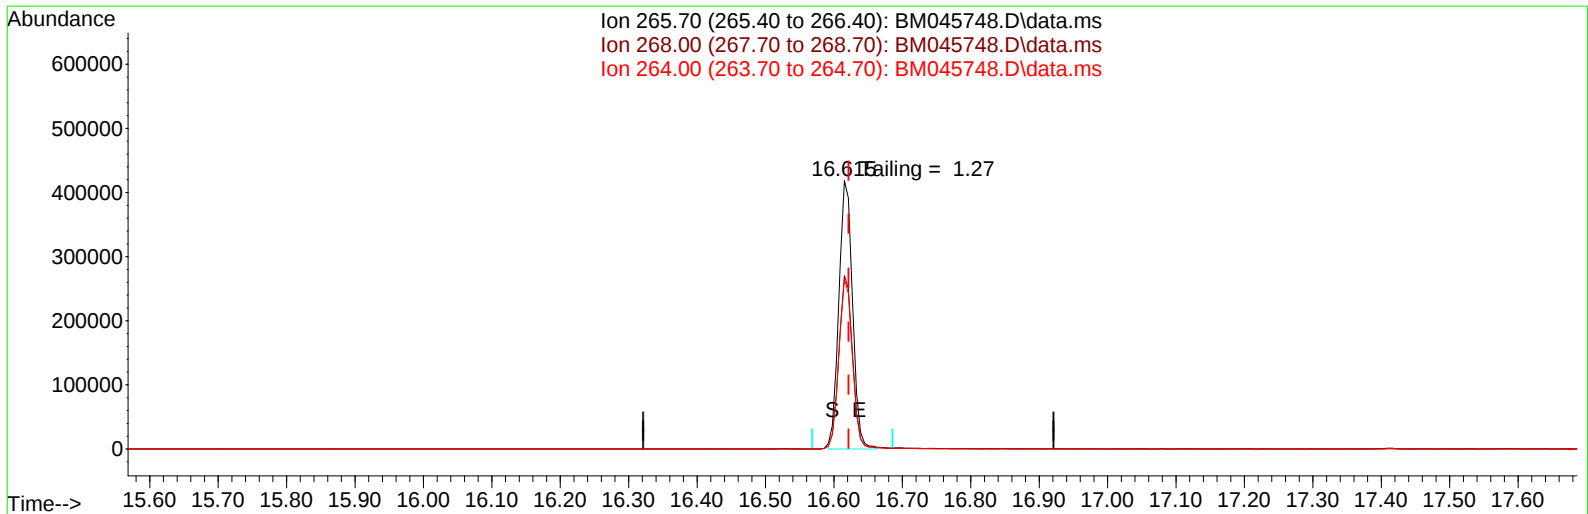

TIC: BM045748.D\data.ms

(70) Pentachlorophenol (C)

16.615min (-0.006) 183203.12 ng




response 585654

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.60
264.00	63.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052324\
Data File : BM045748.D
Acq On : 23 May 2024 09:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 24 04:16:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

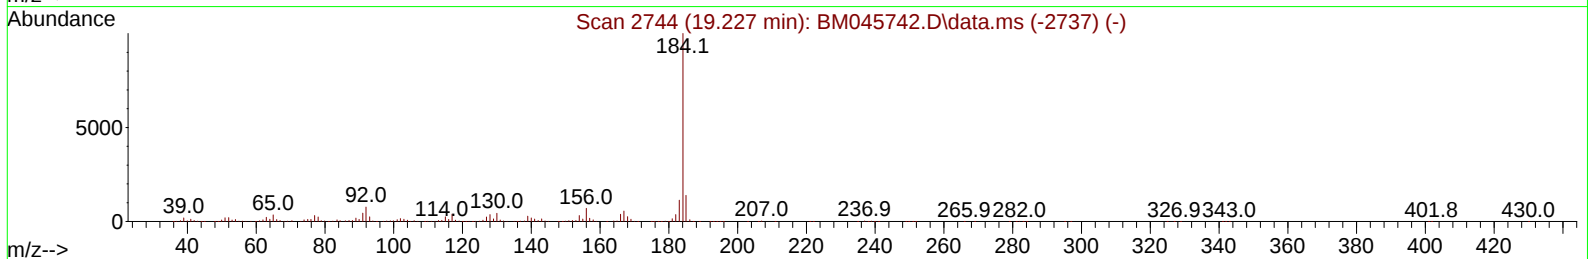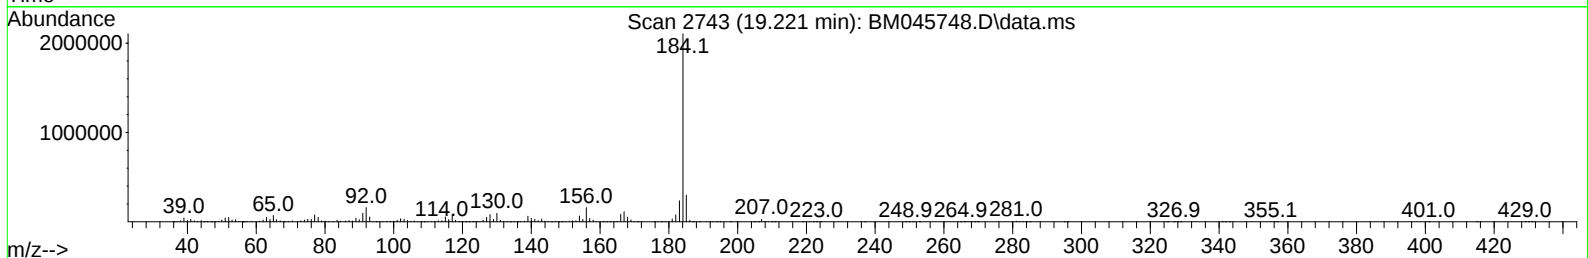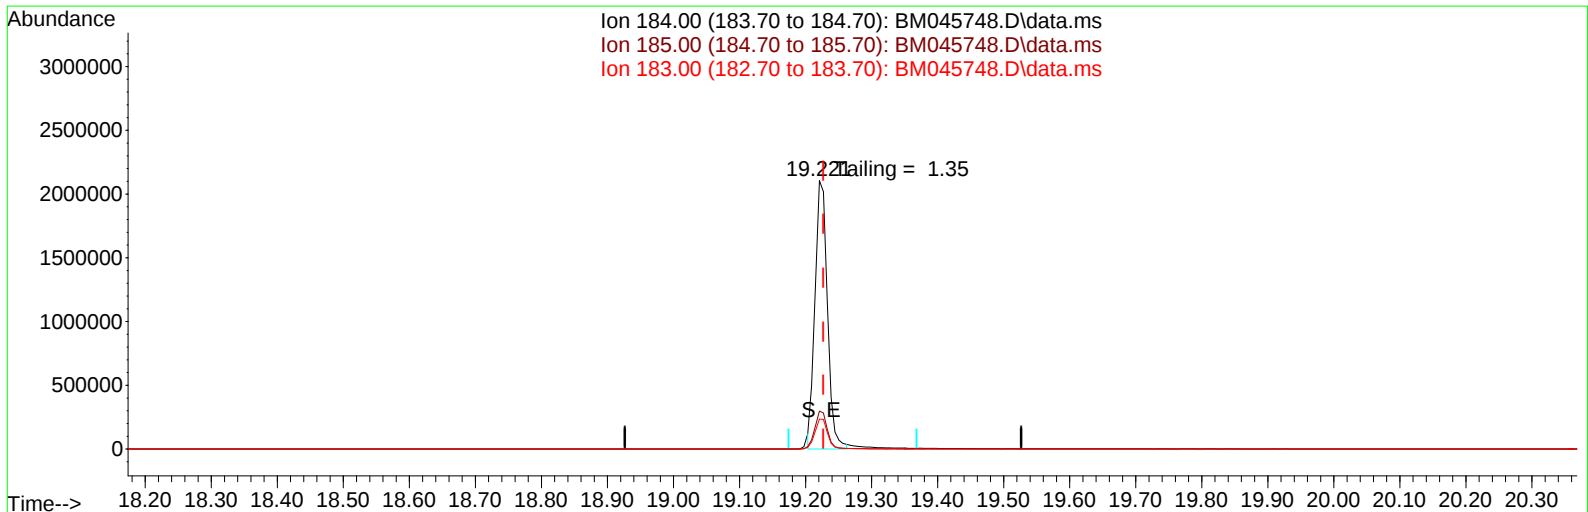

TIC: BM045748.D\data.ms

(77) Benzidine

19.221min (-0.006) 10005.33 ng

response 2874943

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.14
183.00	11.30	11.14
0.00	0.00	0.00