
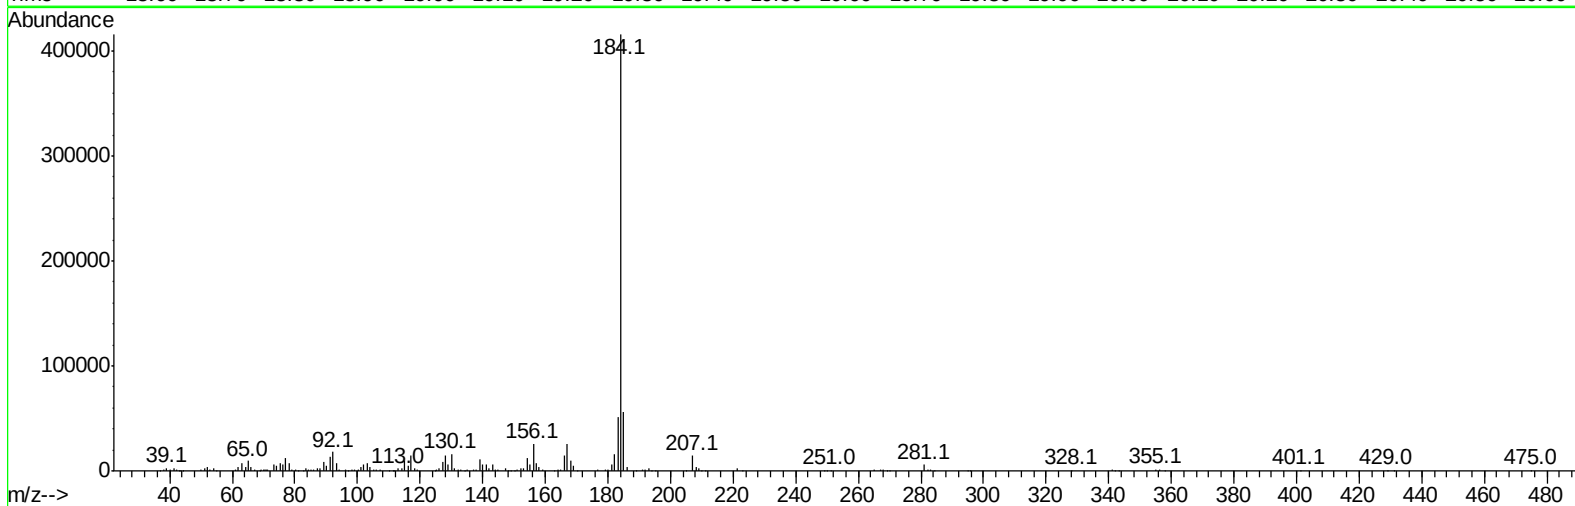


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052417\
Data File : BM010171.D
Acq On : 24 May 2017 09:25
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 07:56:58 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

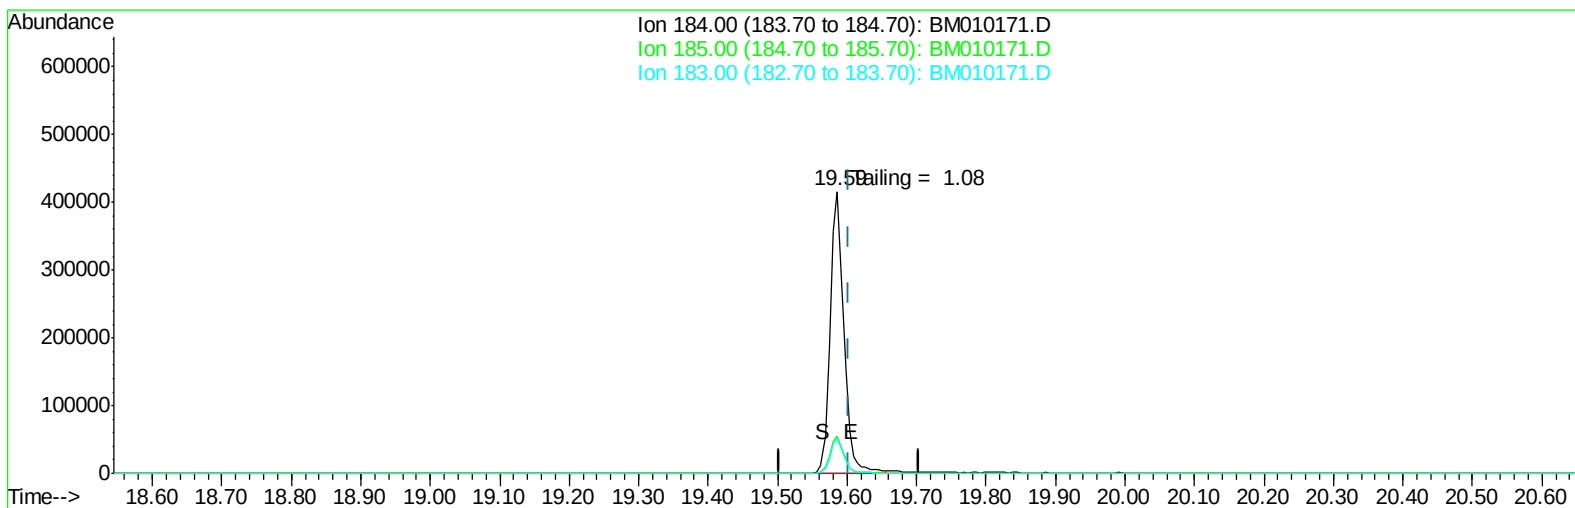

TIC: BM010171.D

(76) Benzidine



19.586min (-0.018) 13257.21ng

response 573661

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.38
183.00	11.10	12.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052417\
Data File : BM010171.D
Acq On : 24 May 2017 09:25
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 07:56:58 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

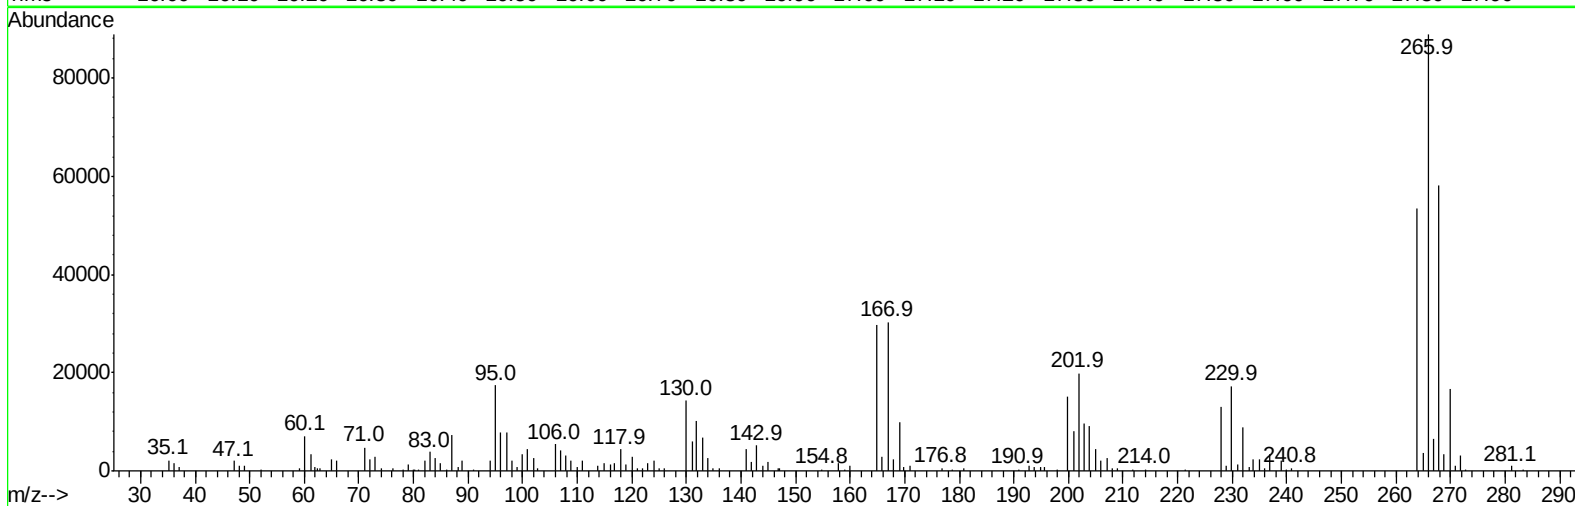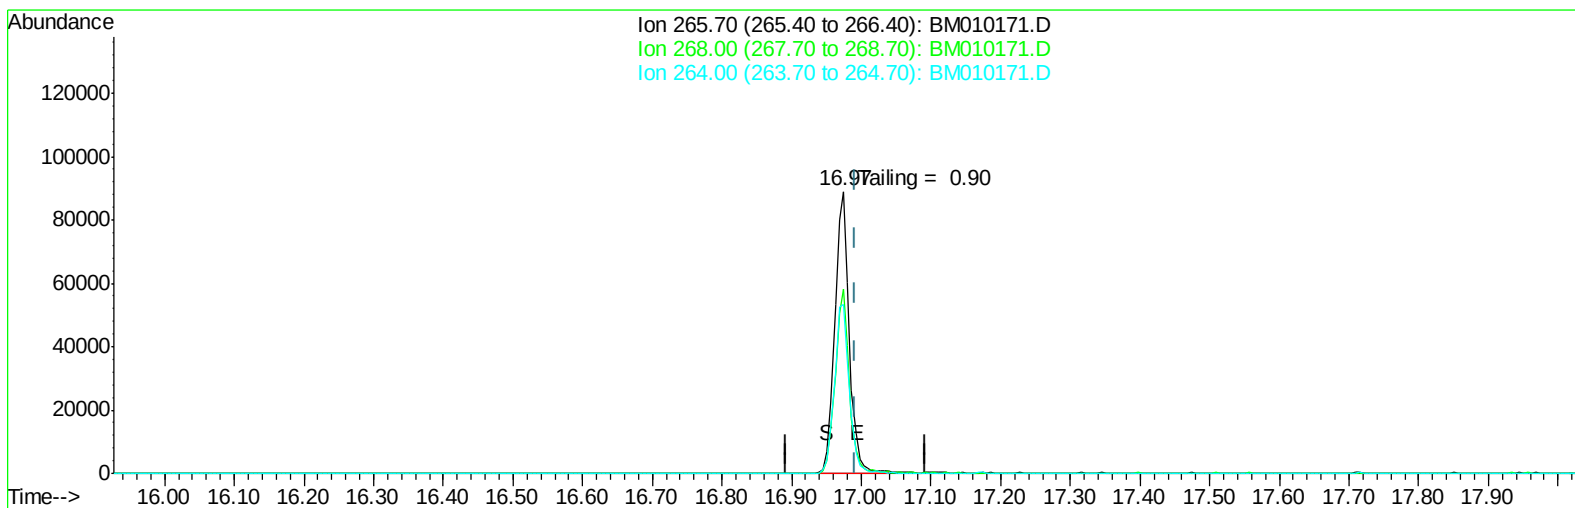

TIC: BM010171.D

(69) Pentachlorophenol (C)

16.974min (-0.018) 0.00ng

response 128334

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.36
264.00	61.20	60.01
0.00	0.00	0.00