
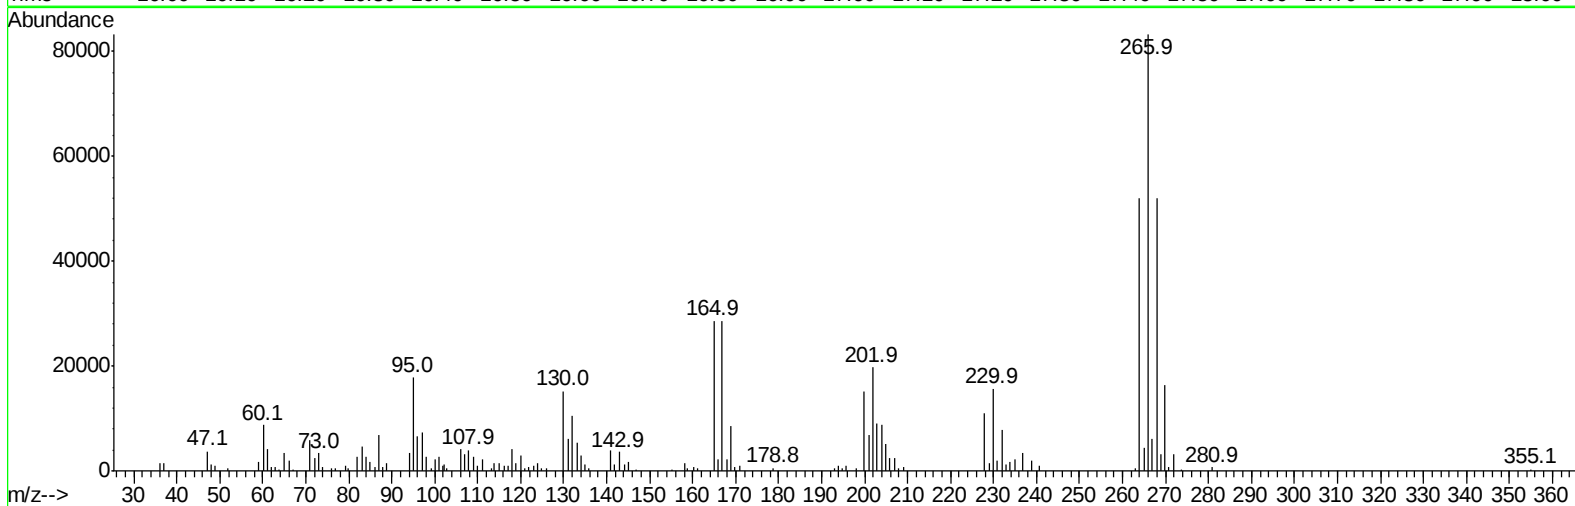


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052417\
Data File : BM010191.D
Acq On : 24 May 2017 22:50
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 08:01:09 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

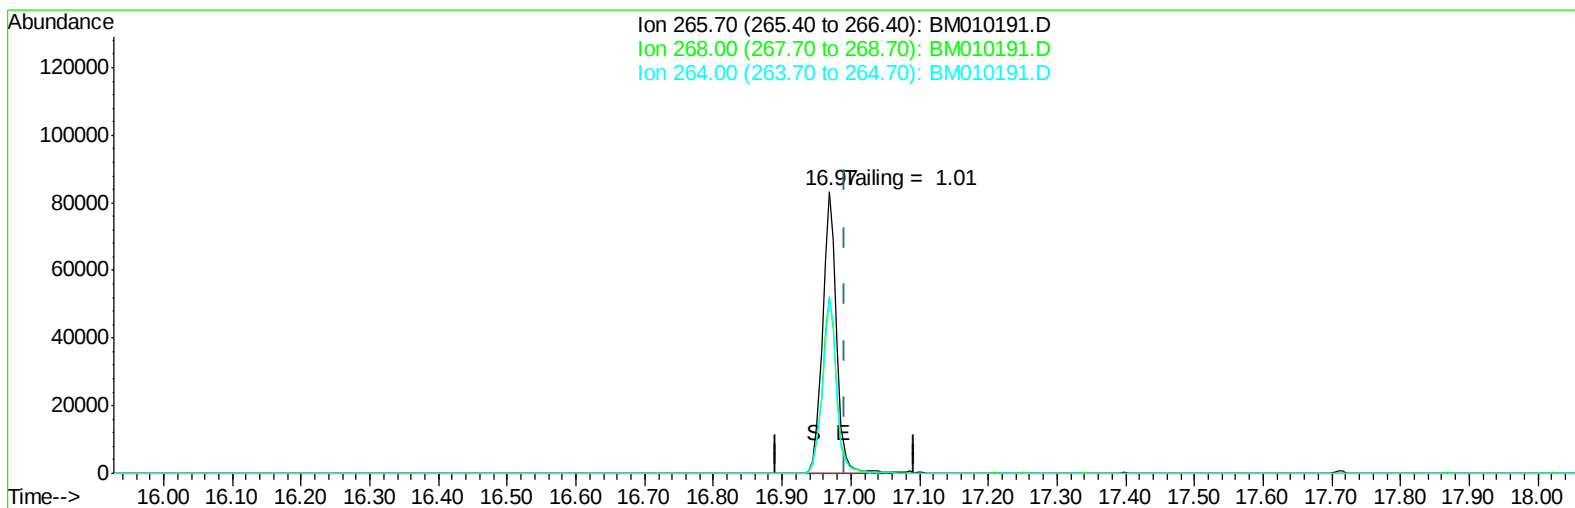

TIC: BM010191.D

(69) Pentachlorophenol (C)



16.968min (-0.024) 0.00ng

response 118873

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.60
264.00	61.20	62.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM052417\
Data File : BM010191.D
Acq On : 24 May 2017 22:50
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 08:01:09 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

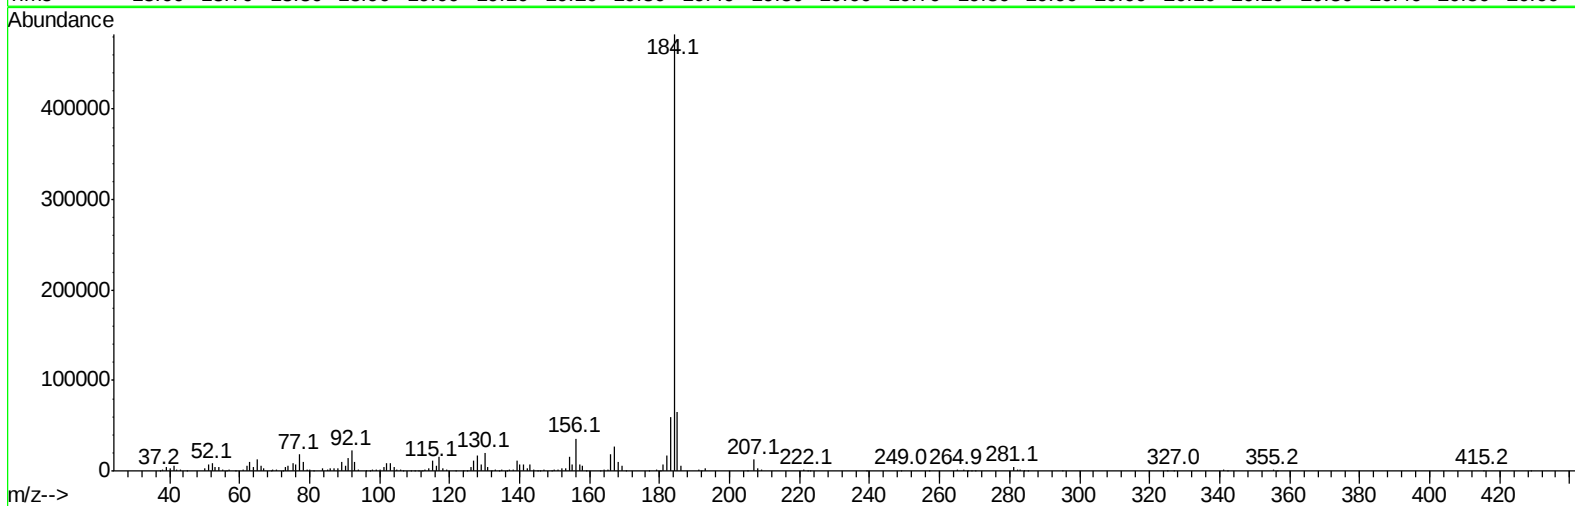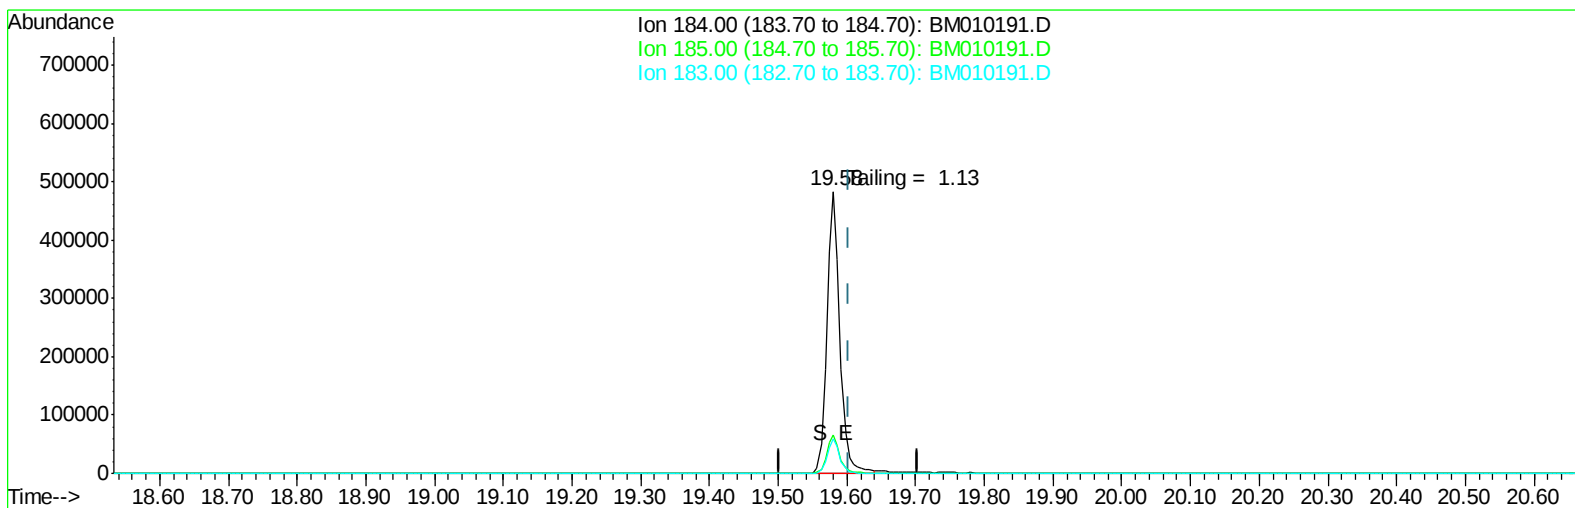

TIC: BM010191.D

(76) Benzidine

19.580min (-0.024) 39671.49ng

response 637341

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.47
183.00	11.10	12.24
0.00	0.00	0.00