


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052417\
 Data File : BM010171.D
 Acq On : 24 May 2017 09:25
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

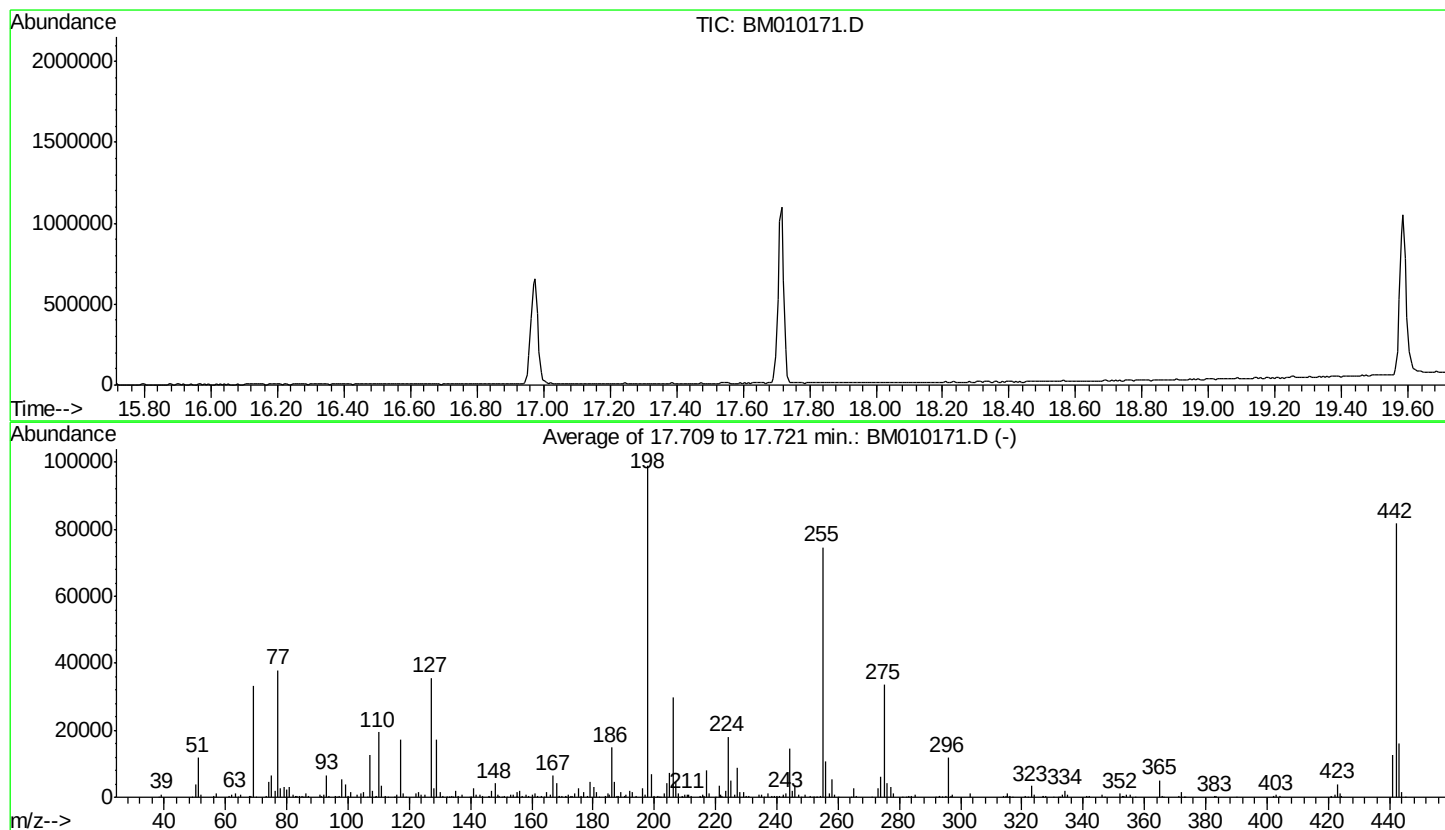

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	11.9	11772	PASS
68	69	0.00	2	1.1	352	PASS
69	198	0.00	100	33.6	33232	PASS
70	69	0.00	2	0.3	107	PASS
127	198	10	80	36.0	35616	PASS
197	198	0.00	2	0.6	606	PASS
198	198	100	100	100.0	99024	PASS
199	198	5	9	7.0	6976	PASS
275	198	10	60	33.9	33522	PASS
365	198	1	100	5.0	5000	PASS
441	442	0.01	24	15.6	12790	PASS
442	198	50	100	82.6	81760	PASS
443	442	15	24	19.6	16048	PASS