

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
 Data File : BM039980.D
 Acq On : 24 May 2023 12:36
 Operator : CG/JU
 Sample : PB152902BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB152902BL

Quant Time: May 24 13:18:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 01:06:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	255798	20.000	ng	0.00
21) Naphthalene-d8	10.834	136	962495	20.000	ng	0.00
39) Acenaphthene-d10	14.651	164	458944	20.000	ng	0.00
64) Phenanthrene-d10	17.392	188	841612	20.000	ng	0.00
76) Chrysene-d12	21.568	240	597104	20.000	ng	0.00
86) Perylene-d12	24.021	264	708376	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.563	112	1681160	100.814	ng	0.00
7) Phenol-d6	7.169	99	1975861	90.830	ng	0.00
23) Nitrobenzene-d5	9.187	82	1662407	93.199	ng	0.00
42) 2,4,6-Tribromophenol	16.133	330	474811	79.710	ng	0.00
45) 2-Fluorobiphenyl	13.280	172	3850538	98.959	ng	0.00
79) Terphenyl-d14	20.009	244	5085910	132.253	ng	0.00
Target Compounds						
						Qvalue
74) Di-n-butylphthalate	18.357	149	147	3.664	ng	# 78
80) Butylbenzylphthalate	20.674	149	236	4.844	ng	# 20
84) Bis(2-ethylhexyl)phtha...	21.480	149	526	3.619	ng	# 53
85) Di-n-octyl phthalate	22.433	149	183	6.617	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
Data File : BM039980.D
Acq On : 24 May 2023 12:36
Operator : CG/JU
Sample : PB152902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB152902BL

Quant Time: May 24 13:18:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 01:06:13 2023
Response via : Initial Calibration




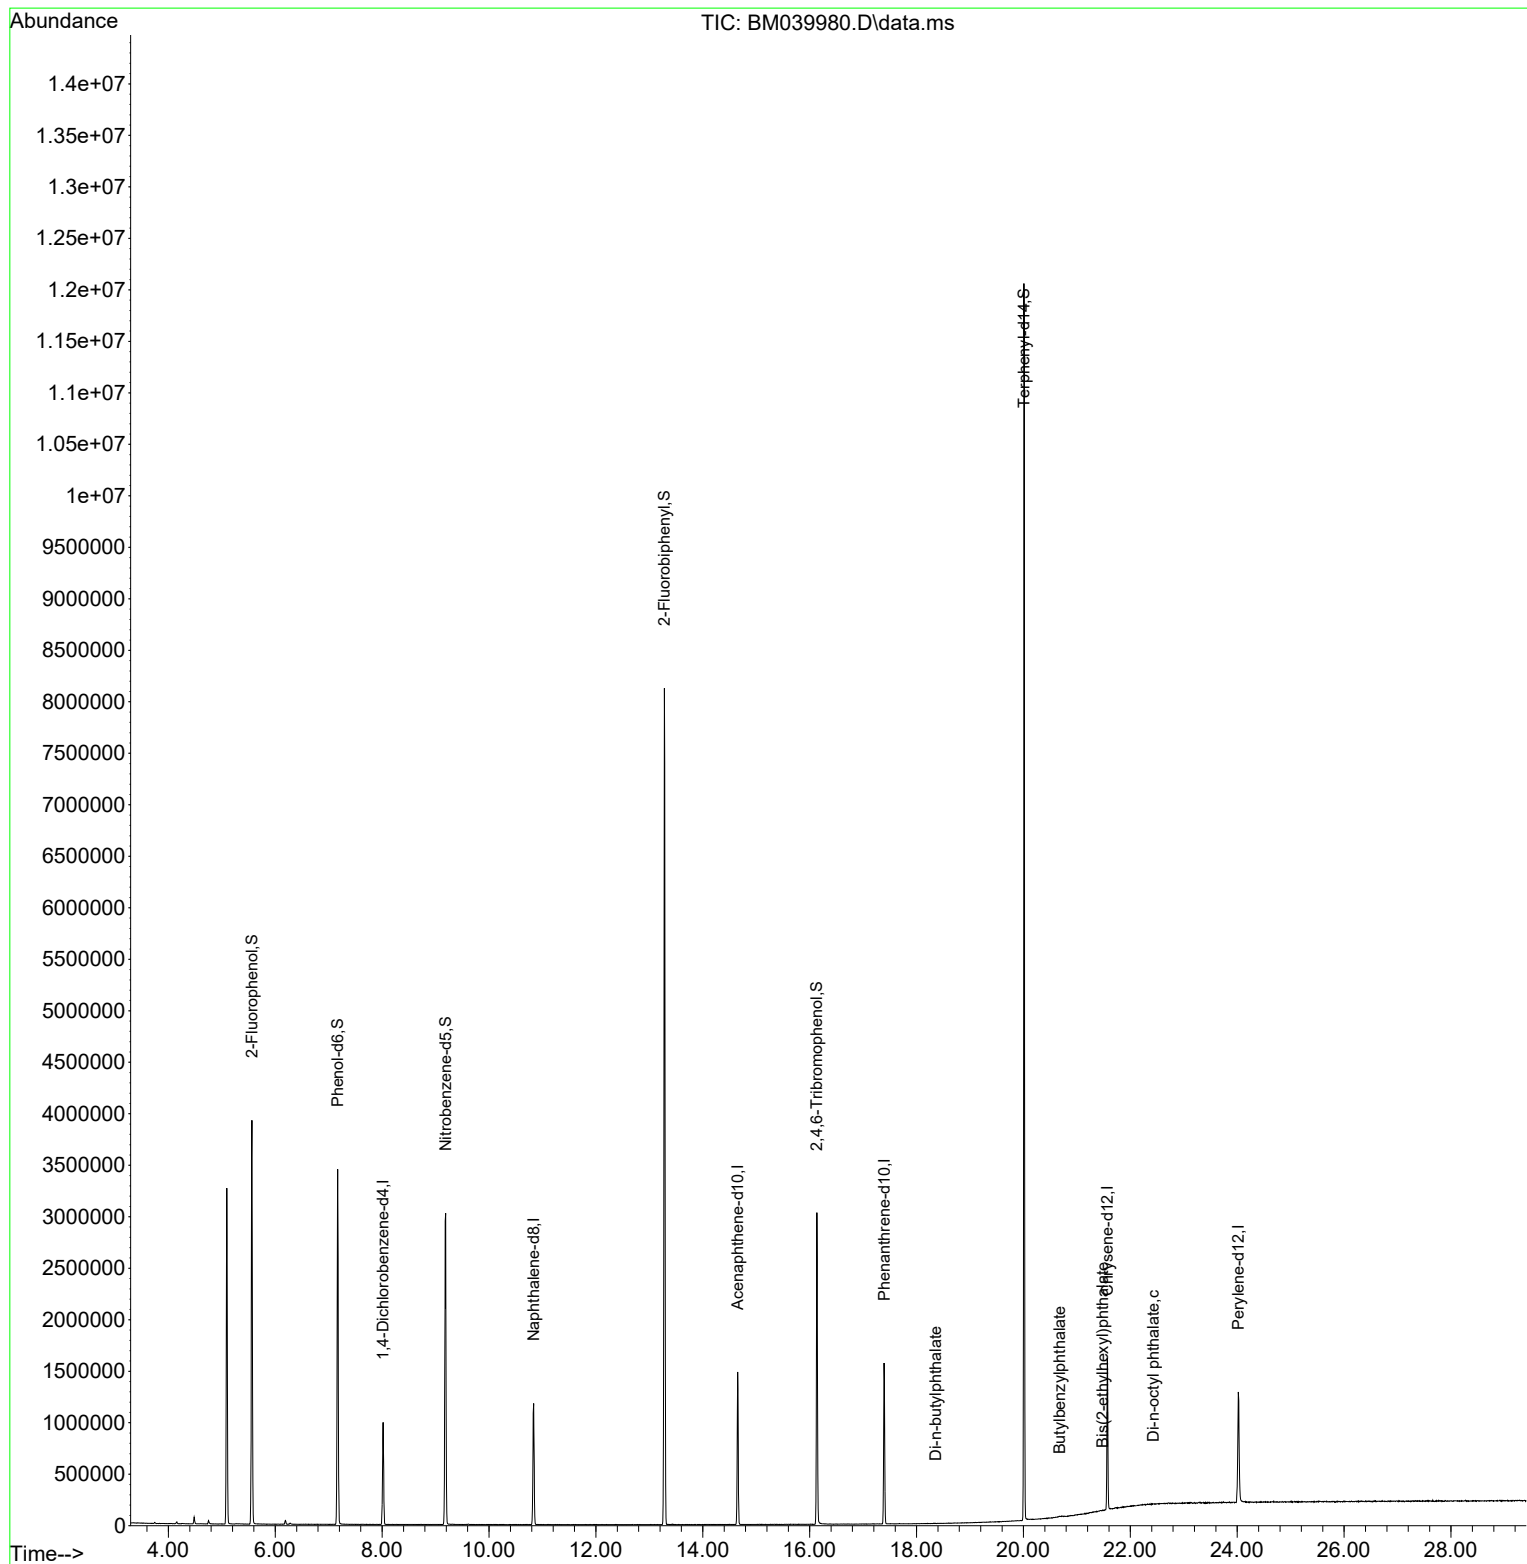


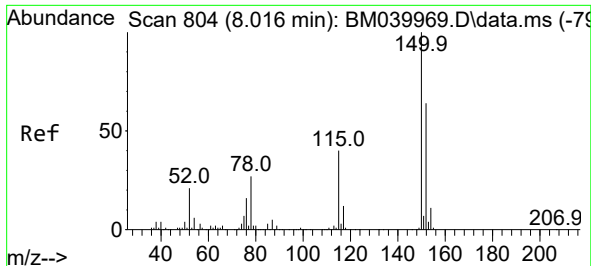

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.016 min Scan# 804
Delta R.T. 0.000 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36




Instrument :
BNA_M
ClientSampleId :
PB152902BL


Tgt Ion:152 Resp: 255798
Ion Ratio Lower Upper
152 100
150 158.4 125.5 188.3
115 60.7 50.2 75.2

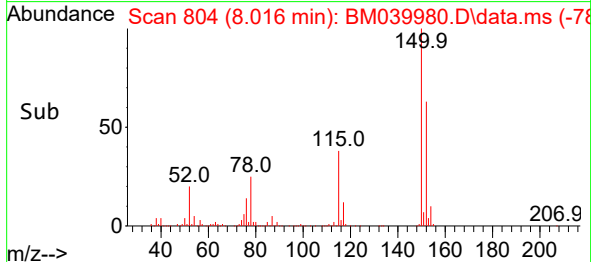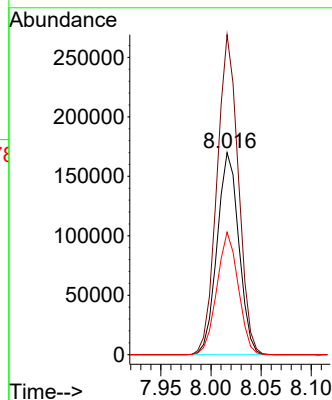

#5
2-Fluorophenol
Concen: 100.814 ng
RT: 5.563 min Scan# 387
Delta R.T. 0.000 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36

Tgt Ion:112 Resp: 1681160
Ion Ratio Lower Upper
112 100
64 52.3 43.0 64.4
63 27.3 22.9 34.3

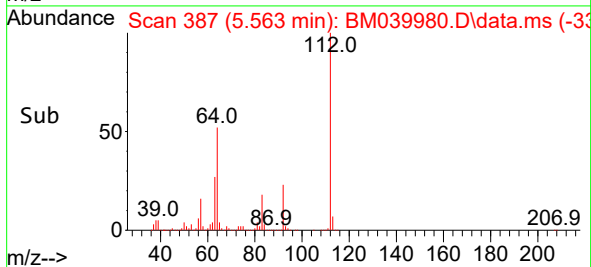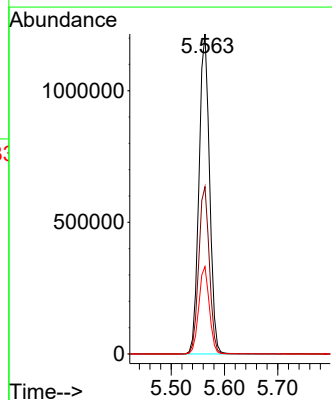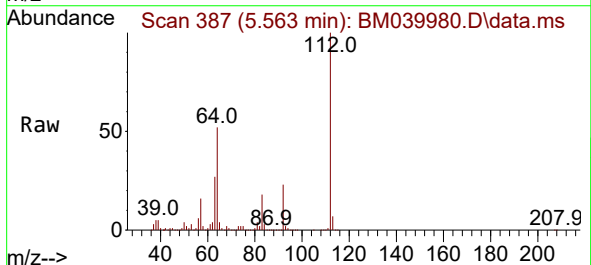




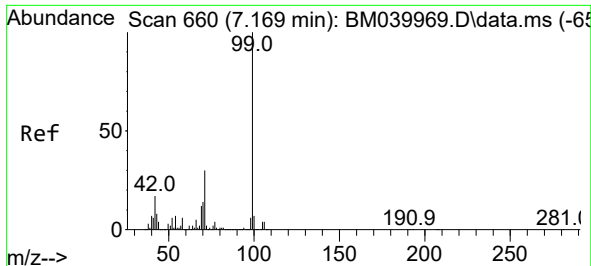


#7
Phenol-d6
Concen: 90.830 ng
RT: 7.169 min Scan# 660
Delta R.T. 0.000 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36

Instrument :
BNA_M
ClientSampleId :
PB152902BL

Tgt Ion: 99 Resp: 1975861




Ion	Ratio	Lower	Upper
99	100		
42	16.2	13.8	20.6
71	29.4	24.4	36.6

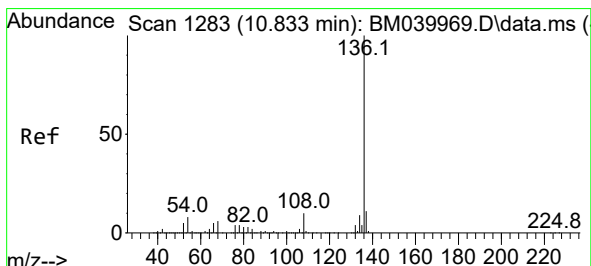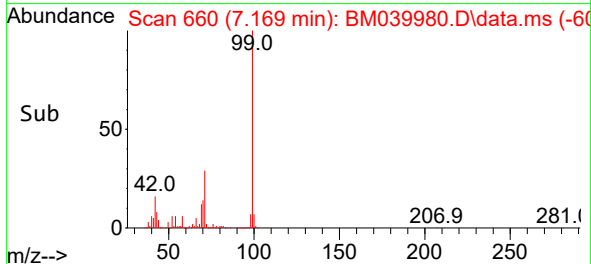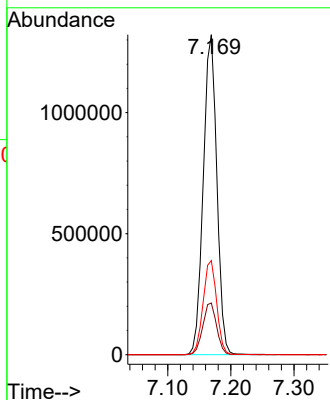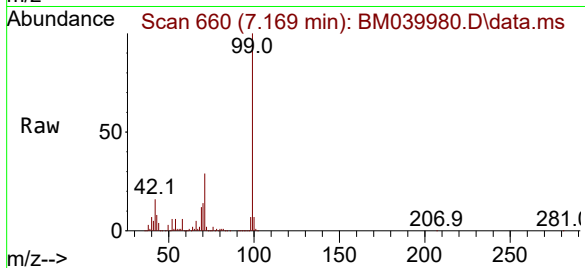


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.834 min Scan# 1283
Delta R.T. 0.001 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36

Tgt Ion: 136 Resp: 962495

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	7.5	6.1	9.1
68	5.9	4.8	7.2

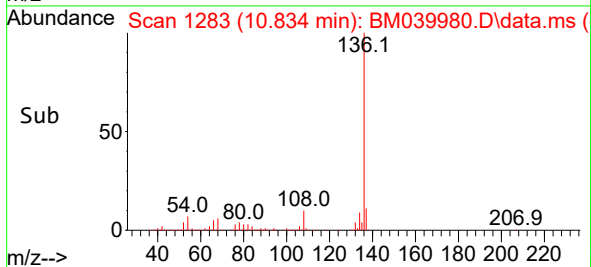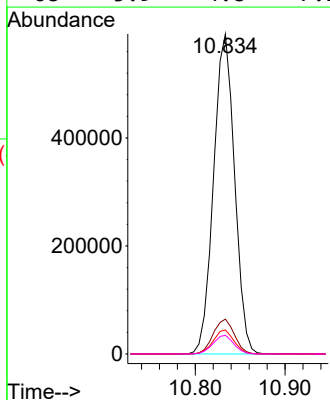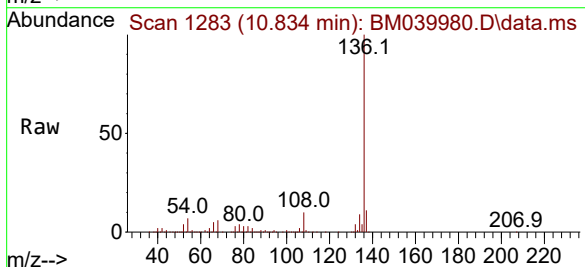



#23

Nitrobenzene-d5

Concen: 93.199 ng

RT: 9.187 min Scan# 1003

Delta R.T. 0.001 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36

Instrument :

BNA_M

ClientSampleId :

PB152902BL





Tgt Ion: 82 Resp: 1662407

Ion Ratio Lower Upper

82 100

128 47.2 36.5 54.7

54 46.4 38.3 57.5

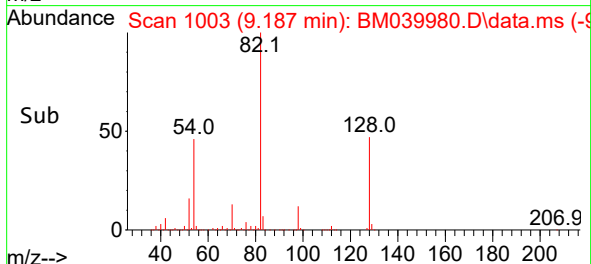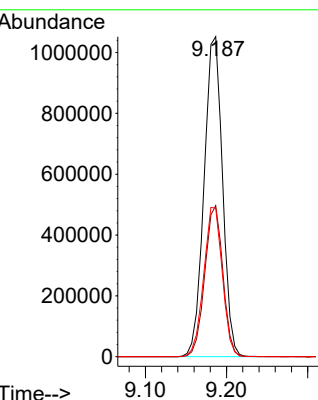

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.651 min Scan# 1932

Delta R.T. -0.006 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36




Tgt Ion:164 Resp: 458944


Ion Ratio Lower Upper

164 100

162 103.0 80.6 120.8

160 47.3 36.7 55.1


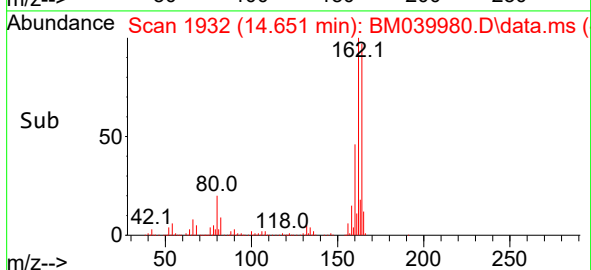
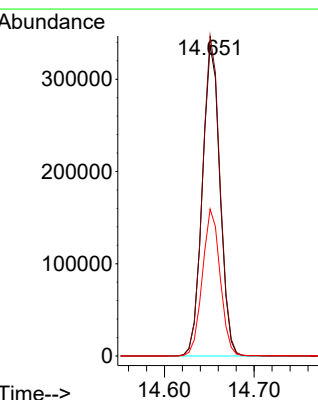
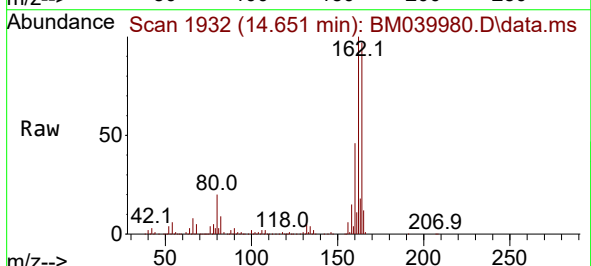


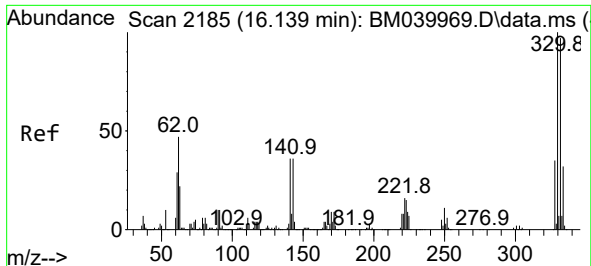

#42
2,4,6-Tribromophenol
Concen: 79.710 ng
RT: 16.133 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36




Instrument :
BNA_M
ClientSampleId :
PB152902BL


Tgt Ion:330 Resp: 474811
Ion Ratio Lower Upper
330 100
332 96.9 77.4 116.2
141 40.1 31.6 47.4

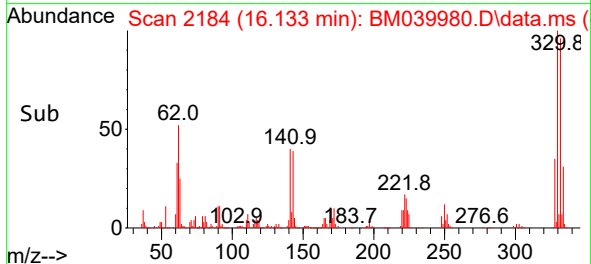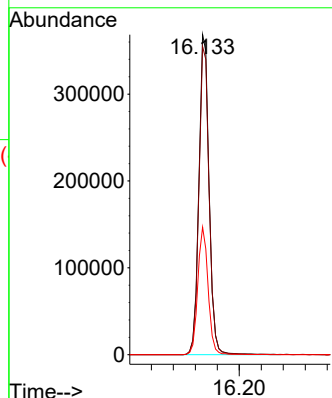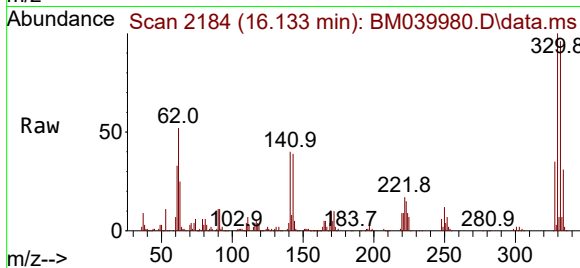

#45
2-Fluorobiphenyl
Concen: 98.959 ng
RT: 13.280 min Scan# 1699
Delta R.T. -0.006 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36

Tgt Ion:172 Resp: 3850538
Ion Ratio Lower Upper
172 100
171 35.6 28.8 43.2
170 24.5 19.6 29.4


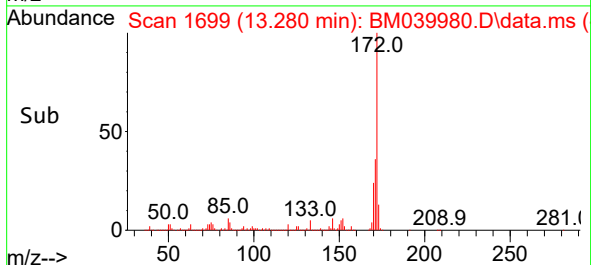
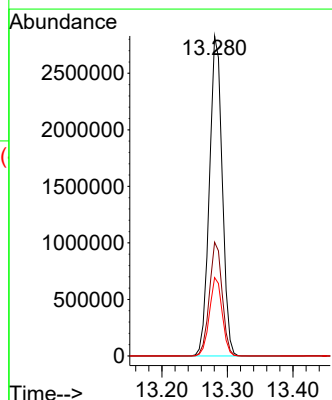
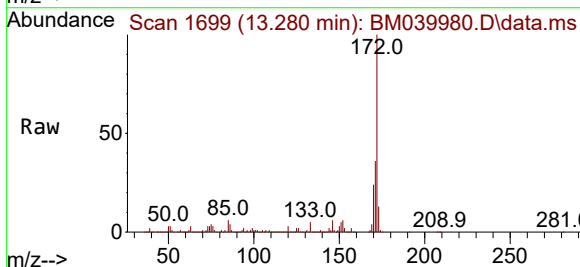


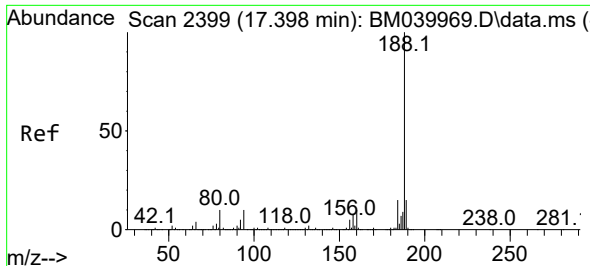

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.392 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36




Instrument :
BNA_M
ClientSampleId :
PB152902BL


Tgt Ion:188 Resp: 841612
Ion Ratio Lower Upper
188 100
94 10.1 7.8 11.8
80 11.2 8.2 12.4

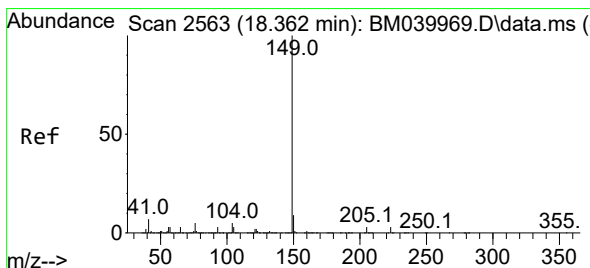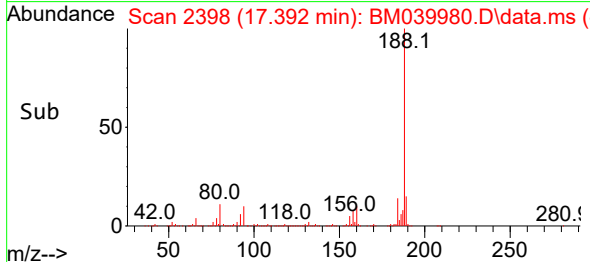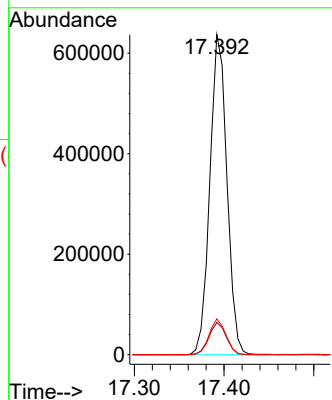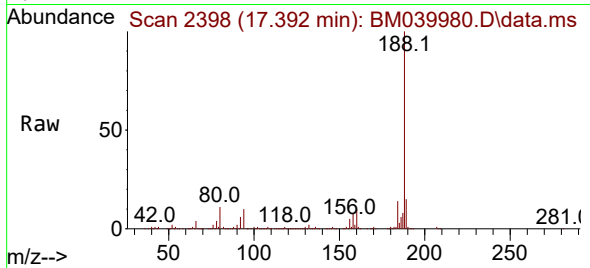

#74
Di-n-butylphthalate
Concen: 3.664 ng
RT: 18.357 min Scan# 2562
Delta R.T. -0.005 min
Lab File: BM039980.D
Acq: 24 May 2023 12:36

Tgt Ion:149 Resp: 147
Ion Ratio Lower Upper
149 100
150 0.0 7.4 11.2#
104 0.0 4.2 6.2#

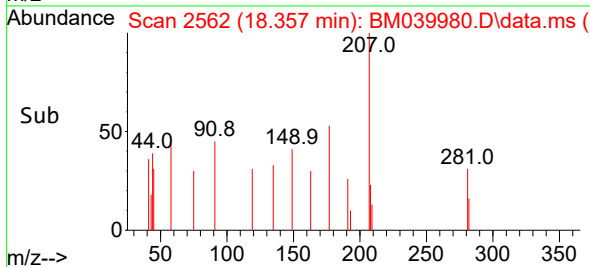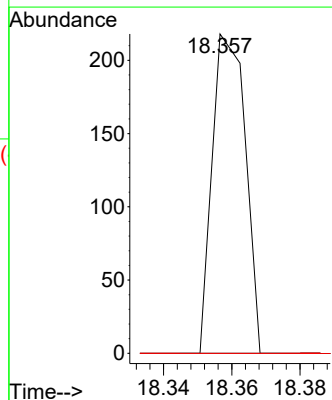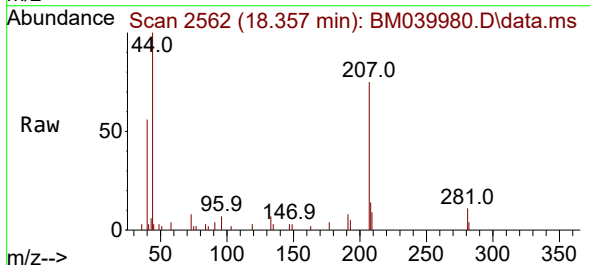



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.568 min Scan# 3108

Delta R.T. 0.000 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36

Instrument :

BNA_M

ClientSampleId :

PB152902BL





Tgt Ion:240 Resp: 597104

Ion Ratio Lower Upper

240 100

120 13.8 10.1 15.1

236 27.0 21.3 31.9

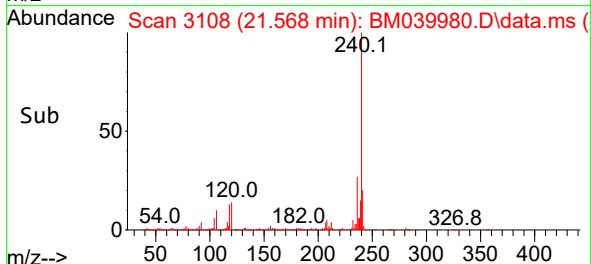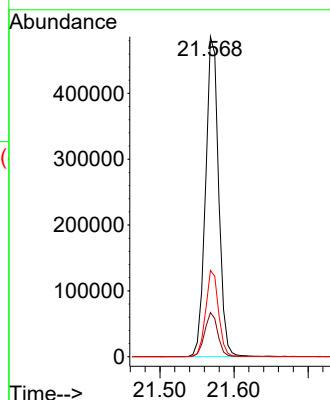

#79

Terphenyl-d14

Concen: 132.253 ng

RT: 20.009 min Scan# 2843

Delta R.T. -0.006 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36




Tgt Ion:244 Resp: 5085910


Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0

122 10.3 7.1 10.7

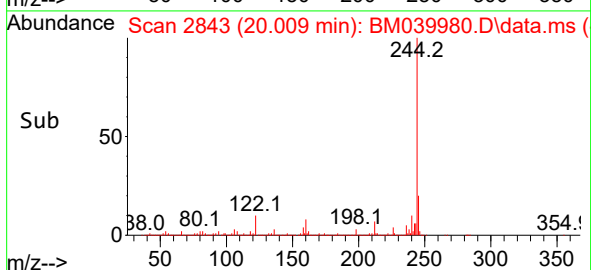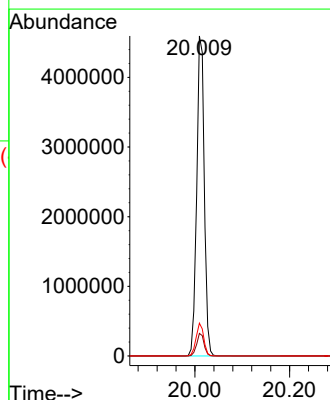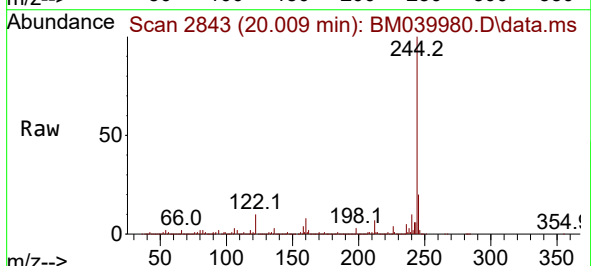

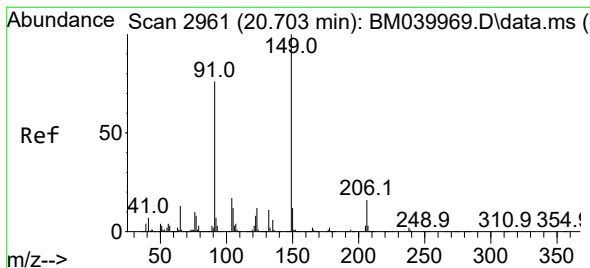

#80

Butylbenzylphthalate

Concen: 4.844 ng

RT: 20.674 min Scan# 2961

Delta R.T. -0.029 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36

Instrument :

BNA_M

ClientSampleId :

PB152902BL





Tgt Ion:149 Resp: 236

Ion Ratio Lower Upper

149 100

91 0.0 61.0 91.4#

206 0.0 12.7 19.1#

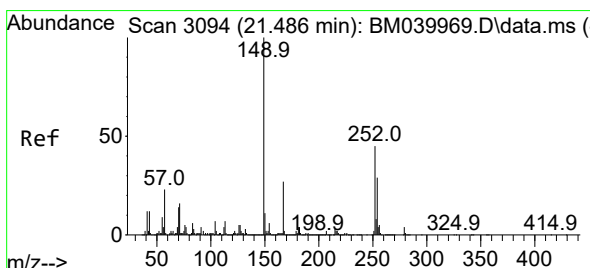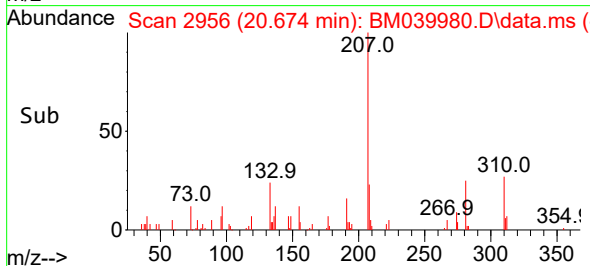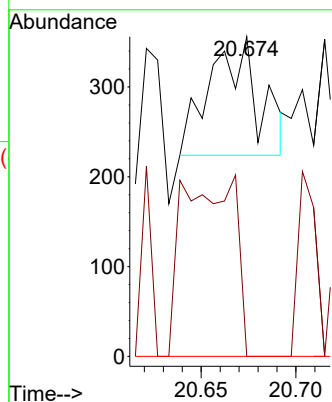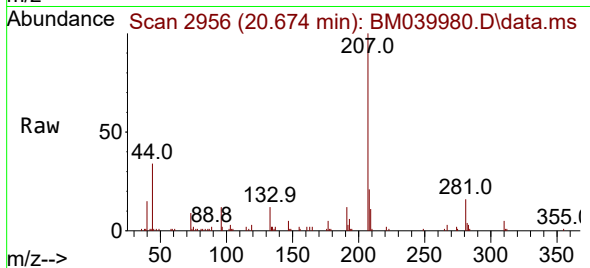

#84

Bis(2-ethylhexyl)phthalate

Concen: 3.619 ng

RT: 21.480 min Scan# 3093

Delta R.T. -0.006 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36




Tgt Ion:149 Resp: 526


Ion Ratio Lower Upper

149 100

167 0.0 21.4 32.2#

279 0.0 3.3 4.9#

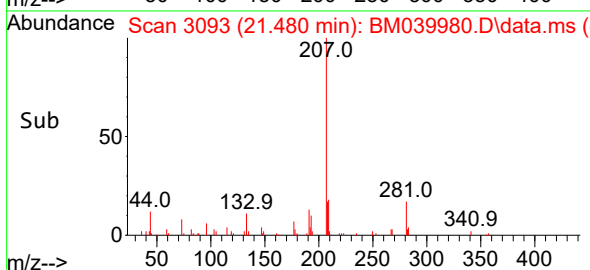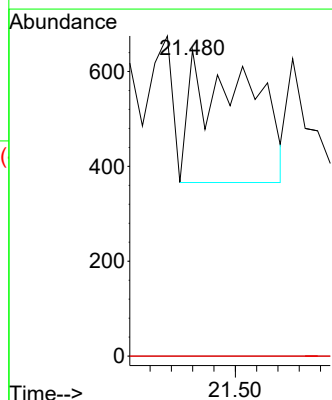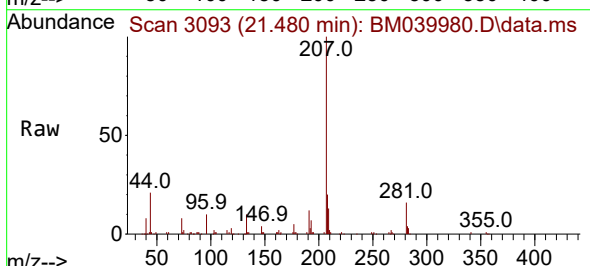



#85

Di-n-octyl phthalate

Concen: 6.617 ng

RT: 22.433 min Scan# 31

Delta R.T. 0.006 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36

Instrument :

BNA_M

ClientSampleId :

PB152902BL





Tgt Ion:149 Resp: 183

Ion Ratio Lower Upper

149 100

167 0.0 1.1 1.7#

43 147.0 7.4 11.0#

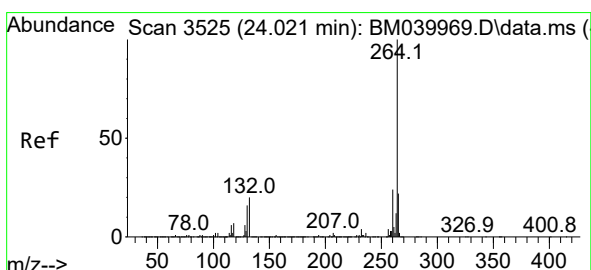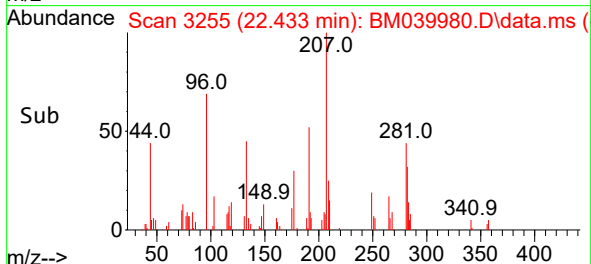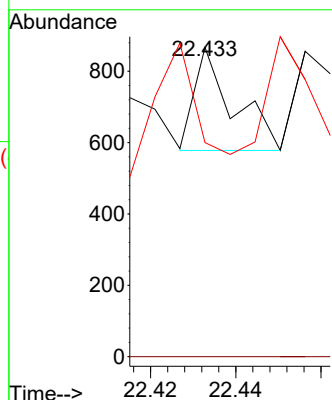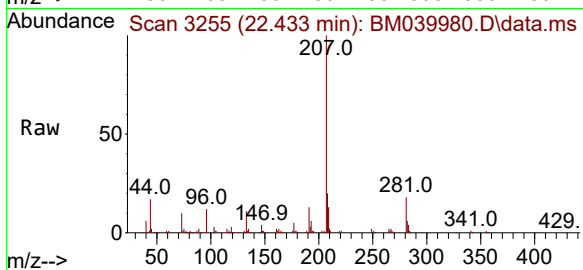

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.021 min Scan# 3525

Delta R.T. 0.000 min

Lab File: BM039980.D

Acq: 24 May 2023 12:36

Tgt Ion:264 Resp: 708376

Ion Ratio Lower Upper

264 100

260 23.4 19.5 29.3

265 21.9 17.7 26.5

