
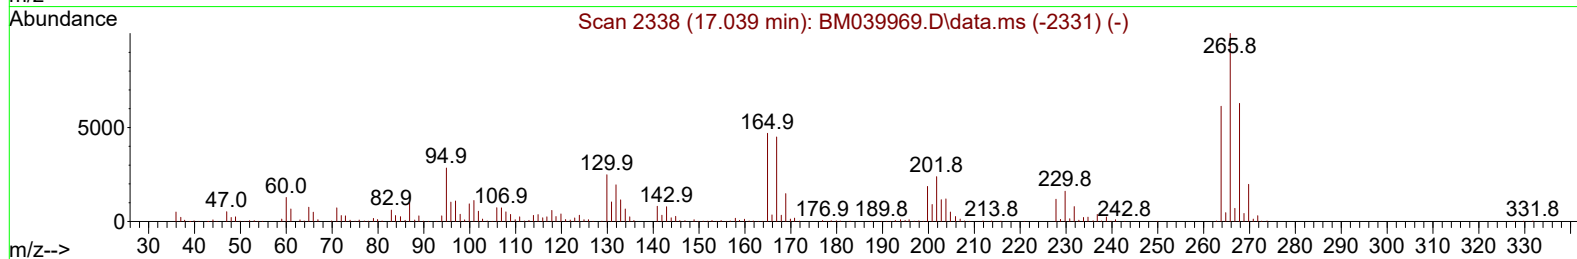
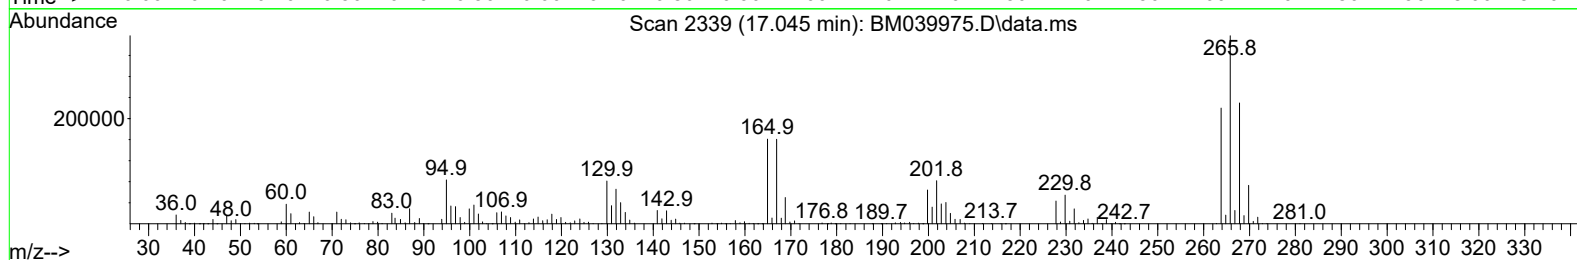


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM052423\  
Data File : BM039975.D  
Acq On : 24 May 2023 09:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 07:20:00 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM052323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 24 01:06:13 2023  
Response via : Initial Calibration

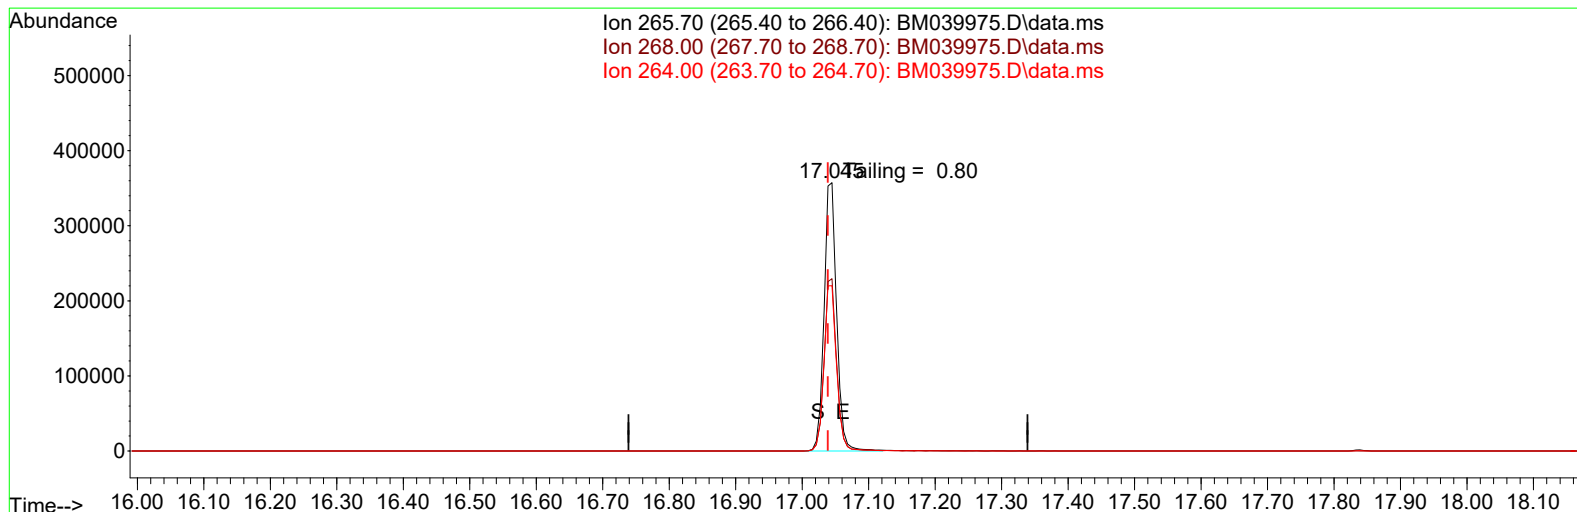

TIC: BM039975.D\data.ms

**(70) Pentachlorophenol (C)**




17.045min (+ 0.006) 1050875.78 ng

response 470392

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.80  | 64.24  |
| 264.00 | 61.30  | 61.59  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM052423\  
Data File : BM039975.D  
Acq On : 24 May 2023 09:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 07:20:00 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM052323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 24 01:06:13 2023  
Response via : Initial Calibration

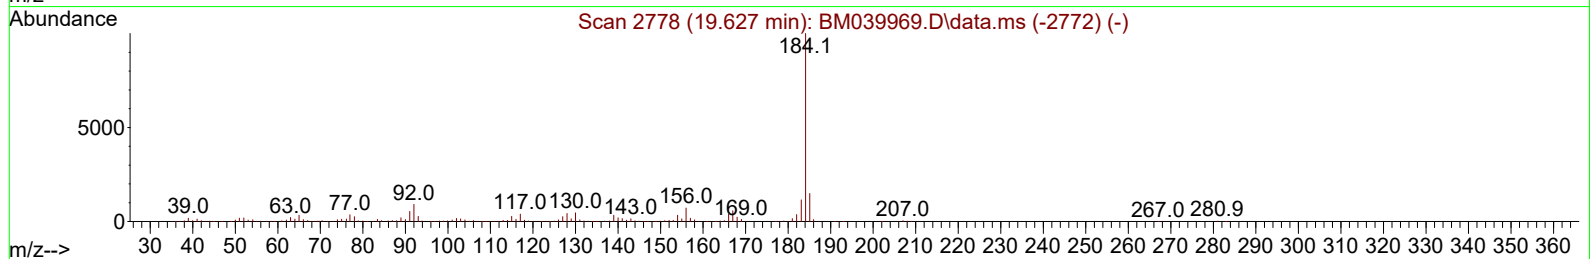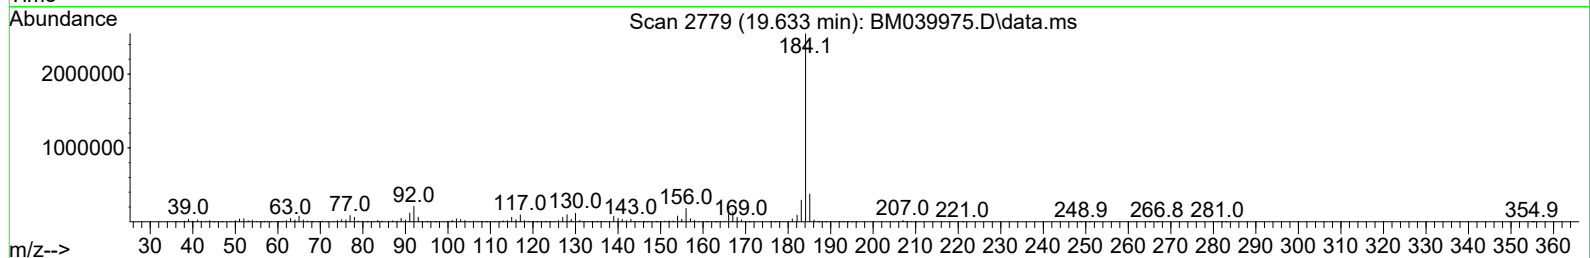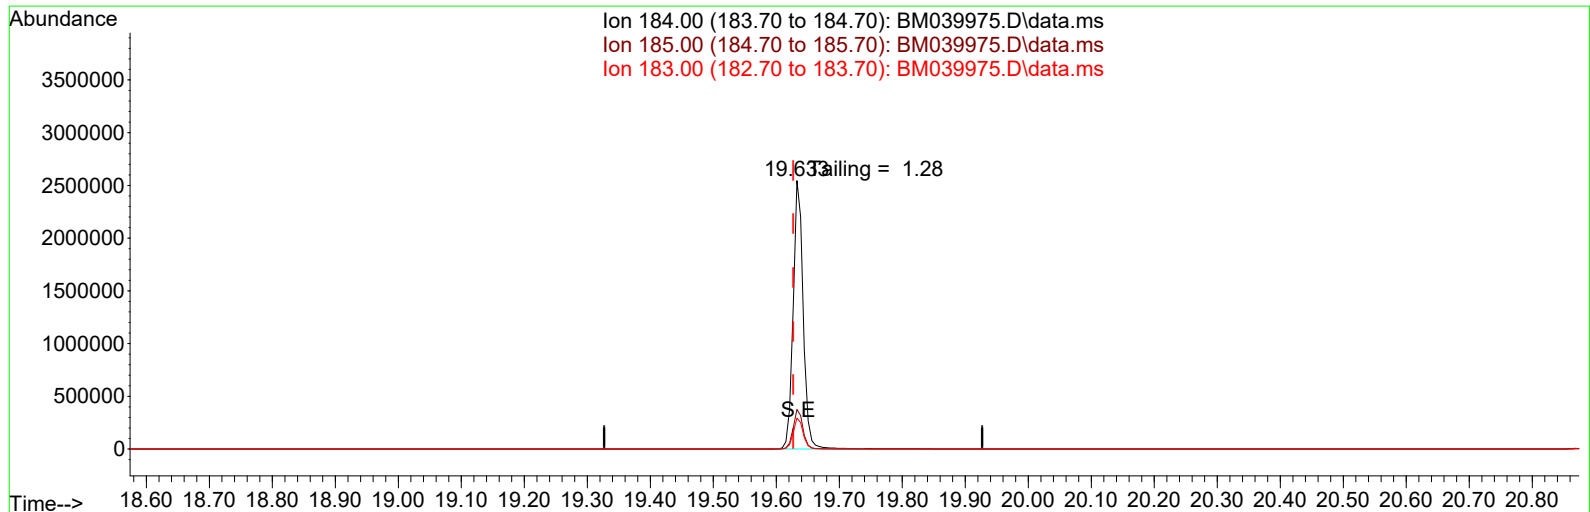

TIC: BM039975.D\data.ms

**(77) Benzidine****19.633min (+ 0.006) 65142.66 ng****response 2836512**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.77  |
| 183.00 | 11.50  | 11.52  |
| 0.00   | 0.00   | 0.00   |