

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
 Data File : BM039980.D
 Acq On : 24 May 2023 12:36
 Operator : CG/JU
 Sample : PB152902BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB152902BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	301	307	318	rBV	3260098	4282426	31.98%	7.186%
2	5.563	380	387	399	rBV	3920744	5420038	40.48%	9.095%
3	7.169	652	660	672	rBV	3447948	5230972	39.07%	8.778%
4	8.016	797	804	812	rBV	990583	1483926	11.08%	2.490%
5	9.187	994	1003	1013	rBV	3021687	4819571	36.00%	8.087%
6	10.834	1274	1283	1291	rBV	1177613	1926861	14.39%	3.233%
7	13.280	1692	1699	1709	rBV	8121326	11064962	82.64%	18.567%
8	14.651	1925	1932	1943	rBV	1480664	2052476	15.33%	3.444%
9	16.133	2178	2184	2195	rBV	3026439	3896876	29.10%	6.539%
10	17.392	2392	2398	2406	rBV	1563262	2080653	15.54%	3.491%
11	20.009	2838	2843	2852	rBV	12007403	13389029	100.00%	22.467%
12	21.568	3103	3108	3118	rBV	1473055	1857625	13.87%	3.117%
13	24.021	3518	3525	3536	rBV	1073225	2088412	15.60%	3.504%




Sum of corrected areas: 59593827

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
Data File : BM039980.D
Acq On : 24 May 2023 12:36
Operator : CG/JU
Sample : PB152902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB152902BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

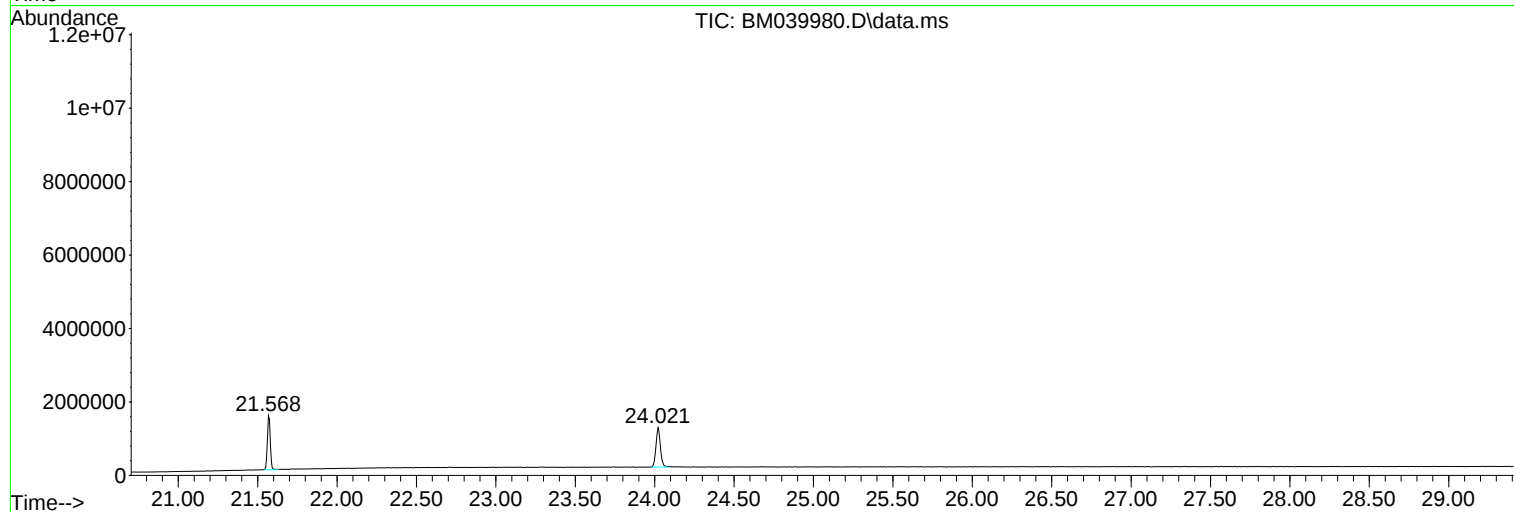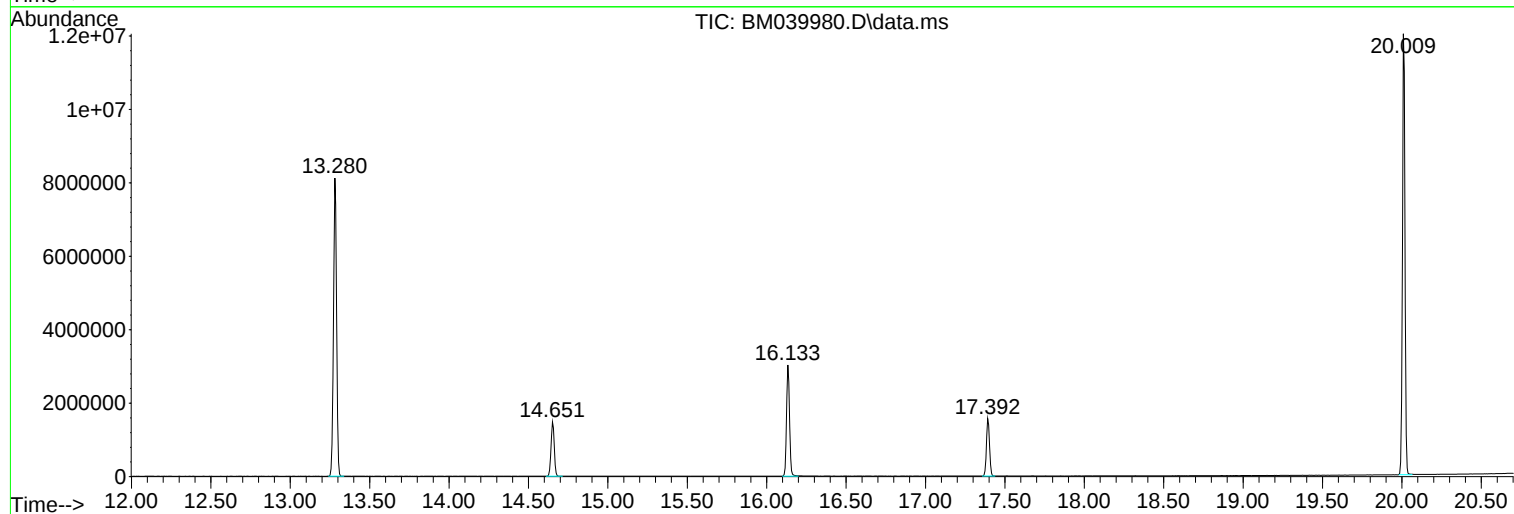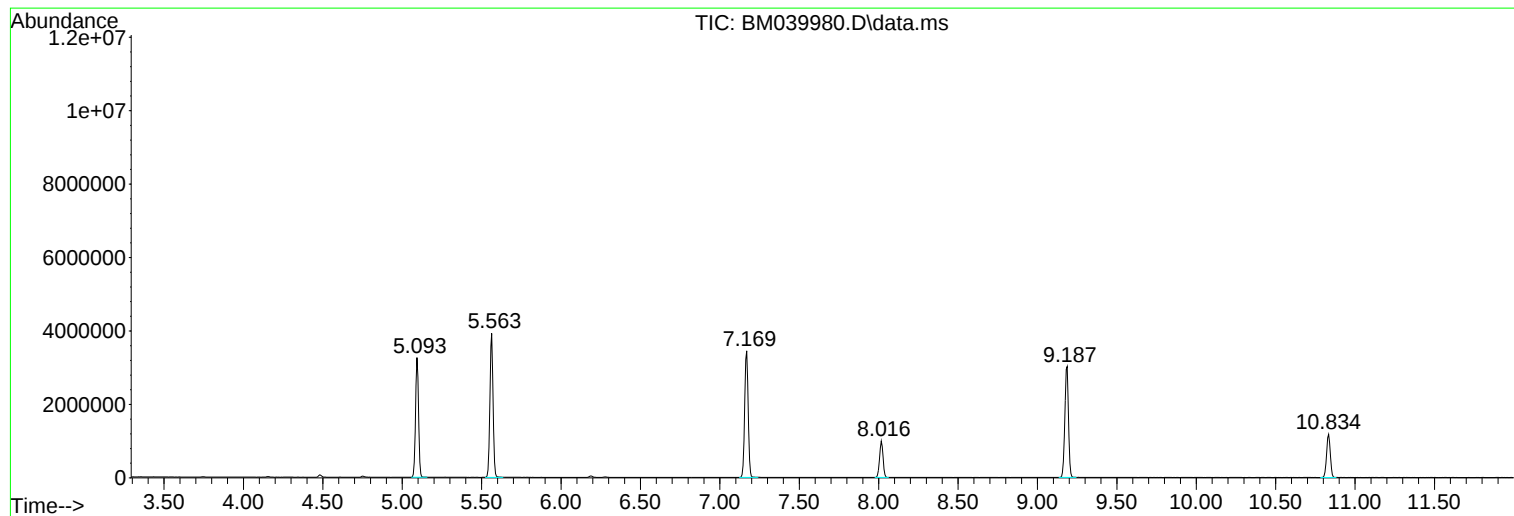

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
Data File : BM039980.D
Acq On : 24 May 2023 12:36
Operator : CG/JU
Sample : PB152902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB152902BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.093	57.72 ng	4282430	1,4-Dichlorobenzene-d4			8.016
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	72
2	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	25
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
4	Acetone		58	C3H6O	000067-64-1	10
5	5-Hexen-2-one		98	C6H10O	000109-49-9	9

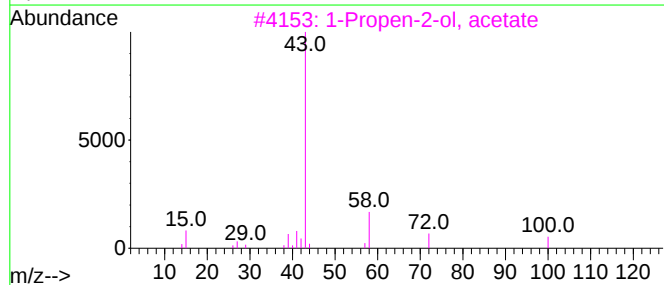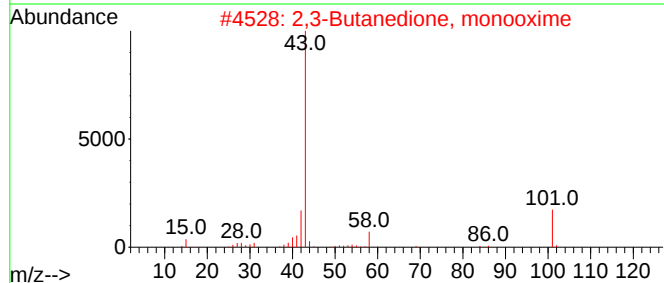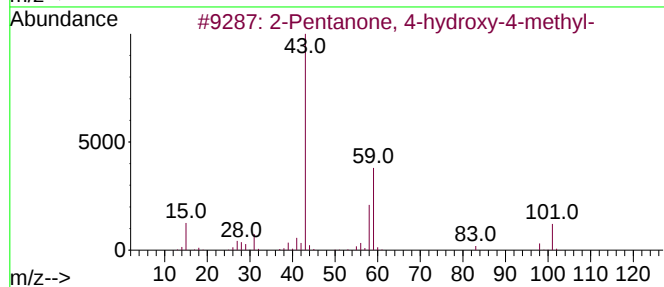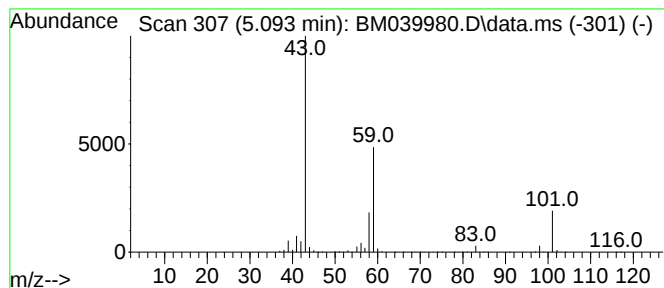

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
Data File : BM039980.D
Acq On : 24 May 2023 12:36
Operator : CG/JU
Sample : PB152902BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB152902BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.093	57.7	ng	4282430	1	8.016	1483930	20.0