


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
 Data File : BM039975.D
 Acq On : 24 May 2023 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 24 01:06:13 2023

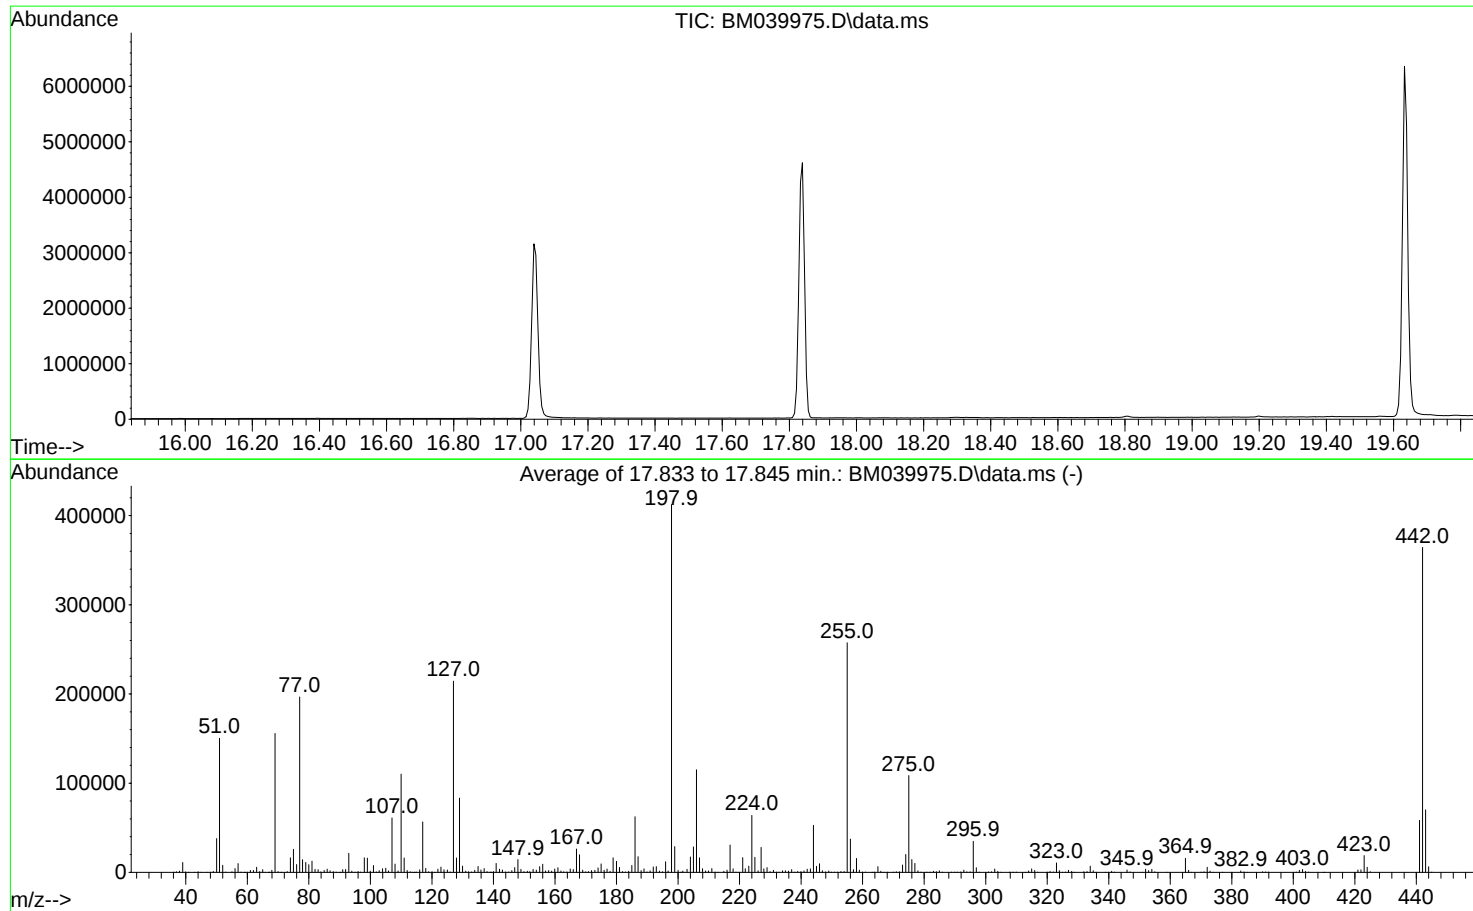

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	150365	PASS
68	69	0.00	2	1.5	2279	PASS
69	198	0.00	100	37.7	155661	PASS
70	69	0.00	2	0.6	872	PASS
127	198	10	80	52.0	214421	PASS
197	198	0.00	2	0.4	1610	PASS
198	198	100	100	100.0	412395	PASS
199	198	5	9	7.0	28829	PASS
275	198	10	60	26.3	108507	PASS
365	198	1	100	3.8	15867	PASS
441	198	0.01	100	14.1	58240	PASS
442	442	50	100	100.0	364245	PASS
443	442	15	24	19.2	70069	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/27/2023	BNA_M	<u>BM039975.D</u>
Compound Name	Response	Retention Time
DDT	1206200	20.868
DDD	7073	20.48
DDE	145	20.003
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7218	1213418	0.59

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
 Data File : BM039975.D
 Acq On : 24 May 2023 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 25 07:20:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 01:06:13 2023
 Response via : Initial Calibration

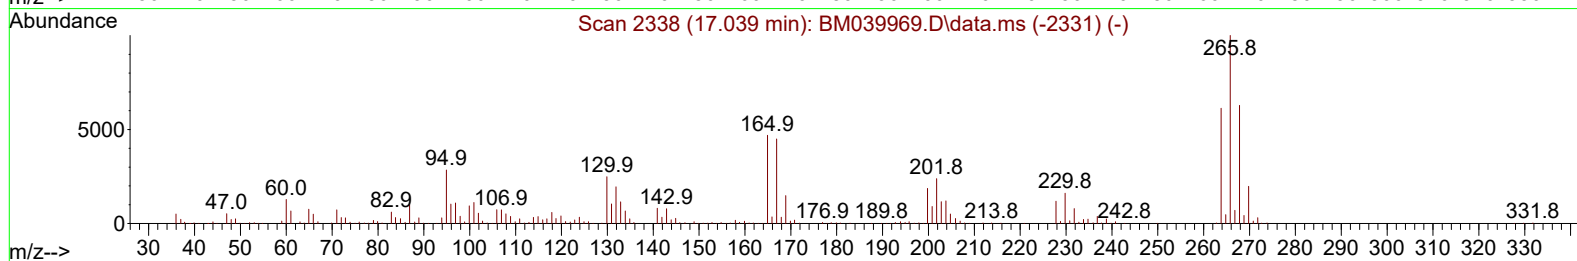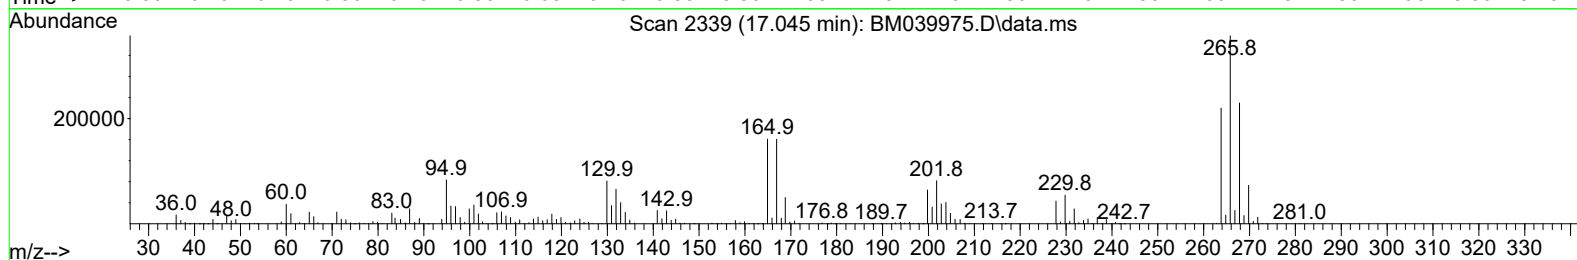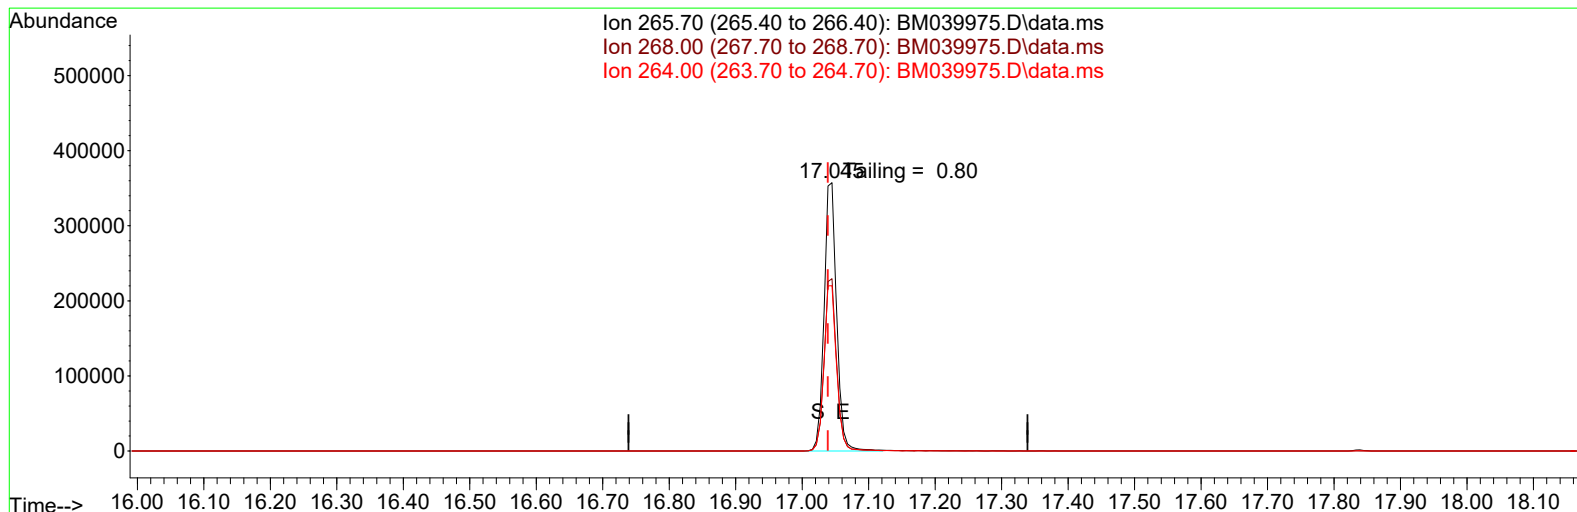

TIC: BM039975.D\data.ms

(70) Pentachlorophenol (C)

17.045min (+ 0.006) 1050875.78 ng




response 470392

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	64.24
264.00	61.30	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052423\
 Data File : BM039975.D
 Acq On : 24 May 2023 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 25 07:20:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 01:06:13 2023
 Response via : Initial Calibration

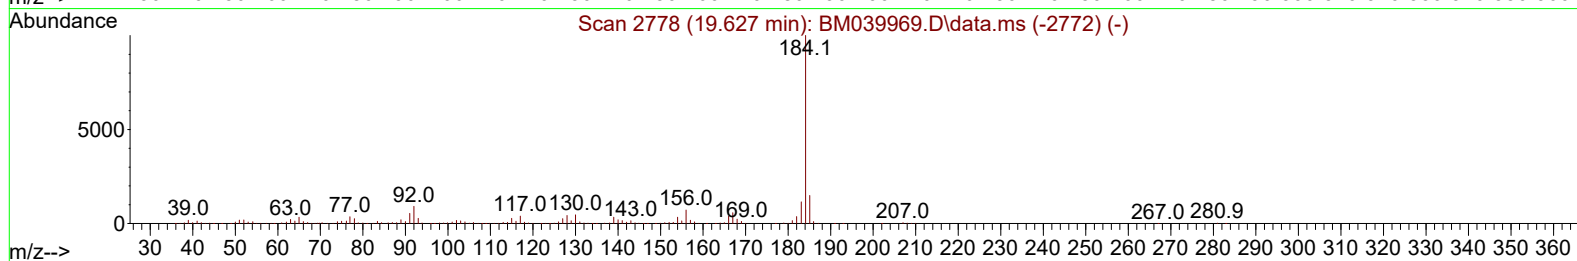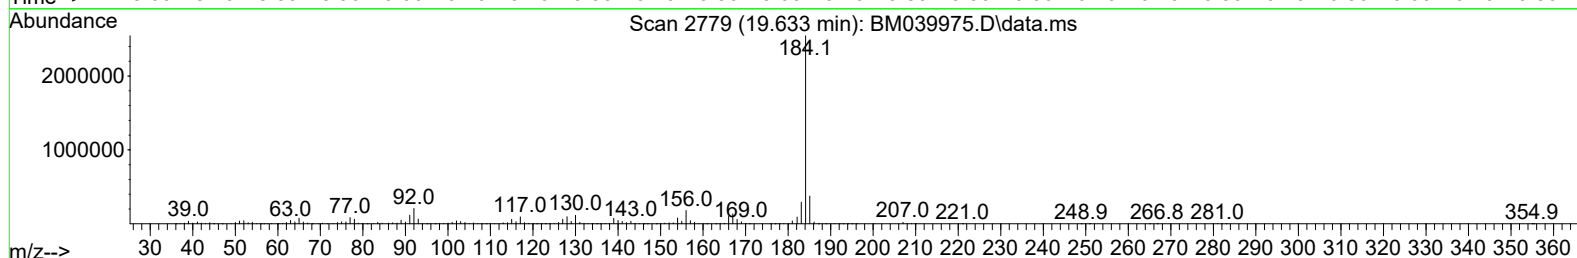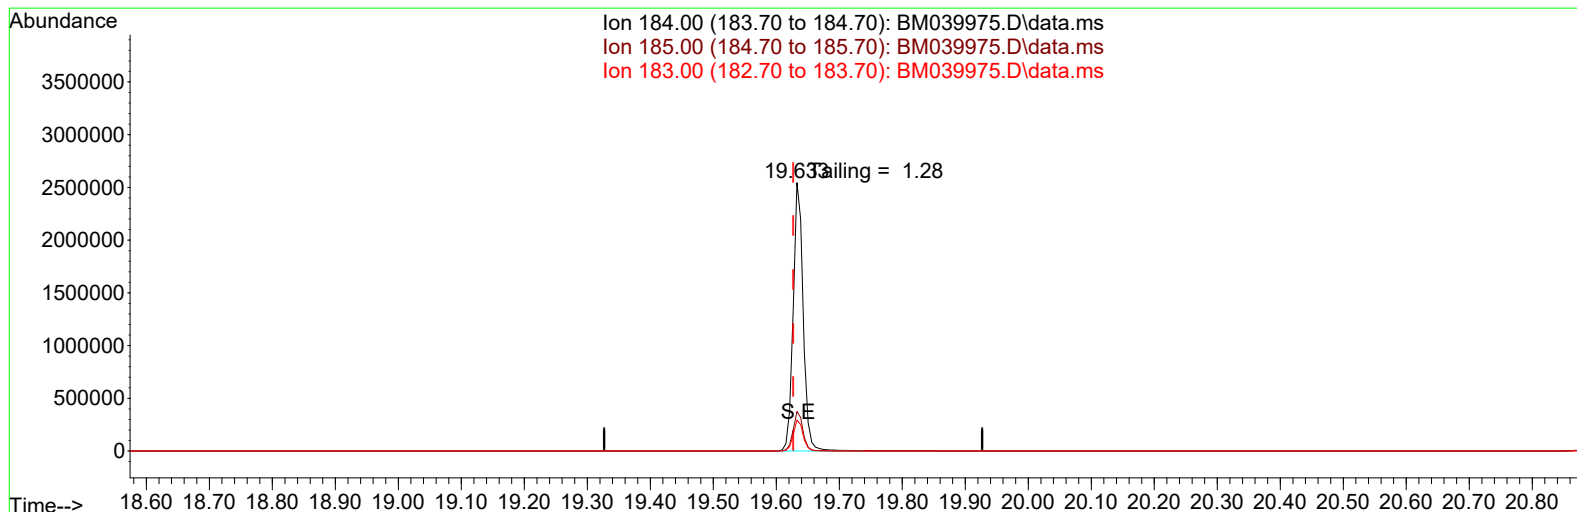

TIC: BM039975.D\data.ms

(77) Benzidine**19.633min (+ 0.006) 65142.66 ng****response 2836512**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.77
183.00	11.50	11.52
0.00	0.00	0.00