
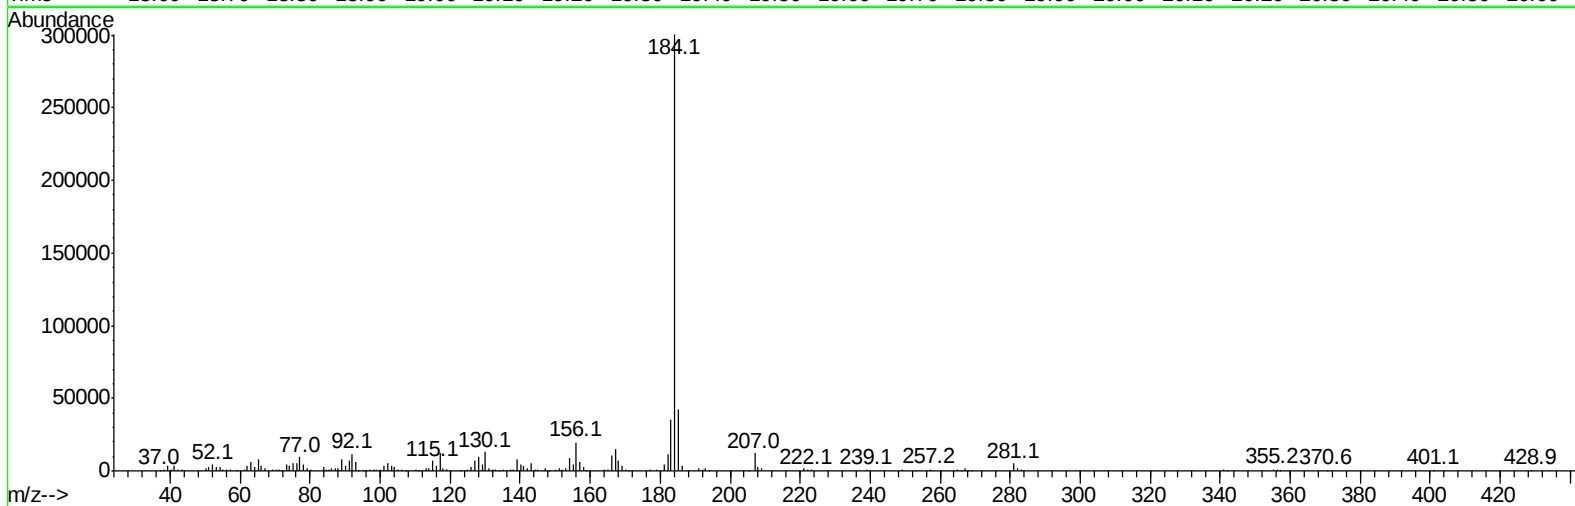


Data Path : Z:\HPCHEM1\BNA M\Data\BM052517\
Data File : BM010212.D
Acq On : 25 May 2017 12:09
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 22:58:43 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

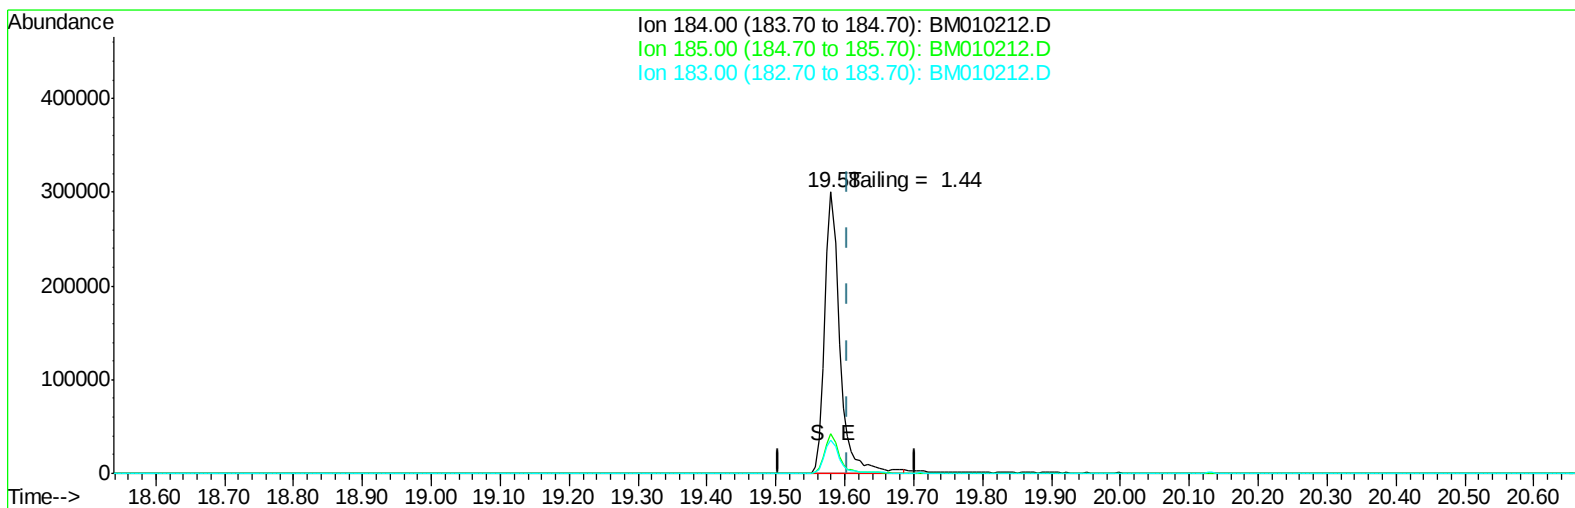

TIC: BM010212.D

(76) Benzidine



19.580min (-0.023) 217489.75ng

response 453307

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.20
183.00	11.10	11.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM052517\
Data File : BM010212.D
Acq On : 25 May 2017 12:09
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 22:58:43 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

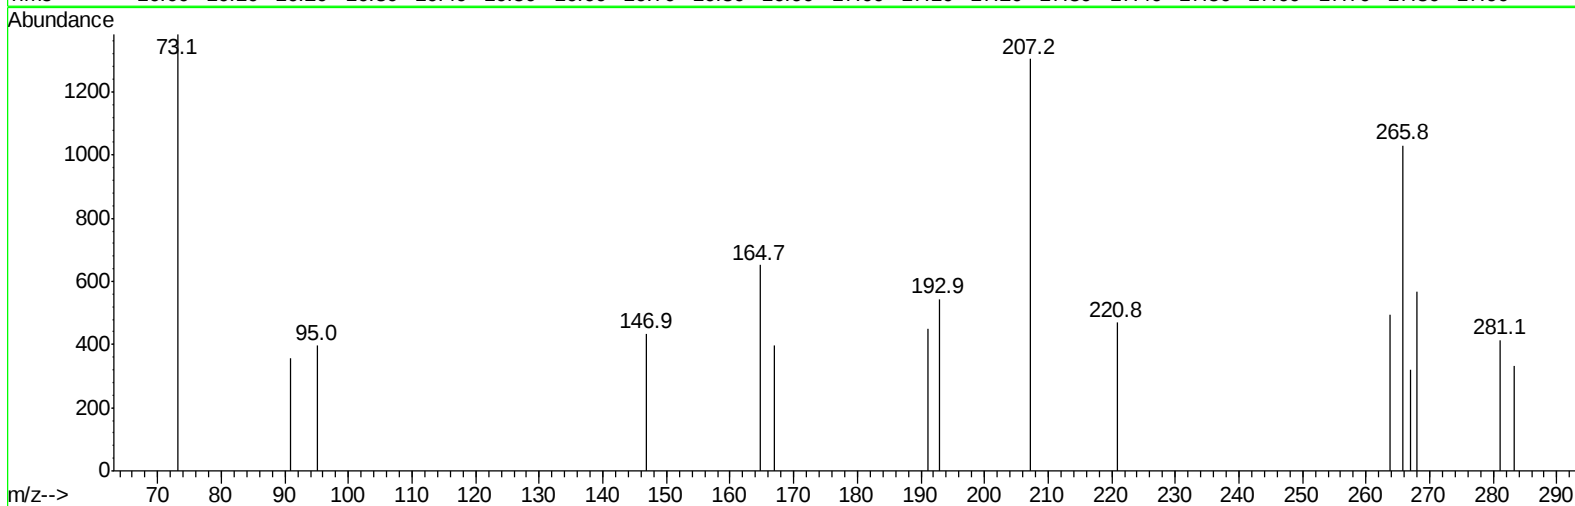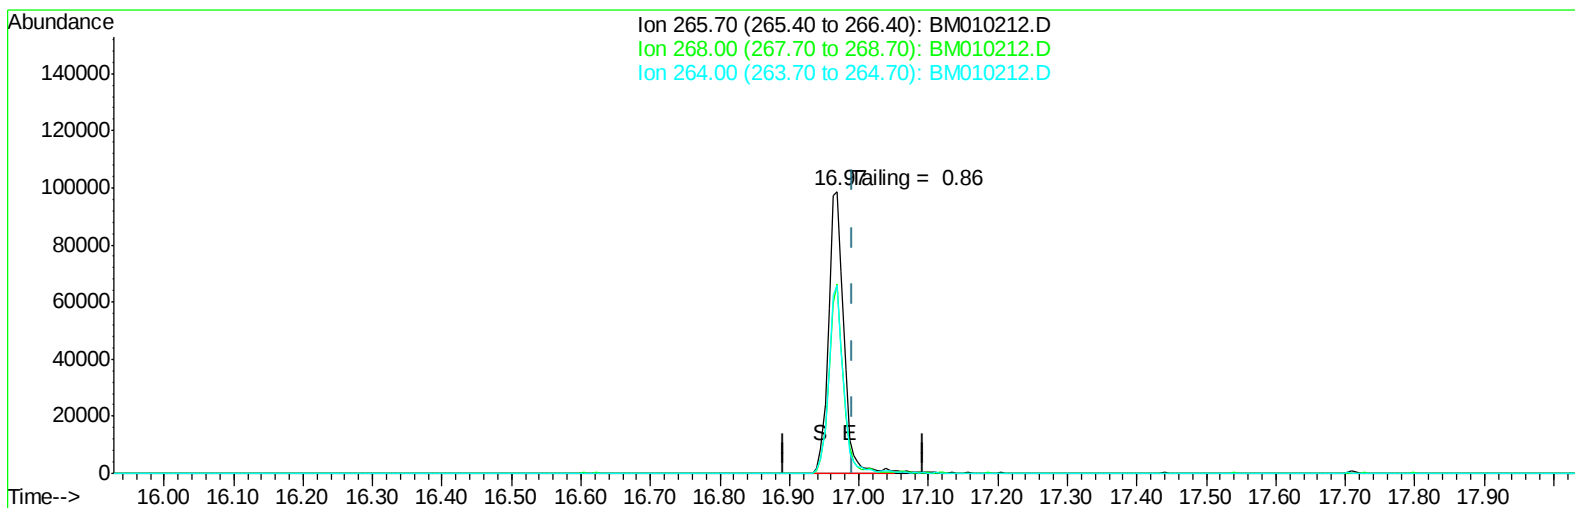

TIC: BM010212.D

(69) Pentachlorophenol (C)

16.969min (-0.023) 0.00ng

response 150564

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.25
264.00	61.20	66.77
0.00	0.00	0.00