


Data Path : Z:\HPCHEM1\BNA M\Data\BM052517\
 Data File : BM010212.D
 Acq On : 25 May 2017 12:09
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 05 14:52:12 2017

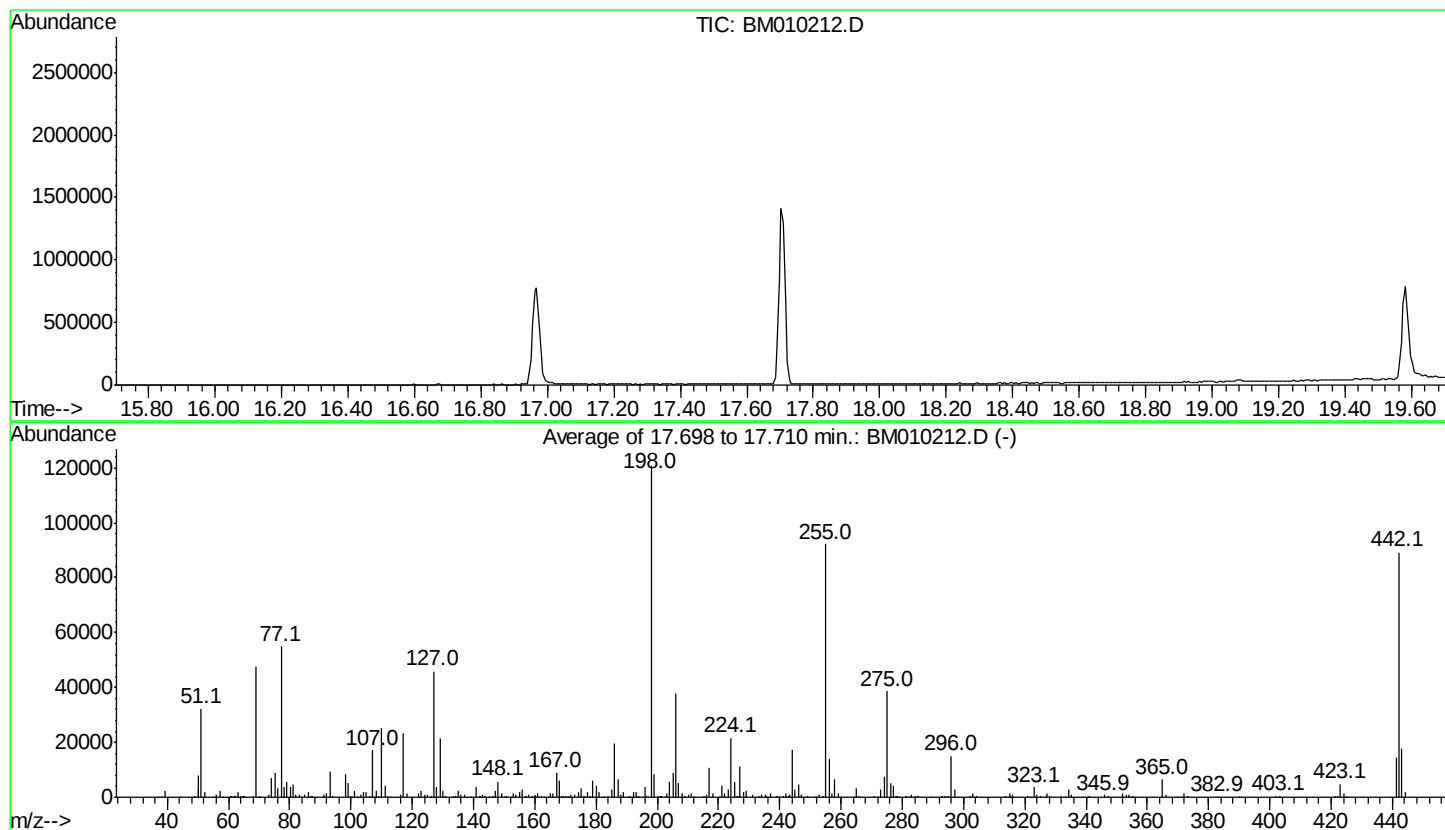

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	32405	PASS
68	69	0.00	2	1.1	508	PASS
69	198	0.00	100	39.4	47648	PASS
70	69	0.00	2	0.7	336	PASS
127	198	10	80	37.8	45701	PASS
197	198	0.00	2	0.1	123	PASS
198	198	100	100	100.0	120792	PASS
199	198	5	9	6.9	8290	PASS
275	198	10	60	31.9	38584	PASS
365	198	1	100	5.3	6398	PASS
441	442	0.01	24	16.2	14440	PASS
442	198	50	100	73.8	89189	PASS
443	442	15	24	19.7	17564	PASS