


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM052517\
Data File : BM010230.D
Acq On : 25 May 2017 22:57
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

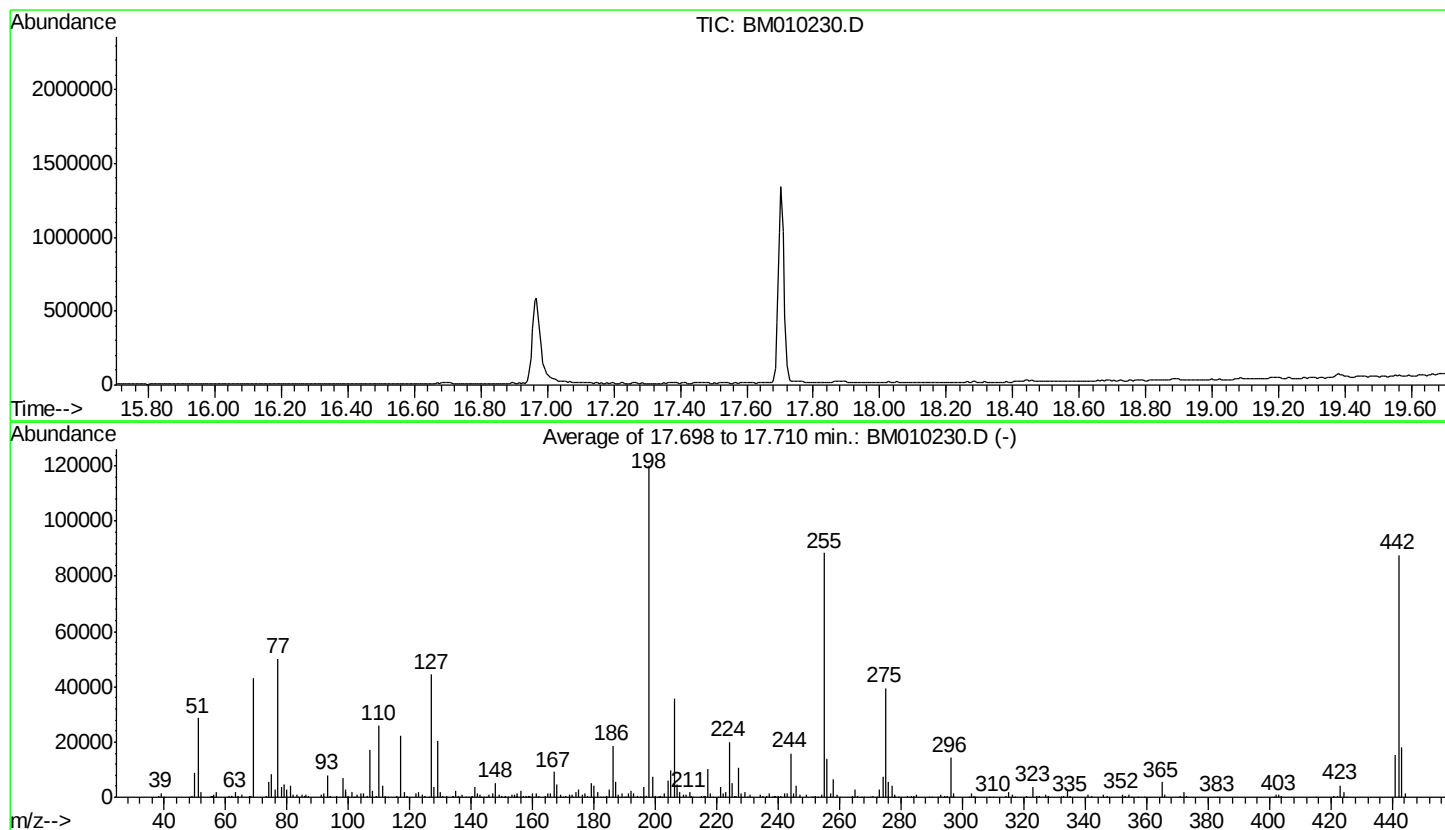

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	28610	PASS
68	69	0.00	2	1.4	607	PASS
69	198	0.00	100	36.0	43234	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.0	44448	PASS
197	198	0.00	2	0.6	695	PASS
198	198	100	100	100.0	120082	PASS
199	198	5	9	6.4	7637	PASS
275	198	10	60	32.8	39410	PASS
365	198	1	100	4.6	5464	PASS
441	443	0.01	100	84.9	15277	PASS
442	198	50	100	73.0	87664	PASS
443	442	15	24	20.5	17990	PASS