

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052523\
 Data File : BM040036.D
 Acq On : 26 May 2023 14:46
 Operator : CG/JU
 Sample : PB153065BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK065

Quant Time: May 26 16:00:22 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 15:01:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	8125	0.400	ng/ul	0.00
4) Naphthalene-d8	10.828	136	27260	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	13603	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.391	188	24111	0.400	ng/ul	0.00
17) Chrysene-d12	21.570	240	12043	0.400	ng/ul	0.00
23) Perylene-d12	24.020	264	12034	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	53449	5.650	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.411	152	10378	0.311	ng/ul	0.00
18) Fluoranthene-d10	19.417	212	14023	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.779	202	3750	0.068	ng/ul#	1
26) Benzo(a)pyrene	23.868	252	5993	0.150	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052523\
Data File : BM040036.D
Acq On : 26 May 2023 14:46
Operator : CG/JU
Sample : PB153065BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK065

Quant Time: May 26 16:00:22 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 15:01:16 2023
Response via : Initial Calibration

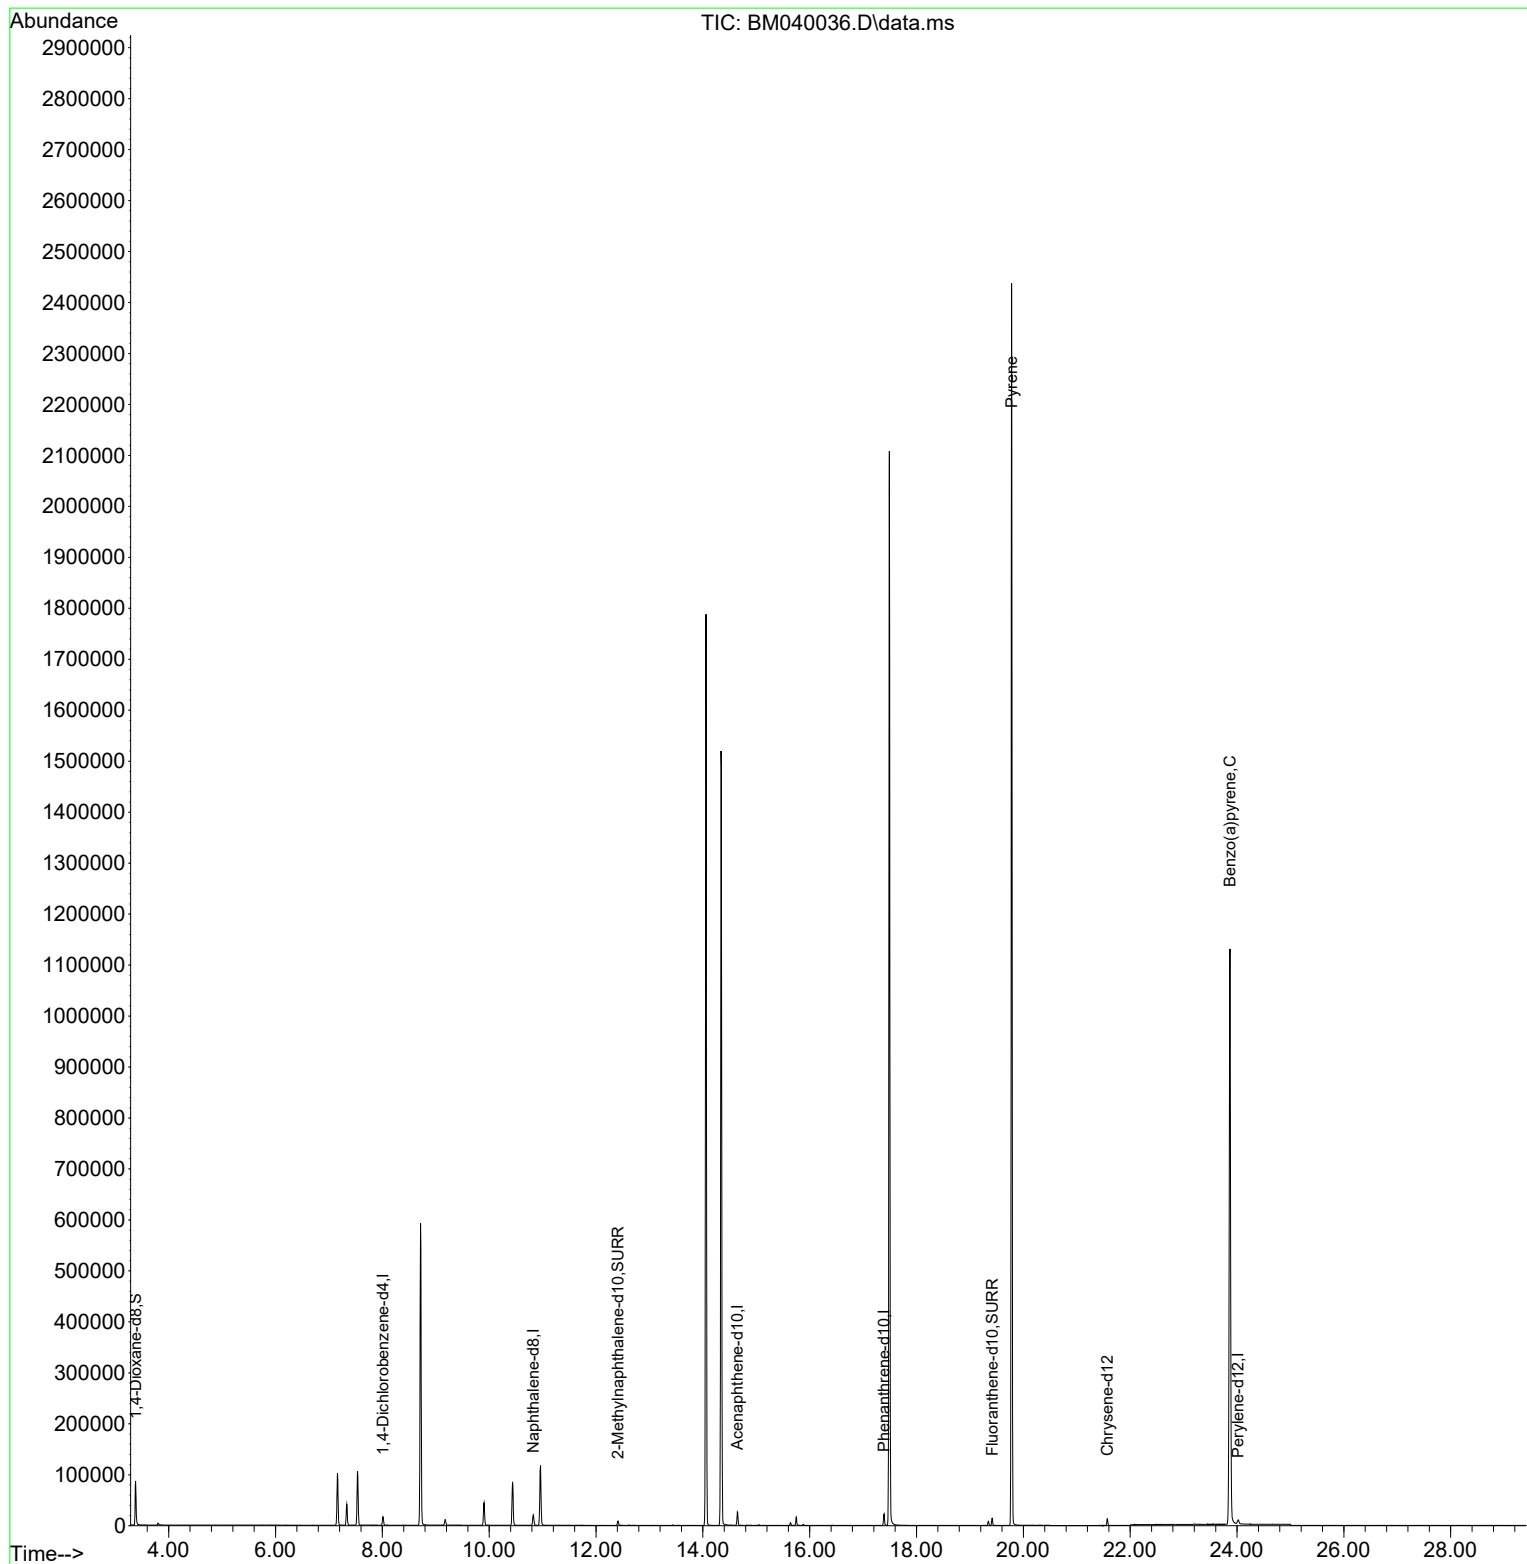

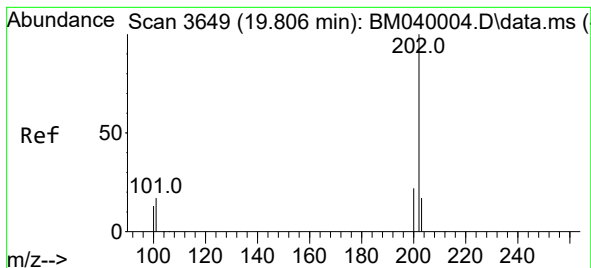

#20

Pyrene

Concen: 0.068 ng/ul

RT: 19.779 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM040036.D

Acq: 26 May 2023 14:46

Instrument :





BNA_M

ClientSampleId :

SBLK065

Tgt Ion:202 Resp: 3750

Ion	Ratio	Lower	Upper
202	100		
101	151.3	13.3	19.9#
100	1147.4	10.9	16.3#

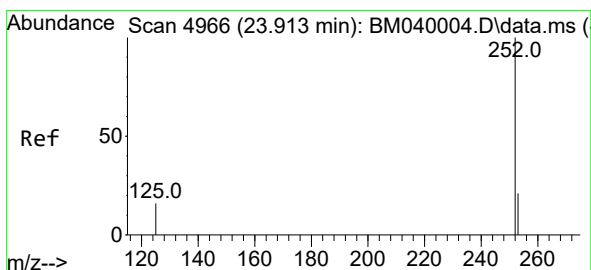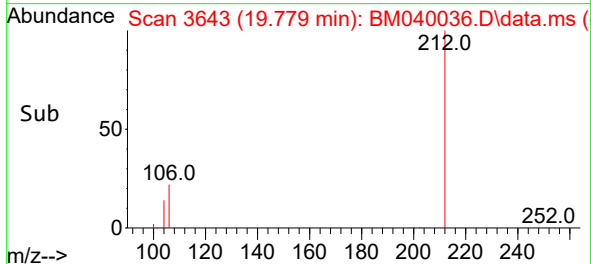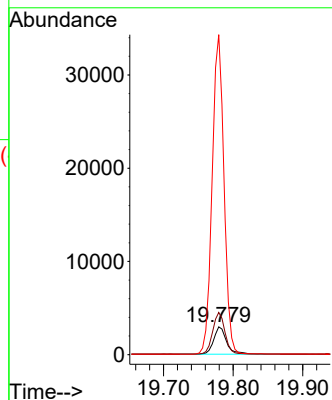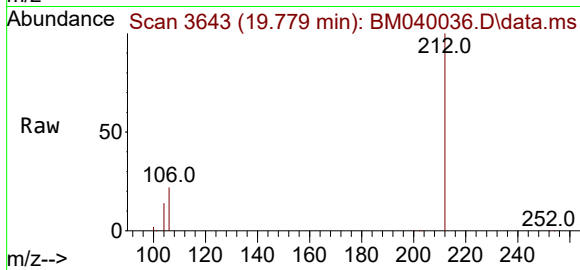

#26

Benzo(a)pyrene

Concen: 0.150 ng/ul

RT: 23.868 min Scan# 4950

Delta R.T. -0.047 min

Lab File: BM040036.D

Acq: 26 May 2023 14:46

Tgt Ion:252 Resp: 5993

Ion	Ratio	Lower	Upper
252	100		
253	37.8	20.6	31.0#
125	34.3	19.1	28.7#

