

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052523\
 Data File : BM040041.D
 Acq On : 26 May 2023 17:48
 Operator : CG/JU
 Sample : 02851-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ8

Quant Time: May 26 19:00:58 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 15:01:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.012	152	8025	0.400	ng/ul	0.00
4) Naphthalene-d8	10.828	136	27032	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	12814	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.391	188	21223	0.400	ng/ul	0.00
17) Chrysene-d12	21.567	240	9285	0.400	ng/ul	0.00
23) Perylene-d12	24.014	264	8999	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.380	96	17944	1.920	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.411	152	3953	0.120	ng/ul	0.00
18) Fluoranthene-d10	19.412	212	5231	0.187	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.445	202	1062	0.025	ng/ul#	Qvalue 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052523\
Data File : BM040041.D
Acq On : 26 May 2023 17:48
Operator : CG/JU
Sample : 02851-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FJ8


Quant Time: May 26 19:00:58 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 15:01:16 2023
Response via : Initial Calibration

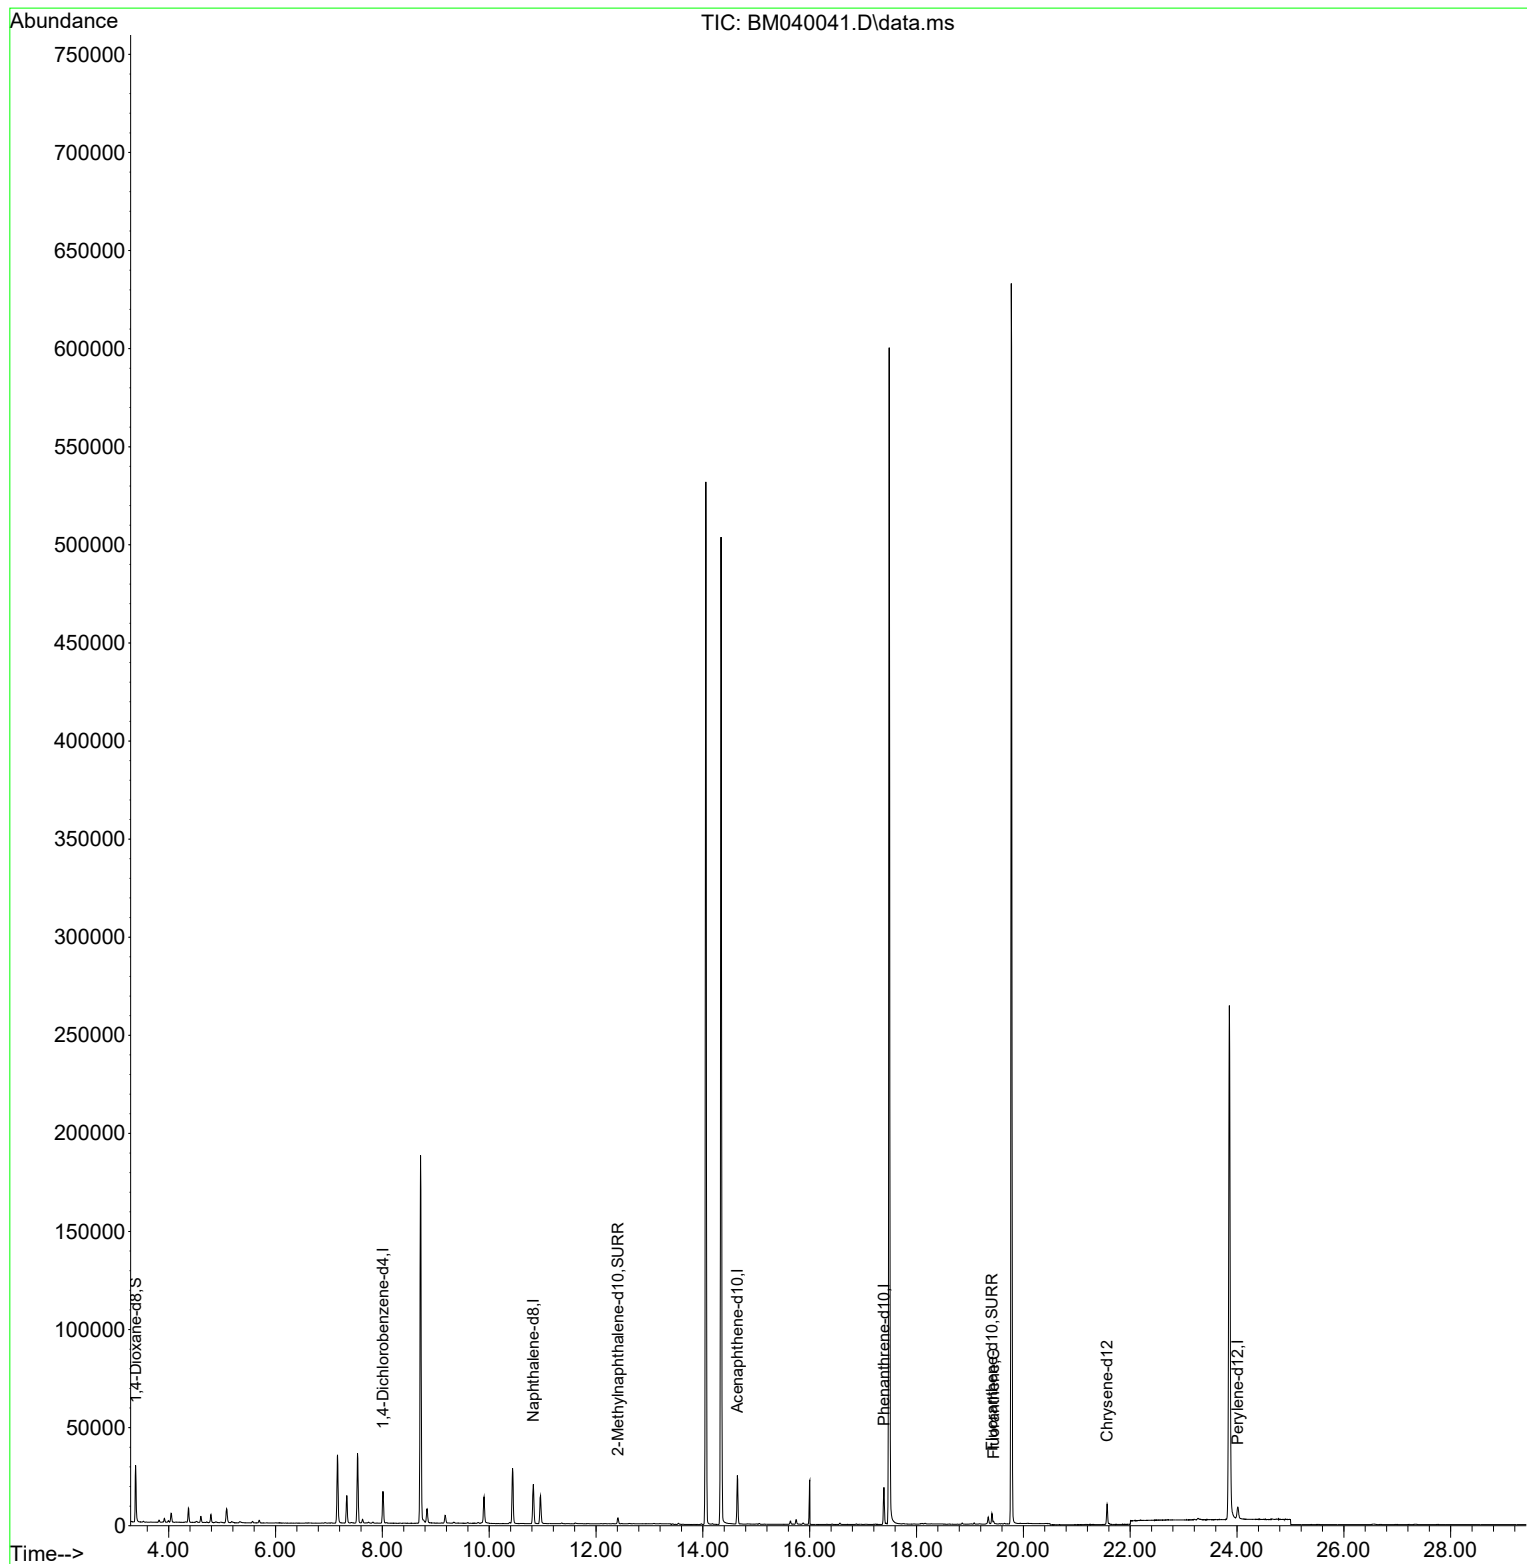

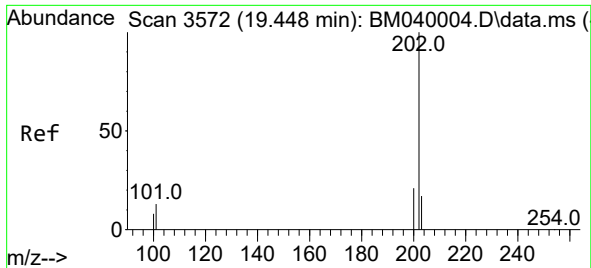

#19
 Fluoranthene
 Concen: 0.025 ng/ul
 RT: 19.445 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM040041.D
 Acq: 26 May 2023 17:48

Instrument :
 BNA_M
 ClientSampleId :
 H0FJ8

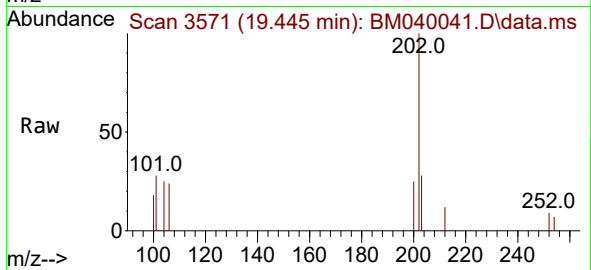

Tgt Ion:202 Resp: 1062
 Ion Ratio Lower Upper
 202 100
 101 27.9 11.5 17.3#
 100 18.3 8.5 12.7#

