
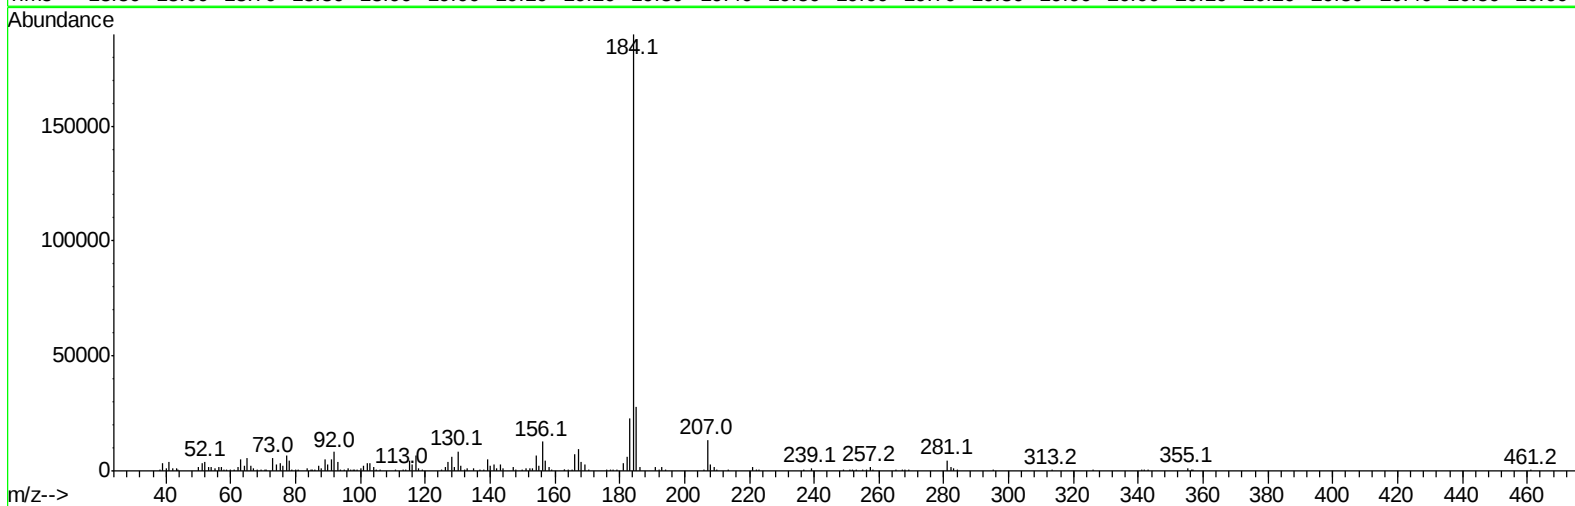


Data Path : Z:\HPCHEM1\BNA M\DATA\BM052617\
Data File : BM010248.D
Acq On : 26 May 2017 09:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 02:59:17 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

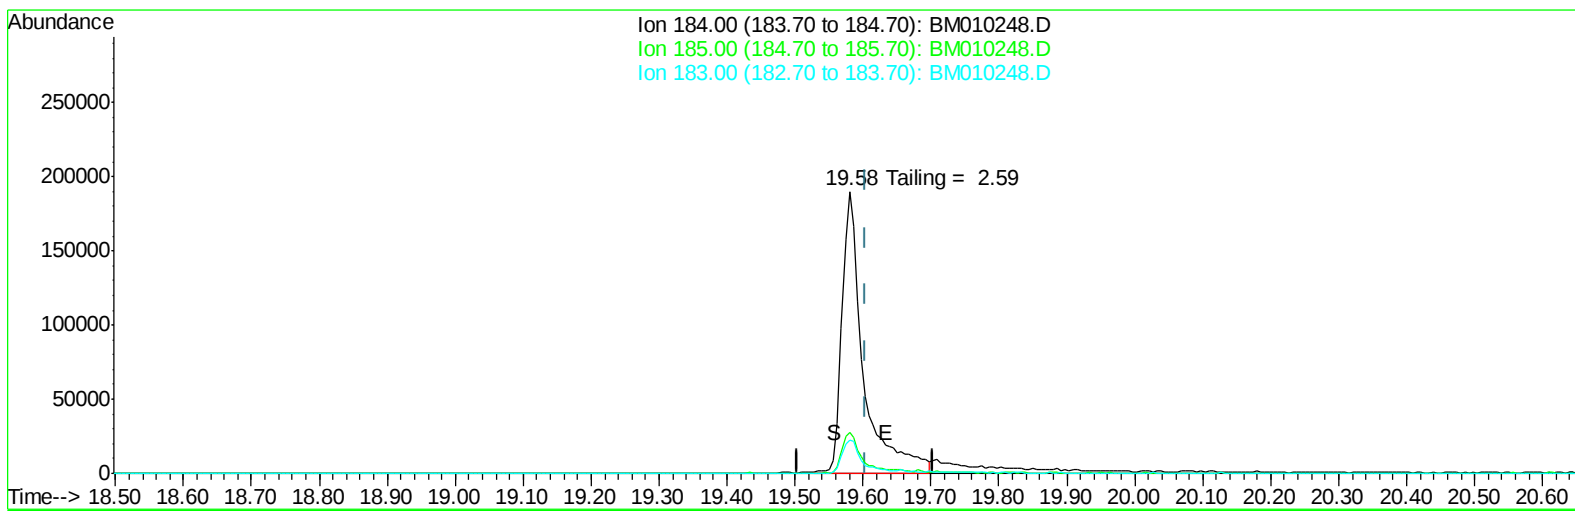

TIC: BM010248.D

(76) Benzidine



19.580min (-0.024) 10045.04ng

response 388716

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.53
183.00	11.10	11.89
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA M\DATA\BM052617\  
Data File : BM010248.D  
Acq On    : 26 May 2017  09:47  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: May 27 02:59:17 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 20 04:25:49 2017
Response via : Initial Calibration

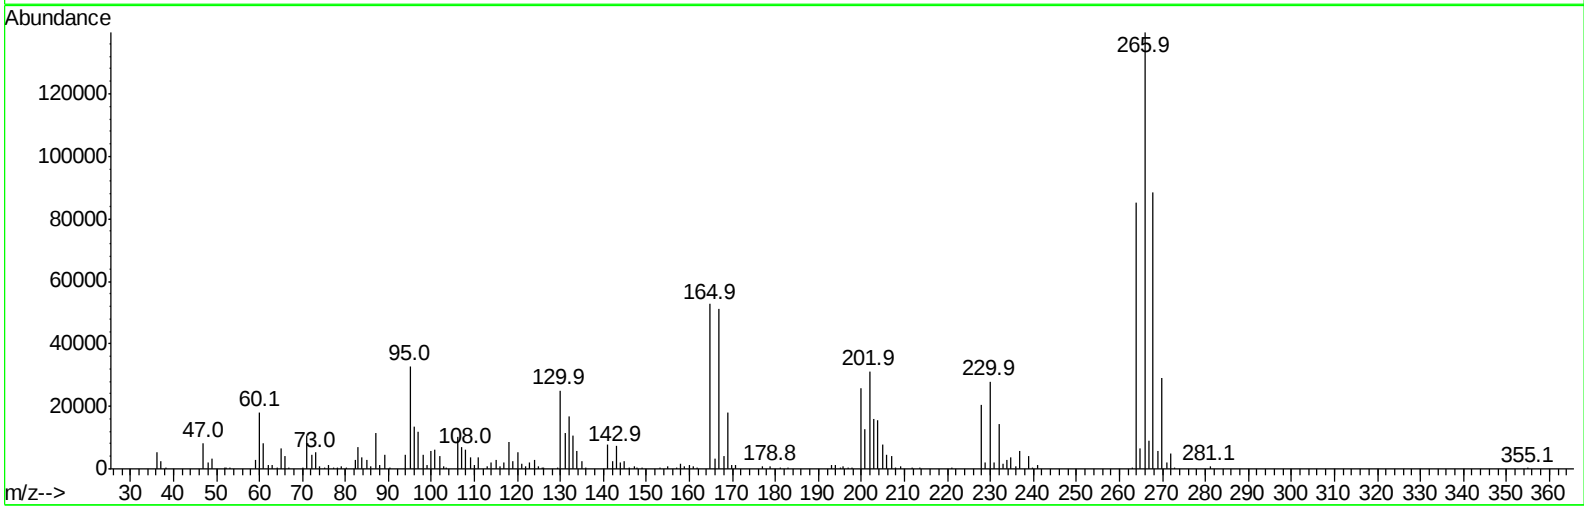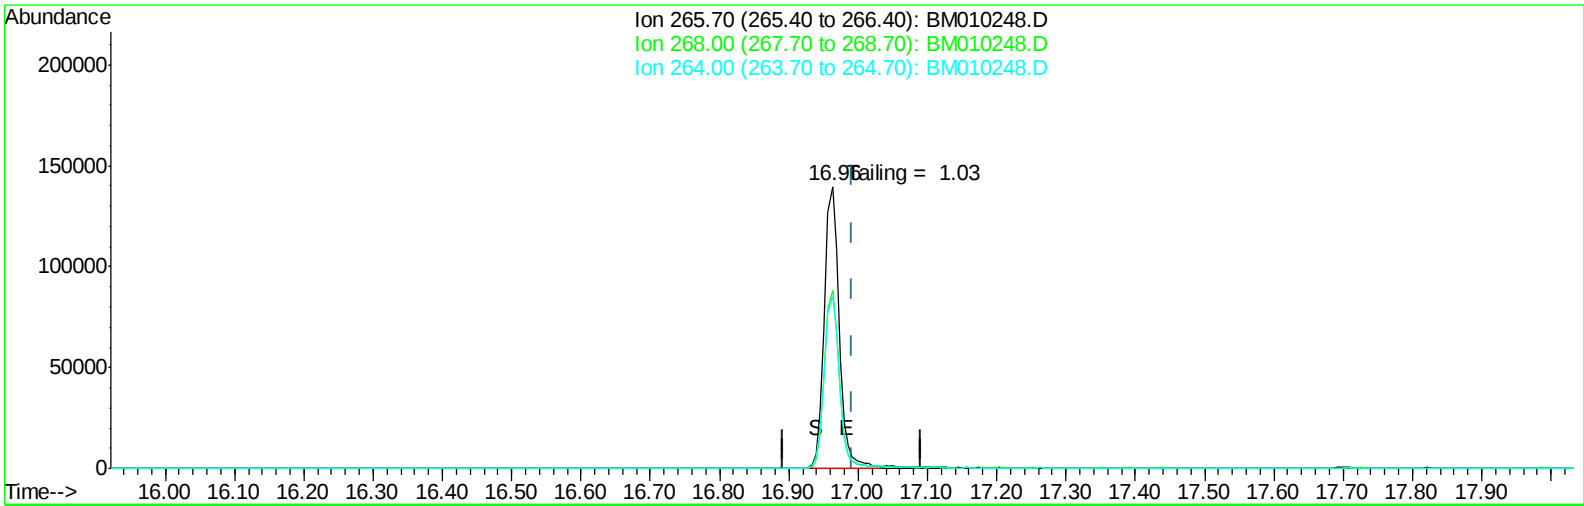

TIC: BM010248.D

(69) Pentachlorophenol (C)

16.962min (-0.030) 46907.97ng

response 207571

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.35
264.00	61.20	60.88
0.00	0.00	0.00