


Data Path : Z:\HPCHEM1\BNA_M\Data\BM052617\
 Data File : BM010248.D
 Acq On : 26 May 2017 09:47
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

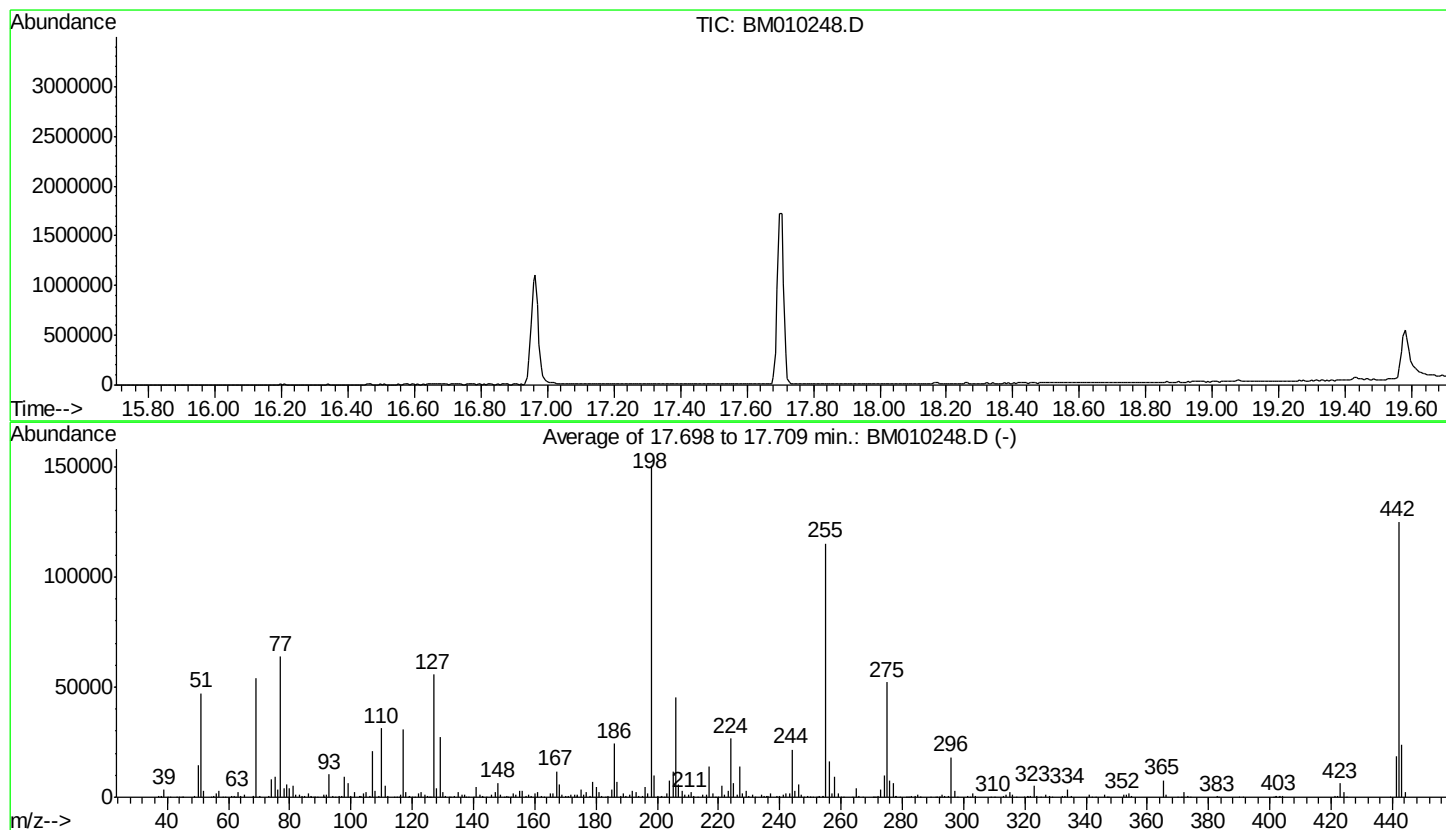

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	47048	PASS
68	69	0.00	2	1.3	718	PASS
69	198	0.00	100	36.1	54248	PASS
70	69	0.00	2	0.6	341	PASS
127	198	10	80	37.0	55621	PASS
197	198	0.00	2	1.0	1533	PASS
198	198	100	100	100.0	150458	PASS
199	198	5	9	6.6	9994	PASS
275	198	10	60	34.6	52080	PASS
365	198	1	100	5.2	7860	PASS
441	442	0.01	24	15.0	18778	PASS
442	198	50	100	83.0	124928	PASS
443	442	15	24	19.3	24090	PASS