

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052620\  
 Data File : BM026130.D  
 Acq On : 27 May 2020 01:33  
 Operator : MA/SJ  
 Sample : L2756-04  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 ETKW8

Quant Time: May 27 03:25:08 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM051320MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue May 26 11:15:44 2020  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.49  | 152  | 173439   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.29 | 136  | 705733   | 20.00 | ng/ul | 0.04     |
| 36) Acenaphthene-d10      | 14.13 | 164  | 435160   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 16.88 | 188  | 914226   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.07 | 240  | 947924   | 20.00 | ng/ul | -0.01    |
| 86) Perylene-d12          | 23.19 | 264  | 977273   | 20.00 | ng/ul | -0.01    |

## System Monitoring Compounds

|                                |       |     |         |       |       |      |
|--------------------------------|-------|-----|---------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.06  | 96  | 26798   | 4.66  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 6.69  | 99  | 113328  | 7.20  | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 6.84  | 67  | 313870  | 28.84 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.03  | 132 | 300001  | 24.36 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.21  | 113 | 204782  | 17.27 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 8.63  | 128 | 226081  | 39.30 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 9.36  | 143 | 205864  | 36.17 | ng/ul | 0.01 |
| 26) 2,4-Dichlorophenol-d3      | 9.91  | 165 | 357228  | 31.26 | ng/ul | 0.02 |
| 29) 4-Chloroaniline-d4         | 10.45 | 131 | 20053   | 1.73  | ng/ul | 0.06 |
| 44) Dimethylphthalate-d6       | 13.56 | 166 | 1230311 | 35.26 | ng/ul | 0.00 |
| 47) Acenaphthylene-d8          | 13.82 | 160 | 1435279 | 34.72 | ng/ul | 0.00 |
| 52) 4-Nitrophenol-d4           | 14.36 | 143 | 51198   | 8.28  | ng/ul | 0.00 |
| 58) Fluorene-d10               | 15.13 | 176 | 1075488 | 35.43 | ng/ul | 0.00 |
| 63) 4,6-Dinitro-2-methylphenol | 15.26 | 200 | 200808  | 37.67 | ng/ul | 0.00 |
| 71) Anthracene-d10             | 16.98 | 188 | 1671727 | 37.11 | ng/ul | 0.00 |
| 79) Pyrene-d10                 | 19.28 | 212 | 1850350 | 38.00 | ng/ul | 0.00 |
| 90) Benzo(a)pyrene-d12         | 23.06 | 264 | 1619663 | 31.14 | ng/ul | 0.00 |

## Target Compounds

|                         |       |     |          |          | Ovalue |     |
|-------------------------|-------|-----|----------|----------|--------|-----|
| 4) Benzaldehyde         | 6.65  | 77  | 210860   | 20.595   | ng/ul# | 1   |
| 6) Phenol               | 6.71  | 94  | 27521    | 1.560    | ng/ul# | 58  |
| 11) 2-Methylphenol      | 7.95  | 108 | 229705   | 18.902   | ng/ul  | 89  |
| 14) Acetophenone        | 8.30  | 105 | 307416   | 15.454   | ng/ul  | 94  |
| 16) 4-Methylphenol      | 8.27  | 108 | 227377   | 17.205   | ng/ul  | 95  |
| 17) Hexachloroethane    | 8.52  | 117 | 84107    | 14.605   | ng/ul# | 10  |
| 20) Nitrobenzene        | 8.67  | 77  | 20186    | 1.142    | ng/ul# | 11  |
| 21) Isophorone          | 9.23  | 82  | 6998410  | 238.120  | ng/ul  | 98  |
| 24) 2,4-Dimethylphenol  | 9.47  | 107 | 61883    | 3.916    | ng/ul  | 99  |
| 30) 4-Chloroaniline     | 10.39 | 127 | 17600057 | 1453.712 | ng/ul# | 18  |
| 34) 2-Methylnaphthalene | 11.95 | 142 | 12927520 | 445.425  | ng/ul  | 100 |
| 35) 1-Methylnaphthalene | 12.16 | 142 | 8590568  | 319.039  | ng/ul  | 99  |
| 41) 1,1'-Biphenyl       | 12.96 | 154 | 2508247  | 64.958   | ng/ul  | 99  |
| 45) Dimethylphthalate   | 13.60 | 163 | 369423   | 10.083   | ng/ul  | 99  |
| 48) Acenaphthylene      | 13.86 | 152 | 6833992  | 150.564  | ng/ul  | 98  |
| 50) Acenaphthene        | 14.20 | 153 | 592085   | 18.497   | ng/ul  | 97  |
| 54) Dibenzofuran        | 14.53 | 168 | 140985   | 3.134    | ng/ul  | 100 |
| 59) Fluorene            | 15.19 | 166 | 2096258  | 57.605   | ng/ul  | 100 |
| 61) 4-Nitroaniline      | 15.19 | 138 | 23554    | 3.151    | ng/ul# | 16  |
| 69) Pentachlorophenol   | 16.54 | 266 | 7928     | 1.203    | ng/ul  | 96  |
| 70) Phenanthrene        | 16.93 | 178 | 5094146  | 88.459   | ng/ul  | 99  |
| 72) Anthracene          | 17.02 | 178 | 781596   | 13.528   | ng/ul  | 98  |
| 75) Carbazole           | 17.29 | 167 | 149160   | 3.121    | ng/ul  | 98  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052620\  
Data File : BM026130.D  
Acq On : 27 May 2020 01:33  
Operator : MA/SJ  
Sample : L2756-04  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
ETKW8

Quant Time: May 27 03:25:08 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM051320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 26 11:15:44 2020  
Response via : Initial Calibration


| Internal Standards | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|--------------------|-------|------|----------|--------|-------|----------|
| 77) Fluoranthene   | 18.94 | 202  | 590009   | 9.767  | ng/ul | 99       |
| 80) Pyrene         | 19.31 | 202  | 792839   | 11.914 | ng/ul | 97       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052620\  
Data File : BM026130.D  
Acq On : 27 May 2020 01:33  
Operator : MA/SJ  
Sample : L2756-04  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
ETKW8

Quant Time: May 27 03:25:08 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM051320MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 26 11:15:44 2020  
Response via : Initial Calibration

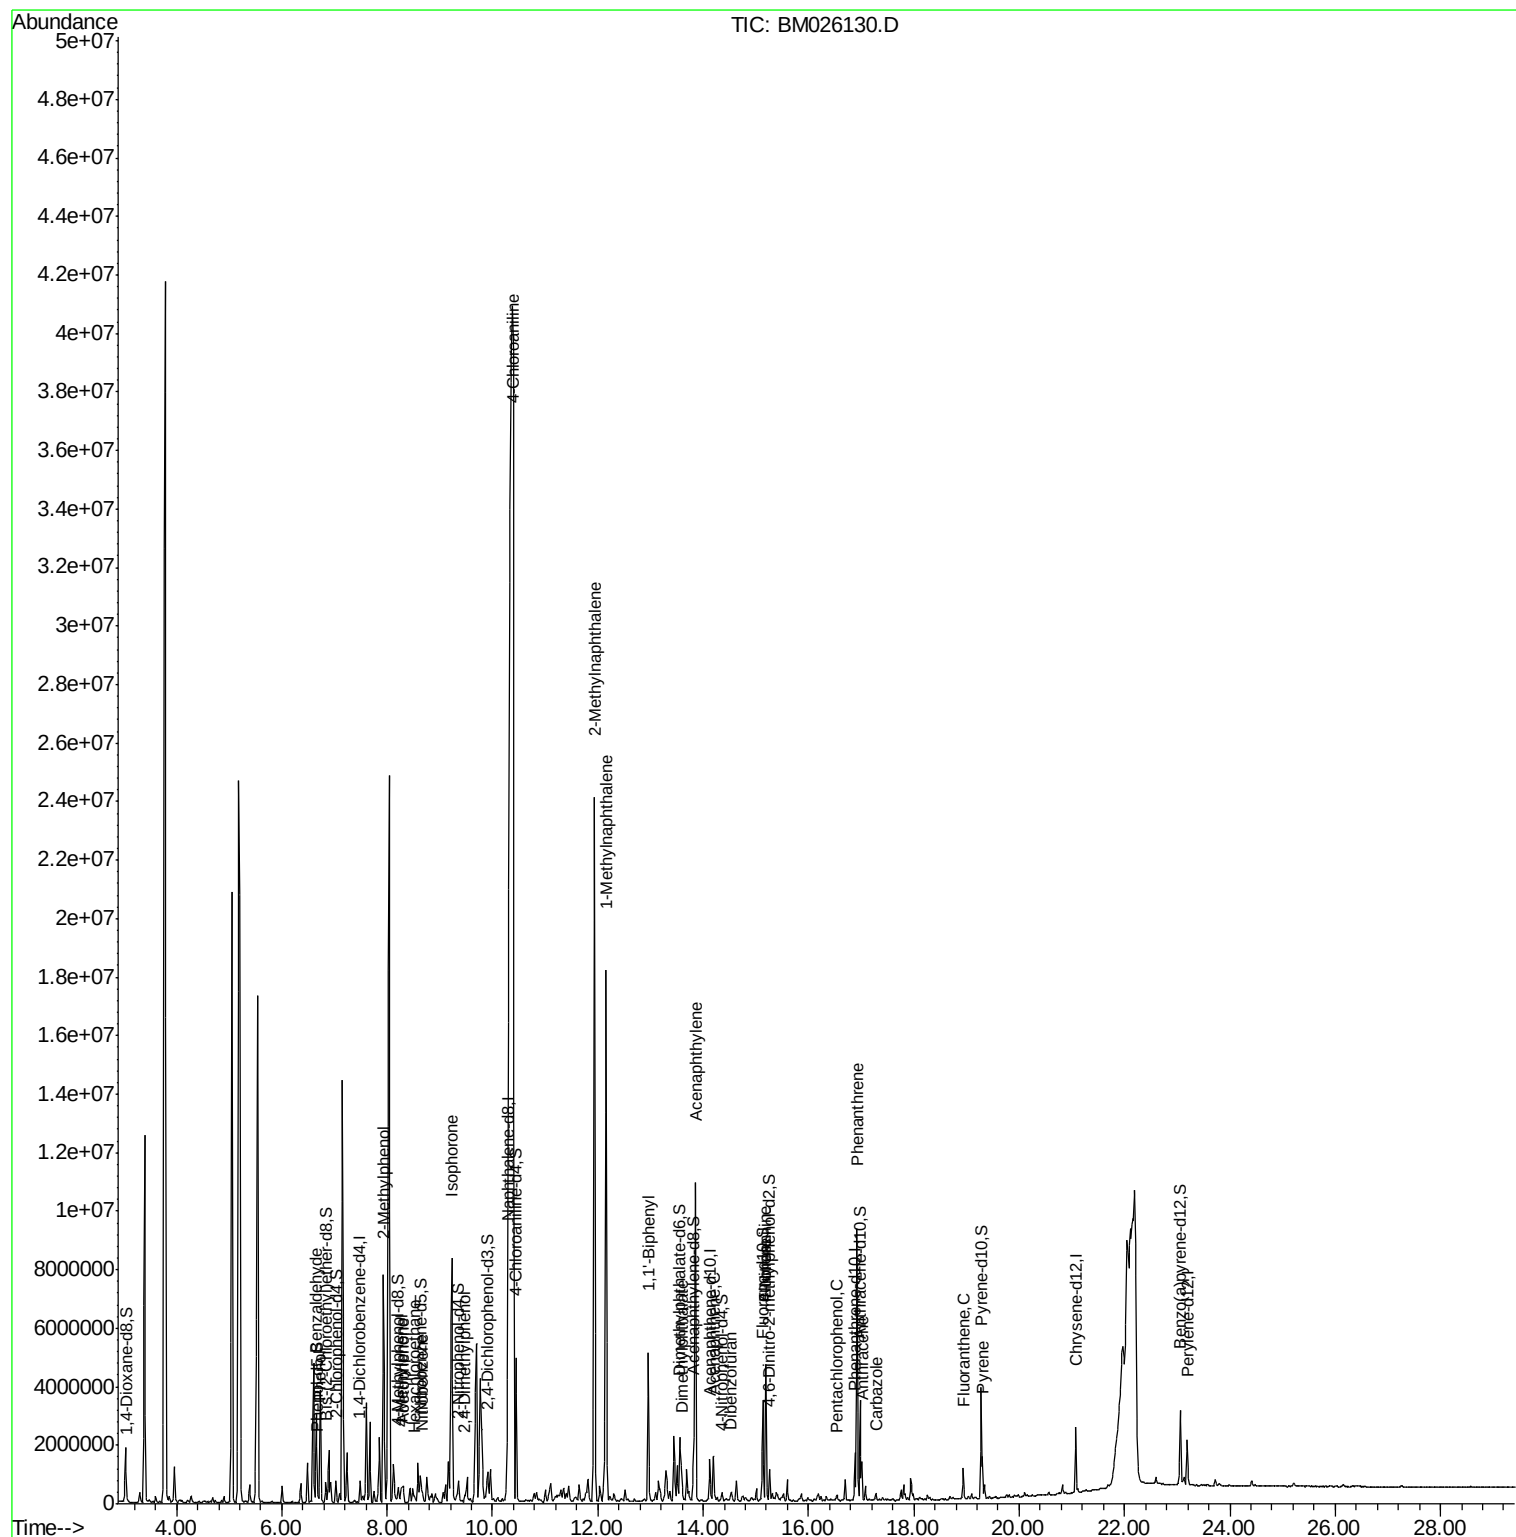

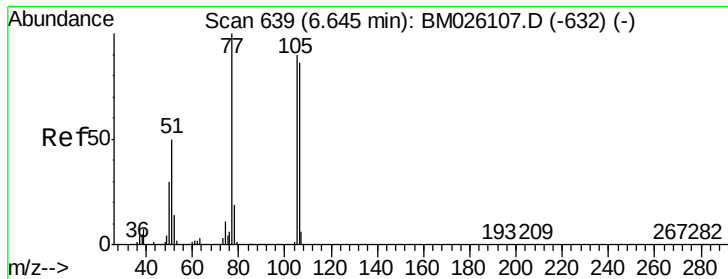

#4

Benzaldehyde

Concen: 20.595 ng/ul

RT: 6.65 min Scan# 640

Delta R.T. 0.01 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampleId :

ETKW8


Tot Ion: 77 Resp: 210860

Ion Ratio Lower Upper

77 100

105 772.6 68.6 102.8#

106 69.6 63.4 95.0

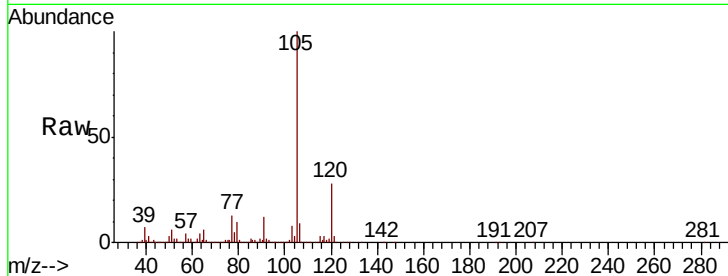

Abundance Ion 77.00 (76.70 to 77.70): BM026130.D (-605) (-)

2500000

Ion 105.00 (104.70 to 105.70): BM026130.D (-605) (-)

2000000

Ion 106.00 (105.70 to 106.70): BM026130.D (-605) (-)



1500000

1000000

500000

0

Time--> 6.60 6.65 6.70

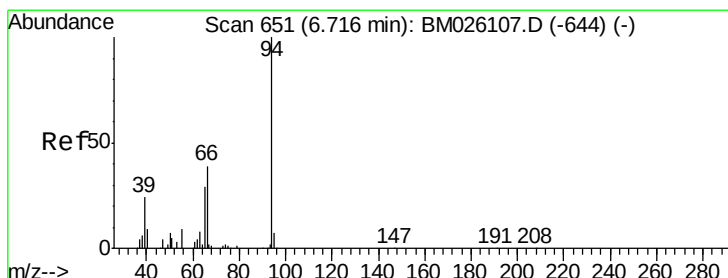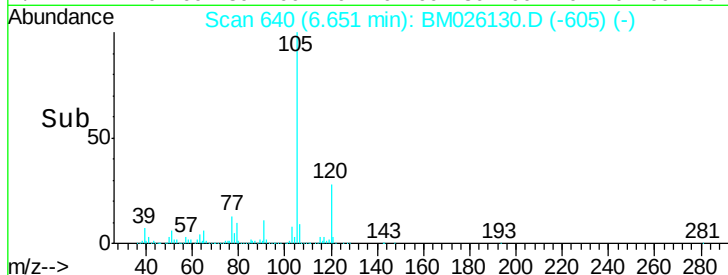

#6

Phenol

Concen: 1.560 ng/ul

RT: 6.71 min Scan# 650

Delta R.T. -0.01 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33


Tgt Ion: 94 Resp: 27521

Ion Ratio Lower Upper

94 100

65 78.6 25.8 38.8#

66 47.7 33.3 49.9

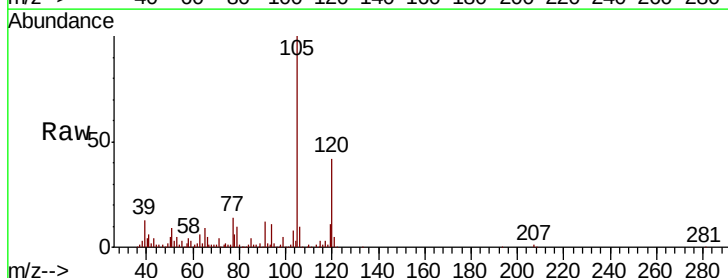

Abundance Ion 94.00 (93.70 to 94.70): BM026130.D (-617) (-)

80000

Ion 65.00 (64.70 to 65.70): BM026130.D (-617) (-)

60000


Ion 66.00 (65.70 to 66.70): BM026130.D (-617) (-)


40000

20000

0

Time--> 6.65 6.70 6.75




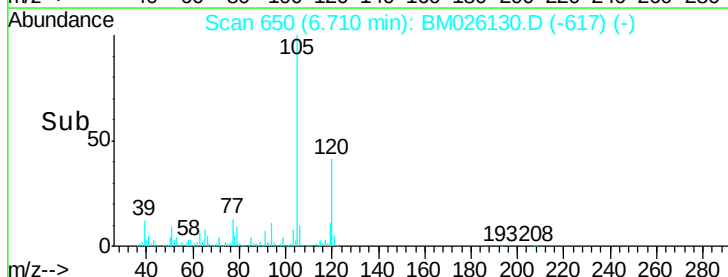




#11  
2-Methylphenol  
Concen: 18.902 ng/ul  
RT: 7.95 min Scan# 860  
Delta R.T. -0.00 min  
Lab File: BM026130.D  
Acq: 27 May 2020 01:33




Instrument :  
BNA\_M  
ClientSampleId :  
ETKW8


Tot Ion:108 Resp: 229705  
Ion Ratio Lower Upper  
108 100  
107 100.4 72.3 108.5

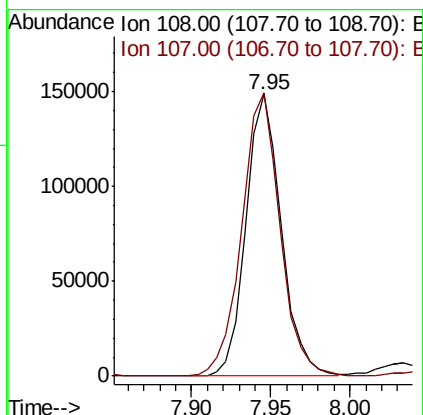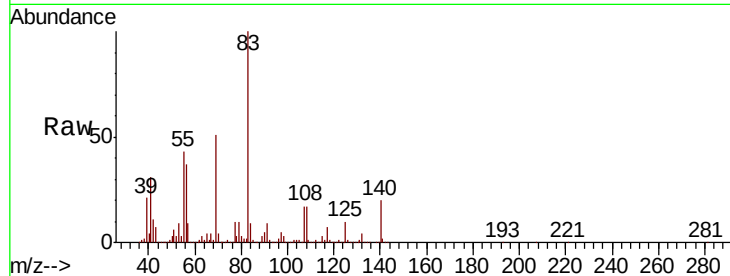

#14  
Acetophenone  
Concen: 15.454 ng/ul  
RT: 8.30 min Scan# 921  
Delta R.T. -0.00 min  
Lab File: BM026130.D  
Acq: 27 May 2020 01:33

Tgt Ion:105 Resp: 307416  
Ion Ratio Lower Upper  
105 100  
77 78.7 67.2 100.8  
51 30.4 27.4 41.0

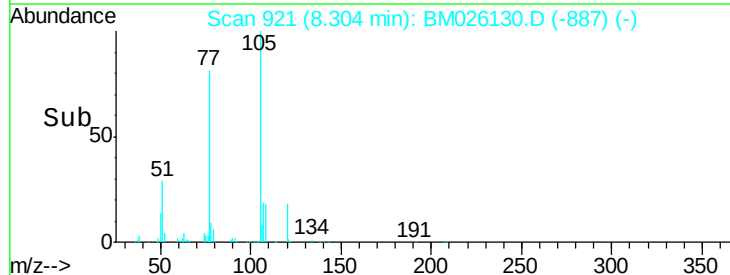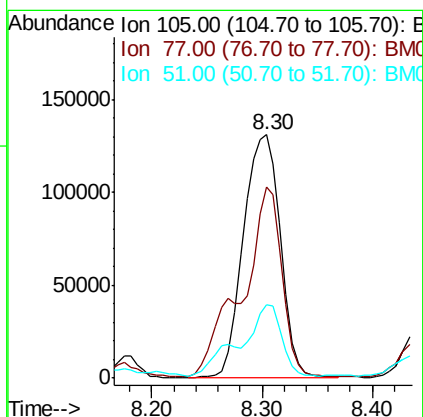

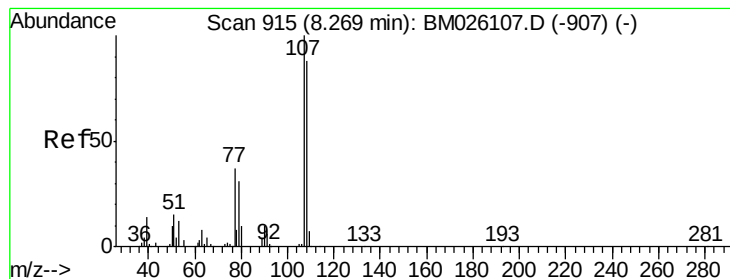

#16

4-Methylphenol

Concen: 17.205 ng/ul

RT: 8.27 min Scan# 915

Delta R.T. -0.00 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampleId :


ETKW8

Tot Ion:108 Resp: 227377

Ion Ratio Lower Upper




108 100

107 115.7 88.6 132.8



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

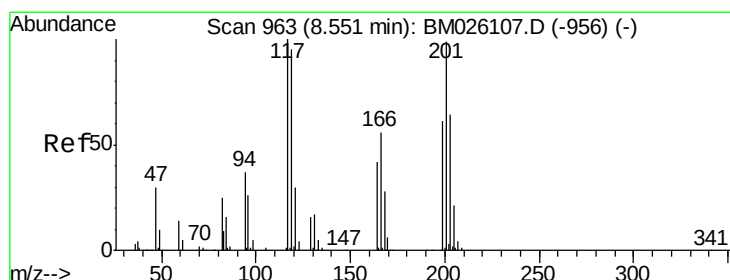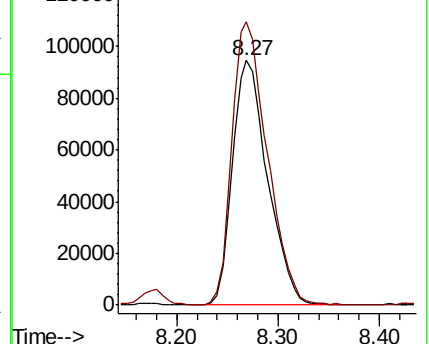

#17

Hexachloroethane

Concen: 14.605 ng/ul

RT: 8.52 min Scan# 958

Delta R.T. -0.03 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33


Tgt Ion:117 Resp: 84107

Ion Ratio Lower Upper

117 100

201 0.0 74.5 111.7#



199 0.0 45.9 68.9#




Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E




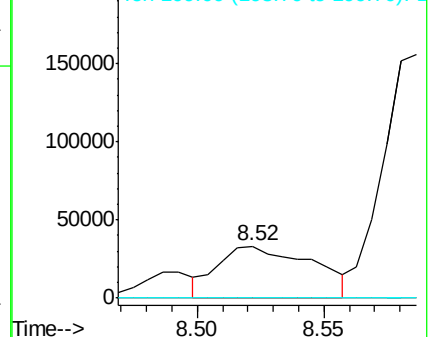




#20  
 Nitrobenzene  
 Concen: 1.142 ng/ul  
 RT: 8.67 min Scan# 984  
 Delta R.T. -0.00 min  
 Lab File: BM026130.D  
 Acq: 27 May 2020 01:33




Instrument :  
 BNA\_M  
 ClientSampled :  
 ETKW8


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 77      | 100   |       |       |
| 123     | 3.2   | 29.5  | 44.3# |
| 65      | 84.2  | 11.0  | 16.4# |

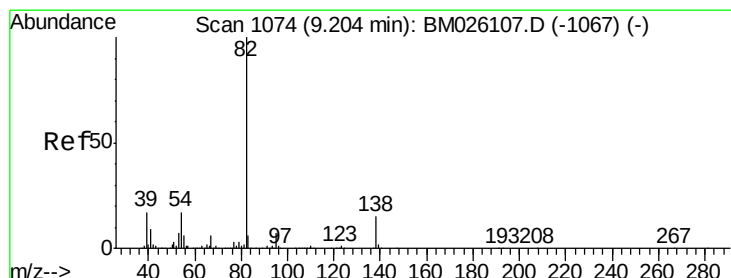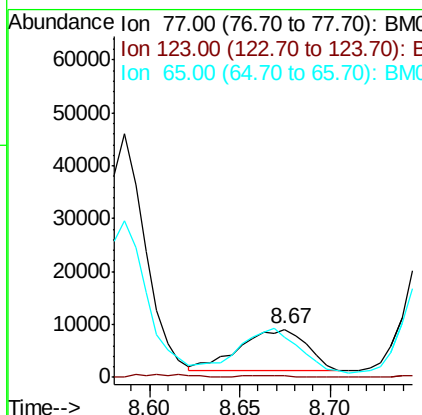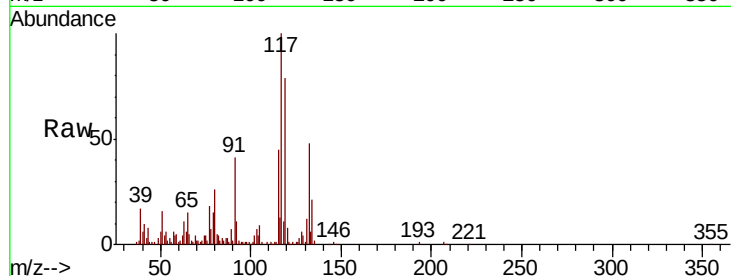

#21  
 Isophorone  
 Concen: 238.120 ng/ul  
 RT: 9.23 min Scan# 1078  
 Delta R.T. 0.02 min  
 Lab File: BM026130.D  
 Acq: 27 May 2020 01:33

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 82      | 100   |       |       |
| 95      | 7.0   | 5.6   | 8.4   |
| 138     | 16.3  | 11.9  | 17.9  |

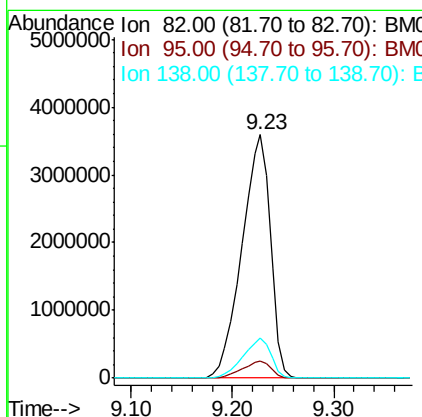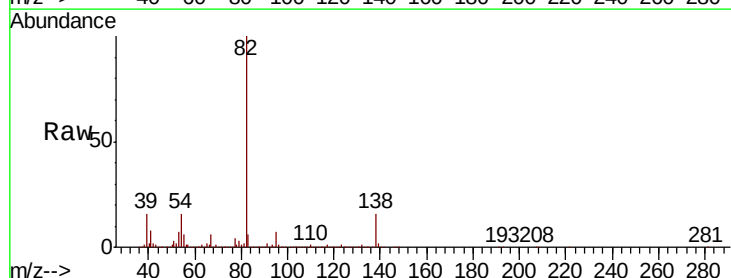

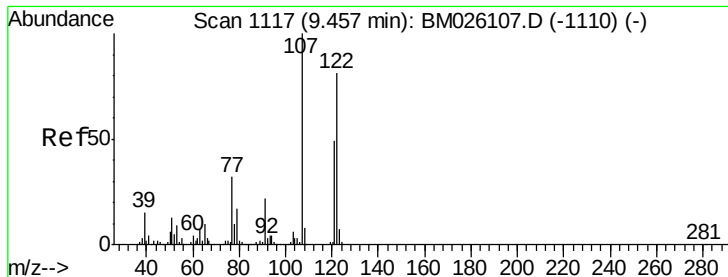

#24

2,4-Dimethylphenol

Concen: 3.916 ng/ul

RT: 9.47 min Scan# 1120

Delta R.T. 0.02 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampleId :

ETKW8


Tot Ion:107 Resp: 61883

Ion Ratio Lower Upper

107 100

121 47.2 37.5 56.3




122 80.6 63.8 95.6

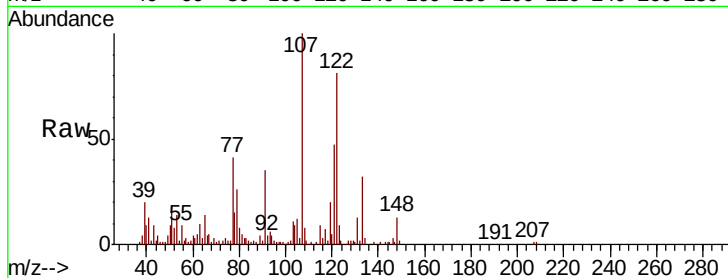

Abundance Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

Ion 122.00 (121.70 to 122.70): E

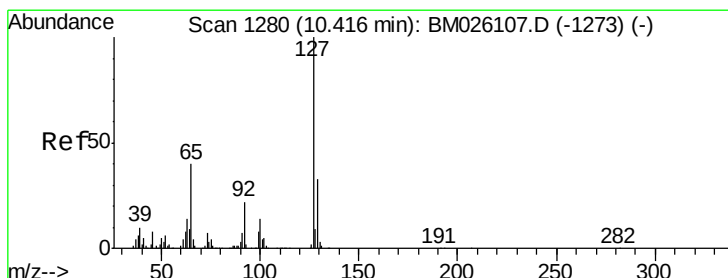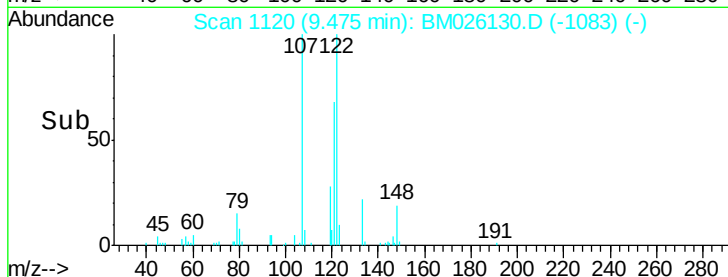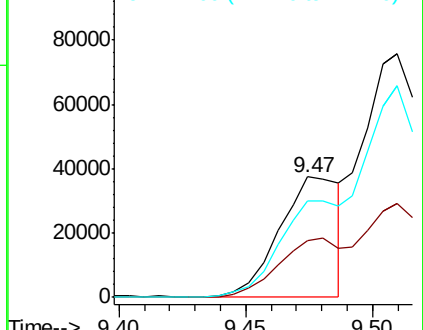

#30

4-Chloroaniline

Concen: 1453.712 ng/ul

RT: 10.39 min Scan# 1276

Delta R.T. -0.02 min

Lab File: BM026130.D


Acq: 27 May 2020 01:33

Tgt Ion:127 Resp:17600057

Ion Ratio Lower Upper



127 100

129 78.7 26.2 39.2#

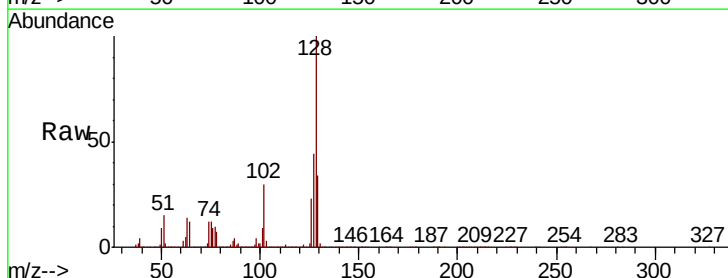


Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

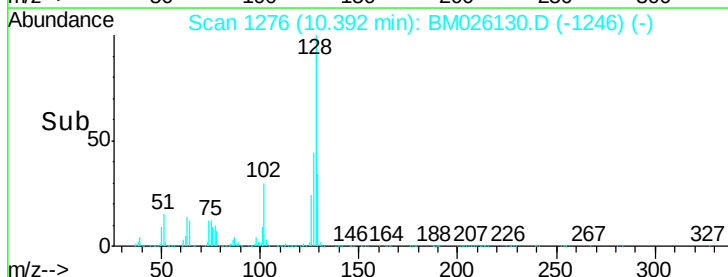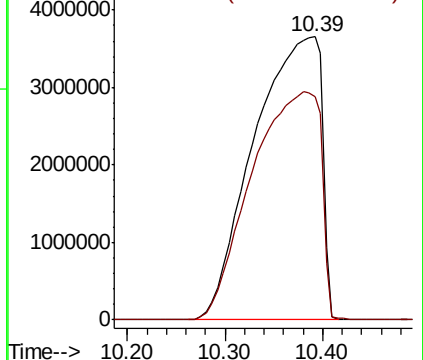



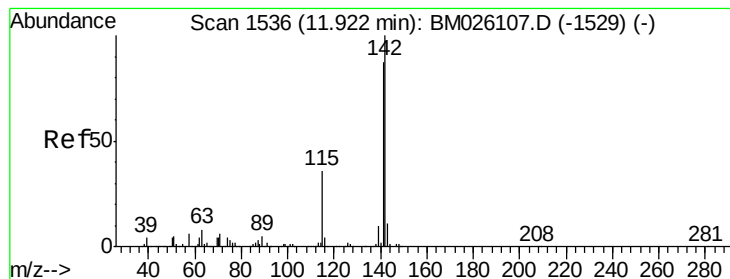

#34

2-Methylnaphthalene

Concen: 445.425 ng/ul

RT: 11.95 min Scan# 1540

Delta R.T. 0.02 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampleId :


ETKW8

Tot Ion:142 Resp:12927520

Ion Ratio Lower Upper




142 100

141 90.2 71.8 107.6



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

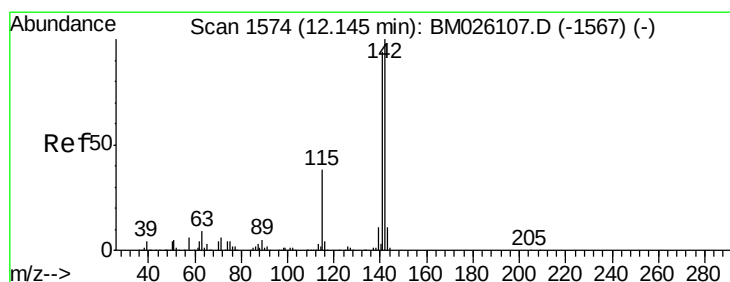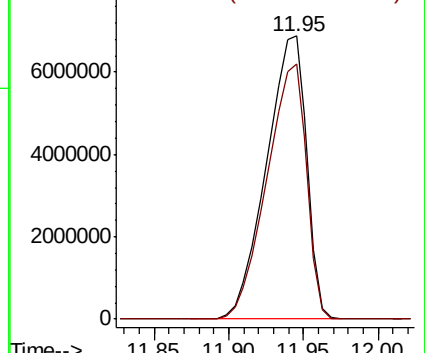

#35

1-Methylnaphthalene

Concen: 319.039 ng/ul

RT: 12.16 min Scan# 1577

Delta R.T. 0.02 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33


Tgt Ion:142 Resp: 8590568

Ion Ratio Lower Upper

142 100

141 92.3 73.0 109.4



116 4.0 3.3 4.9

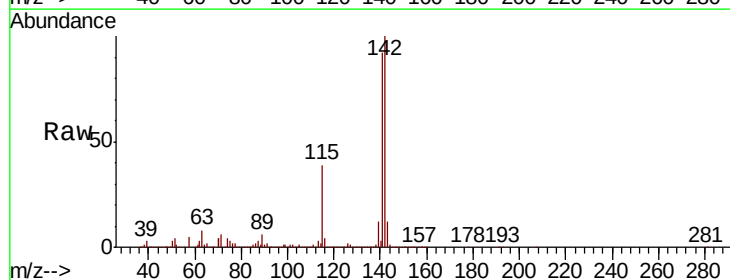


Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E




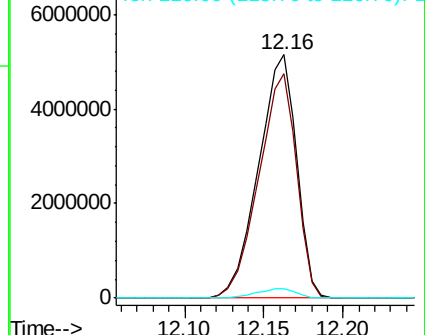




#41  
 1,1'-Biphenyl  
 Concen: 64.958 ng/ul  
 RT: 12.96 min Scan# 1712  
 Delta R.T. -0.00 min  
 Lab File: BM026130.D  
 Acq: 27 May 2020 01:33




Instrument :  
 BNA\_M  
 ClientSampleId :  
 ETKW8


Tot Ion:154 Resp: 2508247  
 Ion Ratio Lower Upper  
 154 100  
 153 40.0 32.3 48.5  
 76 14.9 13.0 19.6

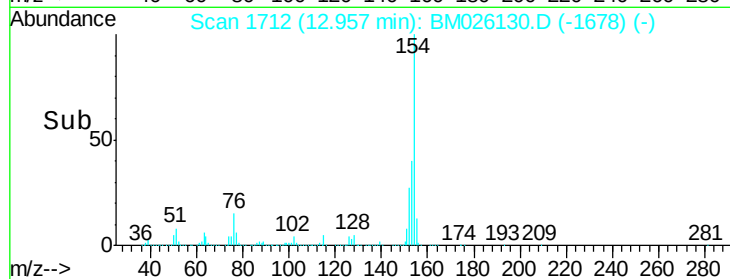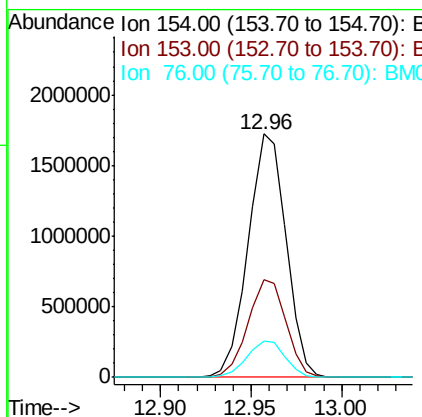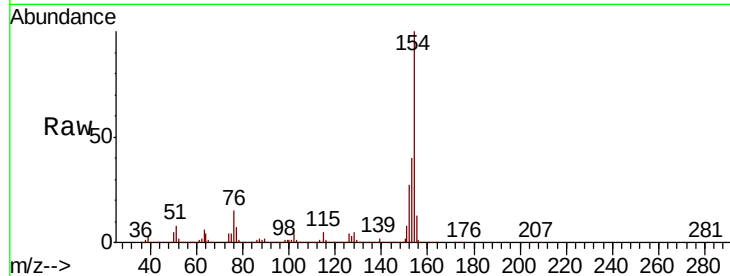

#45  
 Dimethylphthalate  
 Concen: 10.083 ng/ul  
 RT: 13.60 min Scan# 1822  
 Delta R.T. -0.00 min  
 Lab File: BM026130.D  
 Acq: 27 May 2020 01:33

Tgt Ion:163 Resp: 369423  
 Ion Ratio Lower Upper  
 163 100  
 194 4.4 3.2 4.8  
 164 10.4 8.0 12.0

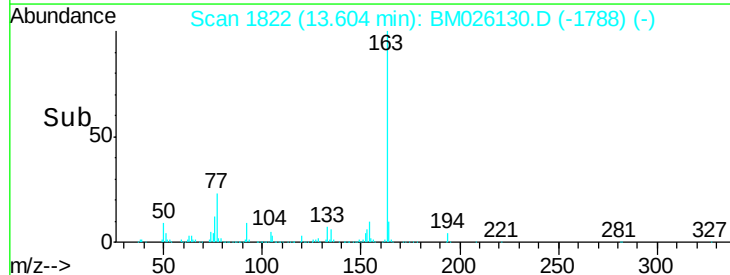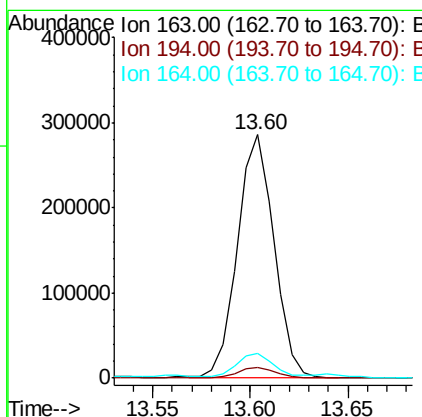



#48

Acenaphthylene

Concen: 150.564 ng/ul

RT: 13.86 min Scan# 1865

Delta R.T. 0.01 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampleId :

ETKW8


Tot Ion:152 Resp: 6833992

Ion Ratio Lower Upper




152 100

151 20.2 15.7 23.5

153 13.7 10.2 15.2



Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 151.00 (150.70 to 151.70): E  
Ion 153.00 (152.70 to 153.70): E

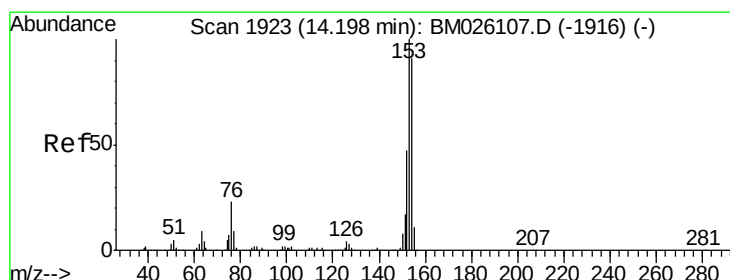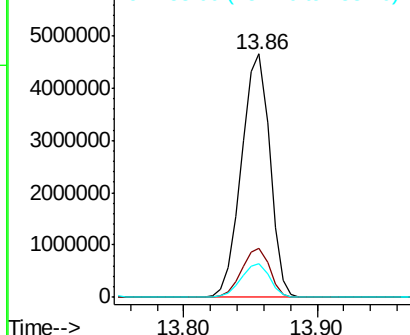

#50

Acenaphthene

Concen: 18.497 ng/ul

RT: 14.20 min Scan# 1923

Delta R.T. -0.00 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33


Tgt Ion:153 Resp: 592085

Ion Ratio Lower Upper



153 100


152 46.8 37.2 55.8

154 91.2 69.8 104.8



Abundance Ion 153.00 (152.70 to 153.70): E  
Ion 152.00 (151.70 to 152.70): E  
Ion 154.00 (153.70 to 154.70): E

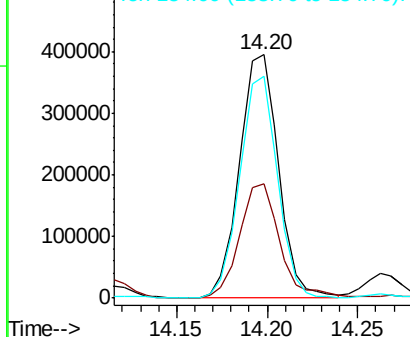

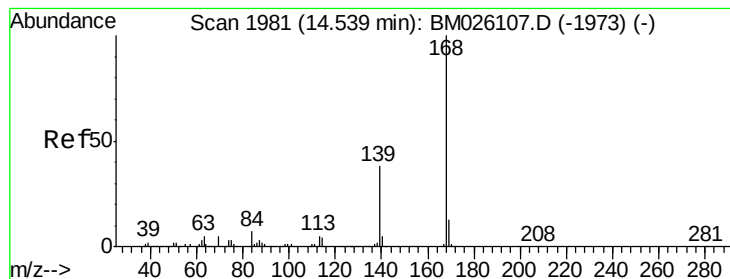

#54

Dibenzenofuran

Concen: 3.134 ng/ul

RT: 14.53 min Scan# 1980

Delta R.T. -0.01 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampled :


ETKW8

Tot Ion:168 Resp: 140985

Ion Ratio Lower Upper




168 100

139 38.4 30.7 46.1



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

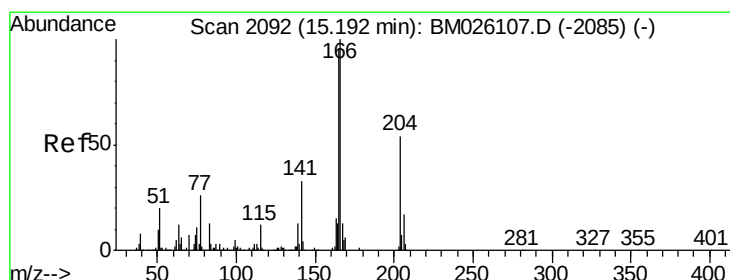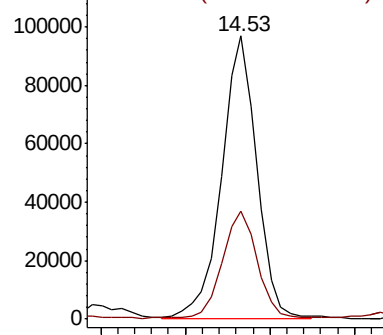

#59

Fluorene

Concen: 57.605 ng/ul

RT: 15.19 min Scan# 2091

Delta R.T. -0.01 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33


Tgt Ion:166 Resp: 2096258

Ion Ratio Lower Upper

166 100

165 96.1 77.3 115.9



167 13.3 10.6 16.0




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E




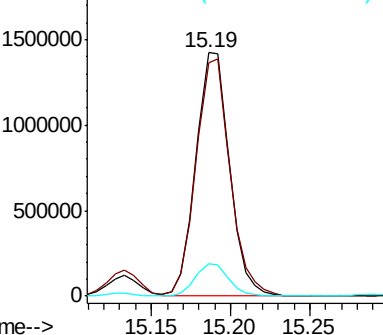




#61  
4-Nitroaniline  
Concen: 3.151 ng/ul  
RT: 15.19 min Scan# 2092  
Delta R.T. -0.02 min  
Lab File: BM026130.D  
Acq: 27 May 2020 01:33




Instrument :  
BNA\_M  
ClientSampleId :  
ETKW8


Tot Ion:138 Resp: 23554  
Ion Ratio Lower Upper  
138 100  
92 2.4 49.4 74.2#  
108 4.8 68.3 102.5#

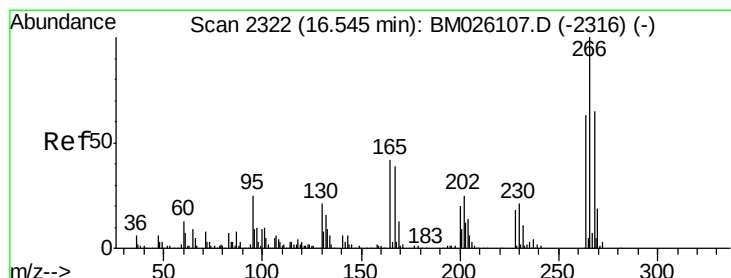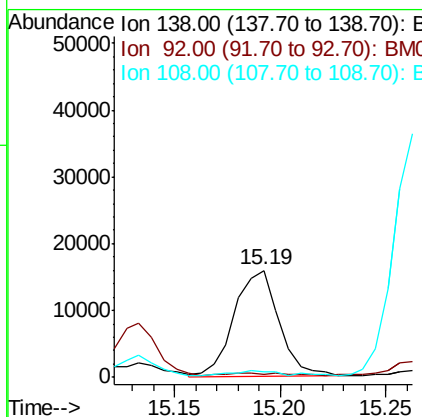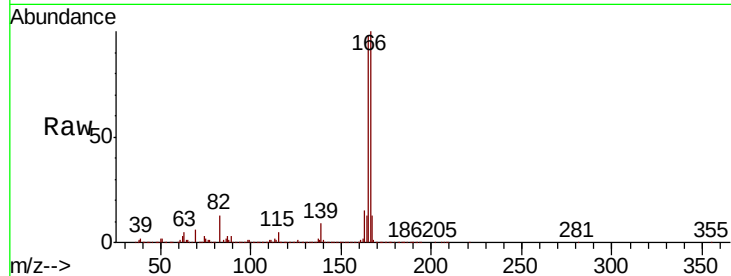

#69  
Pentachlorophenol  
Concen: 1.203 ng/ul  
RT: 16.54 min Scan# 2321  
Delta R.T. -0.01 min  
Lab File: BM026130.D  
Acq: 27 May 2020 01:33

Tgt Ion:266 Resp: 7928  
Ion Ratio Lower Upper  
266 100  
264 62.4 49.3 73.9  
268 59.4 52.4 78.6

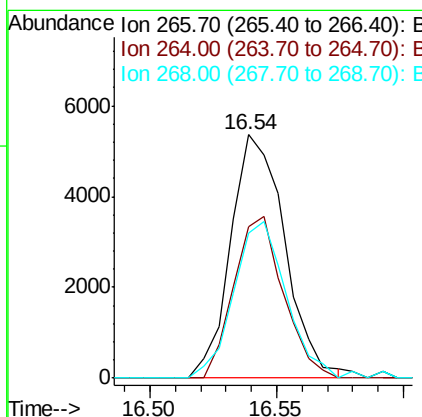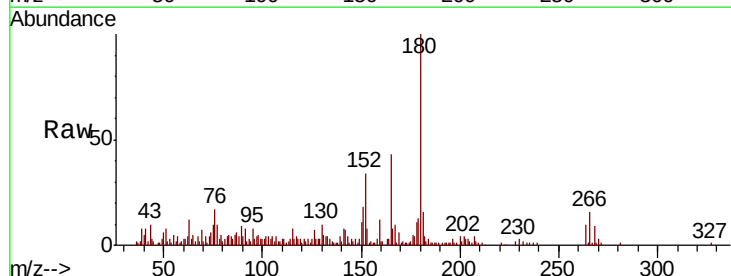



#70

Phenanthrene

Concen: 88.459 ng/ul

RT: 16.93 min Scan# 2387

Delta R.T. -0.00 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :


BNA\_M

ClientSampleId :

ETKW8

Tot Ion:178 Resp: 5094146

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 178 | 100   |       |       |
| 179 | 15.4  | 11.9  | 17.9  |
| 176 | 18.8  | 14.9  | 22.3  |



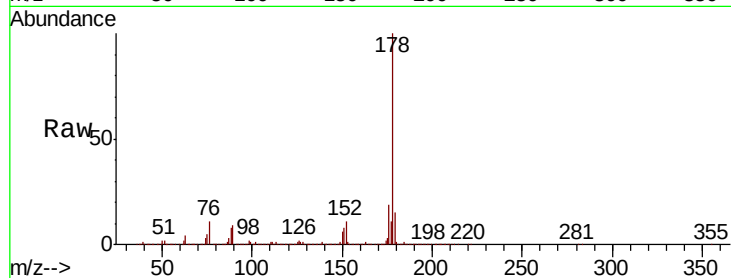


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

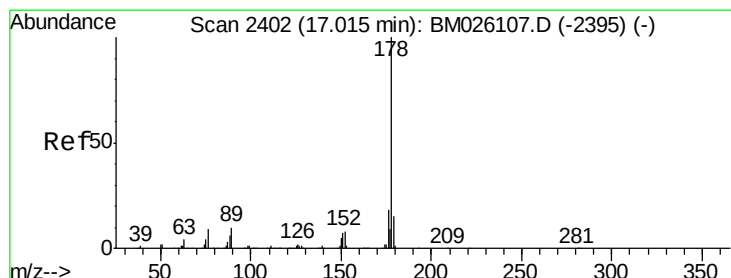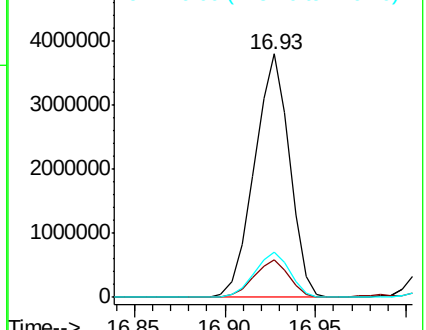

#72

Anthracene

Concen: 13.528 ng/ul

RT: 17.02 min Scan# 2402


Delta R.T. -0.00 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Tgt Ion:178 Resp: 781596

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 178 | 100   |       |       |
| 179 | 15.8  | 12.2  | 18.4  |
| 176 | 17.8  | 14.9  | 22.3  |


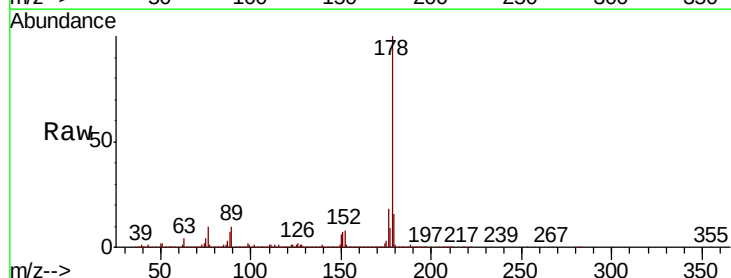



Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

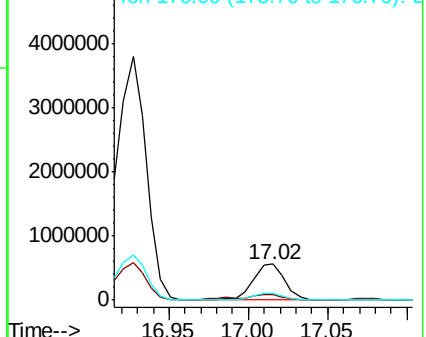



#75

Carbazole

Concen: 3.121 ng/ul

RT: 17.29 min Scan# 2448

Delta R.T. -0.01 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33

Instrument :

BNA\_M

ClientSampleId :

ETKW8


Tot Ion:167 Resp: 149160

Ion Ratio Lower Upper

167 100

166 21.9 16.6 25.0




139 13.2 10.8 16.2

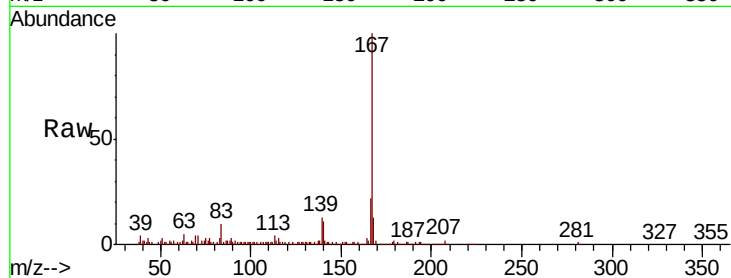

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

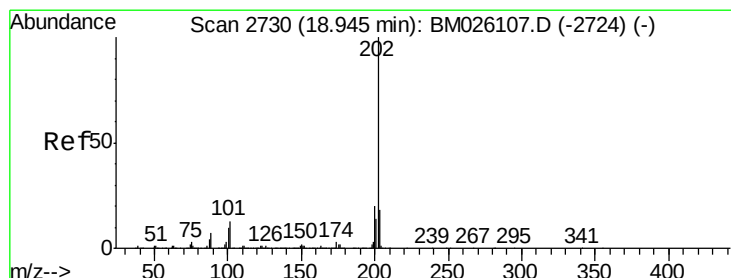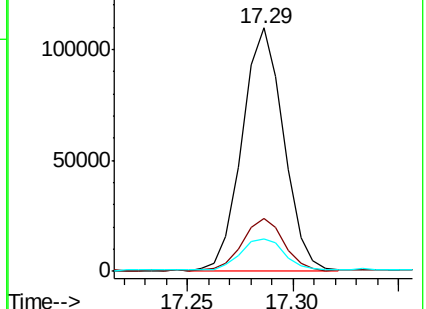

#77

Fluoranthene

Concen: 9.767 ng/ul

RT: 18.94 min Scan# 2730

Delta R.T. -0.00 min

Lab File: BM026130.D

Acq: 27 May 2020 01:33


Tgt Ion:202 Resp: 590009

Ion Ratio Lower Upper

202 100

101 11.4 9.5 14.3



100 9.4 7.6 11.4

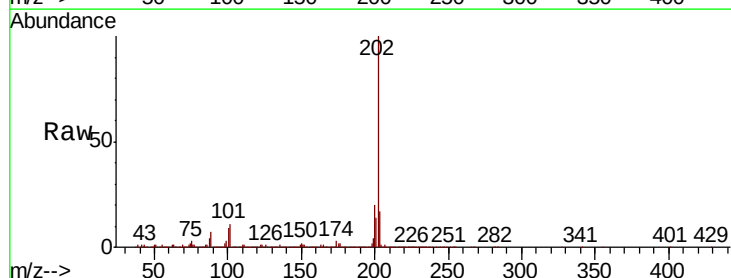


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

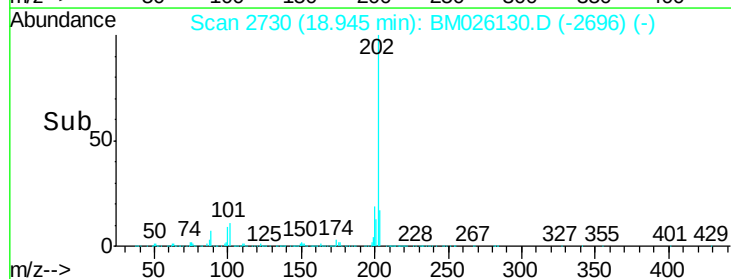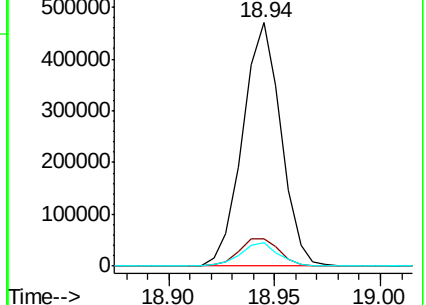



#80  
 Pvrene  
 Concen: 11.914 ng/ul  
 RT: 19.31 min Scan# 2792  
 Delta R.T. -0.00 min  
 Lab File: BM026130.D  
 Acq: 27 May 2020 01:33

Instrument :  
 BNA\_M  
 ClientSampleId :  
 ETKW8

|          |       |       |        |
|----------|-------|-------|--------|
| Tot Ion: | 202   | Resp: | 792839 |
| Ion      | Ratio | Lower | Upper  |
| 202      | 100   |       |        |
| 101      | 14.2  | 12.2  | 18.4   |
| 100      | 11.3  | 10.2  | 15.4   |

