
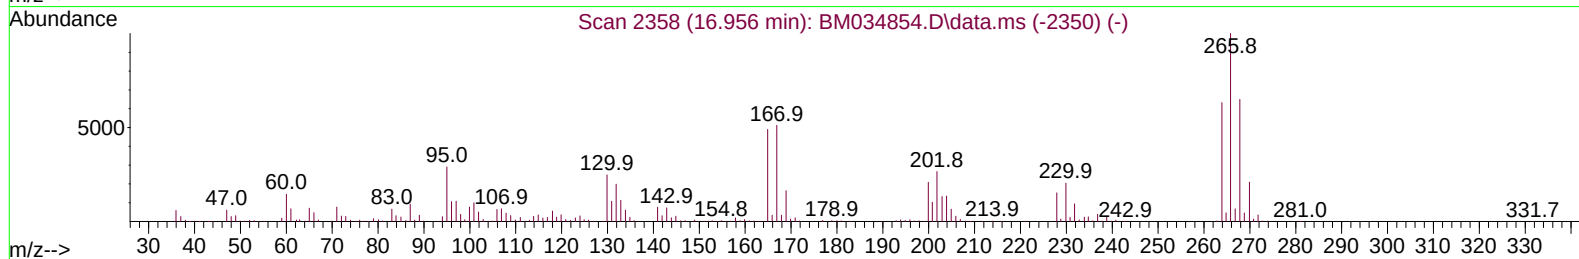
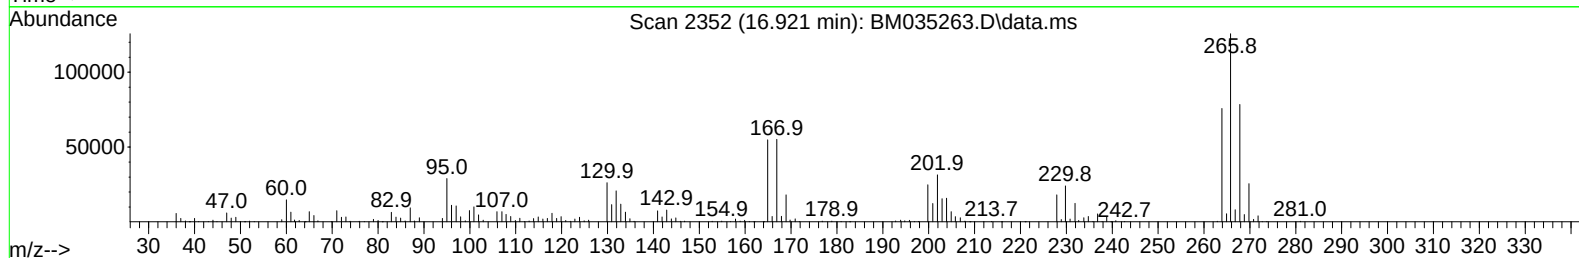


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
 Data File : BM035263.D
 Acq On : 26 May 2022 12:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:38:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 16:33:46 2022
 Response via : Initial Calibration

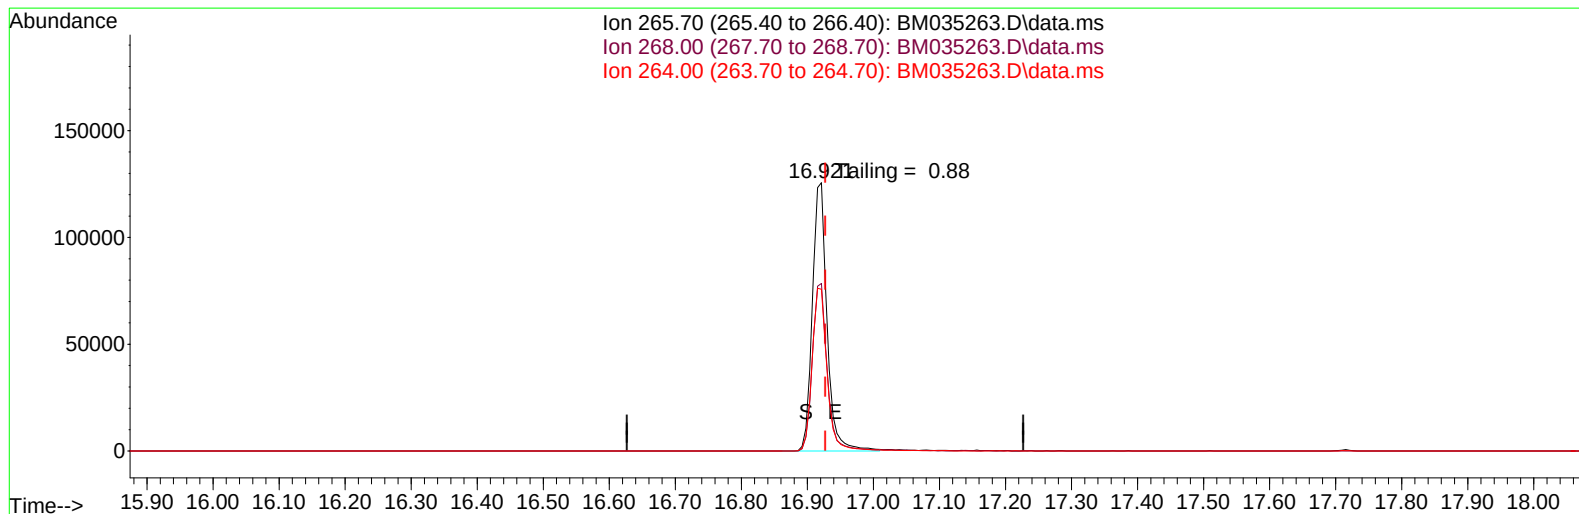

TIC: BM035263.D\data.ms

(70) Pentachlorophenol (C)




16.921min (-0.006) 0.00 ng

response 194847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.42
264.00	63.30	60.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
Data File : BM035263.D
Acq On : 26 May 2022 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:38:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 16:33:46 2022
Response via : Initial Calibration

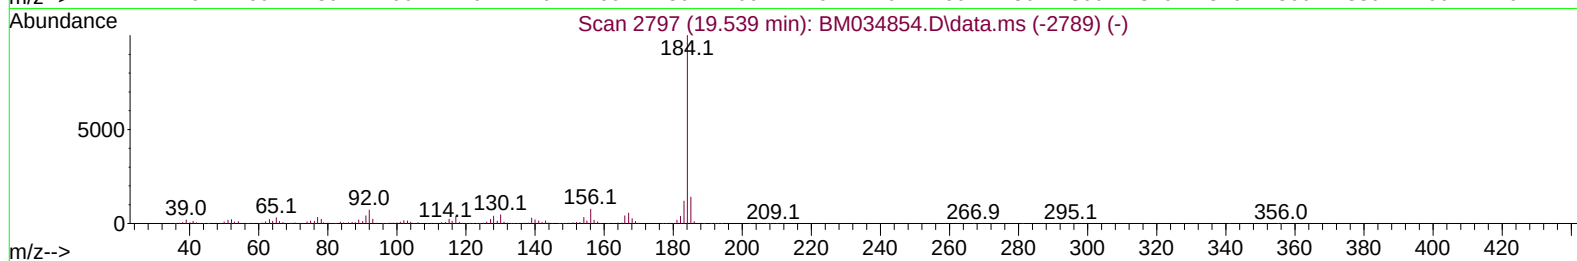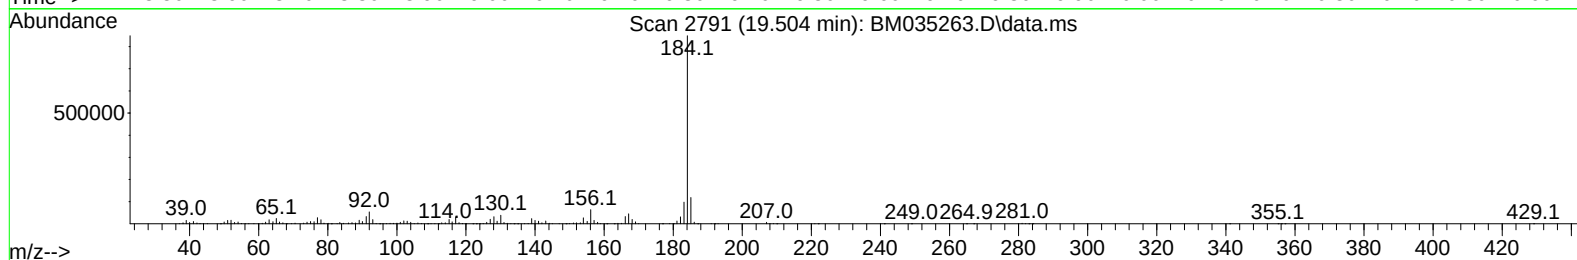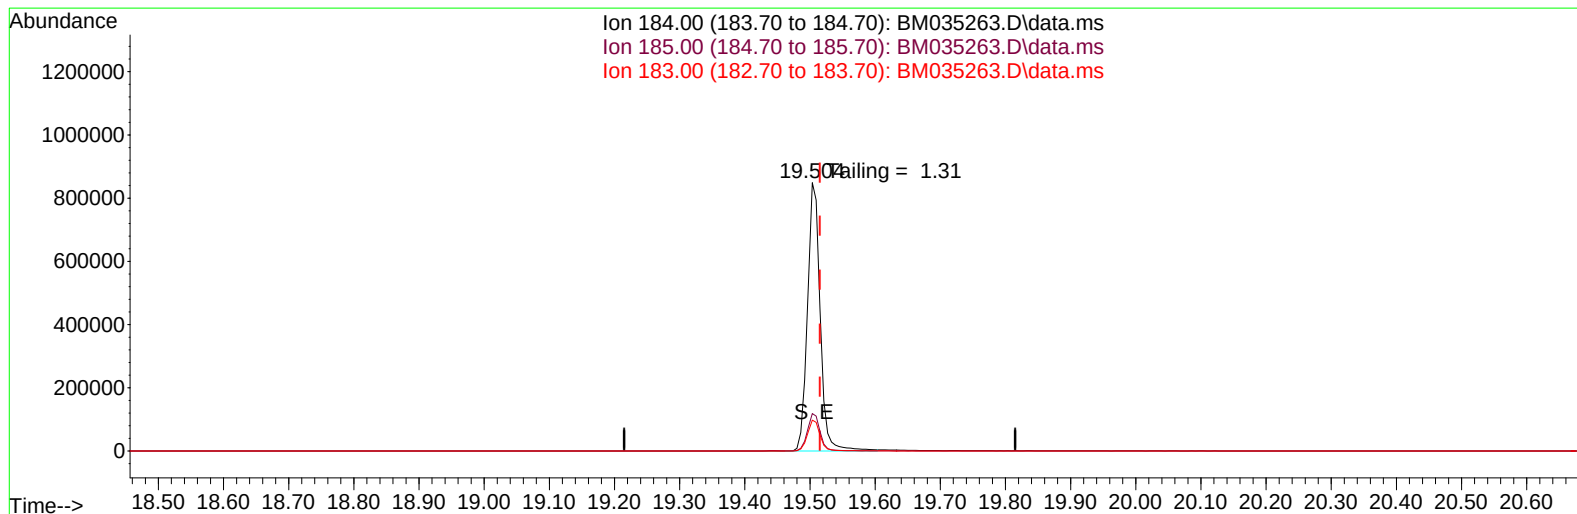

TIC: BM035263.D\data.ms

(77) Benzidine**19.504min (-0.012) 82305.32 ng****response 1164155**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.94
183.00	11.90	11.52
0.00	0.00	0.00