

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
 Data File : BM035273.D
 Acq On : 26 May 2022 18:10
 Operator : CG/JU
 Sample : PB145138BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145138BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	397	404	419	rBV	1230549	1822330	22.19%	6.580%
2	7.057	667	675	691	rBV	1198944	1920460	23.38%	6.934%
3	7.881	808	815	824	rBV	252548	400531	4.88%	1.446%
4	9.039	1003	1012	1026	rBV	749220	1258911	15.33%	4.545%
5	10.680	1284	1291	1308	rBV	327819	582789	7.10%	2.104%
6	13.145	1703	1710	1726	rBV	2646899	3843438	46.80%	13.877%
7	14.521	1937	1944	1956	rBV	635971	955147	11.63%	3.449%
8	16.009	2190	2197	2212	rBV	2437729	3455331	42.07%	12.476%
9	17.262	2404	2410	2421	rBV	941020	1304916	15.89%	4.711%
10	19.892	2851	2857	2868	rVB	6333437	8212558	100.00%	29.652%
11	21.444	3116	3121	3128	rBV	1484683	1857724	22.62%	6.707%
12	23.815	3517	3524	3535	rVB2	1023203	2082414	25.36%	7.519%




Sum of corrected areas: 27696549

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
Data File : BM035273.D
Acq On : 26 May 2022 18:10
Operator : CG/JU
Sample : PB145138BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145138BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

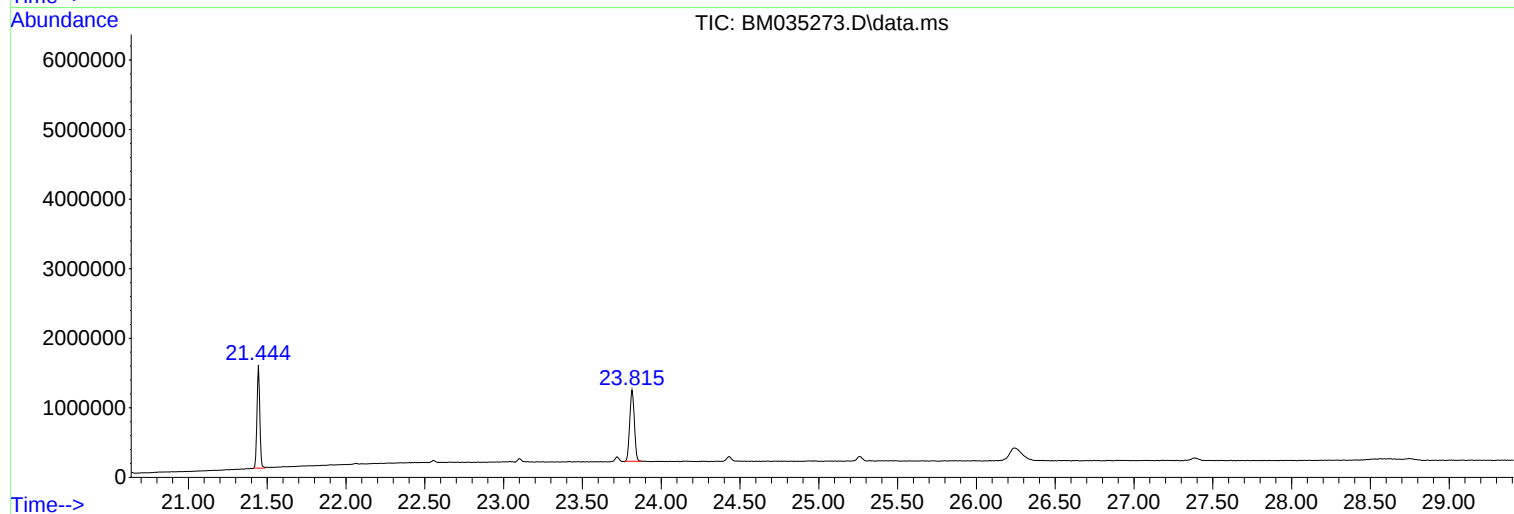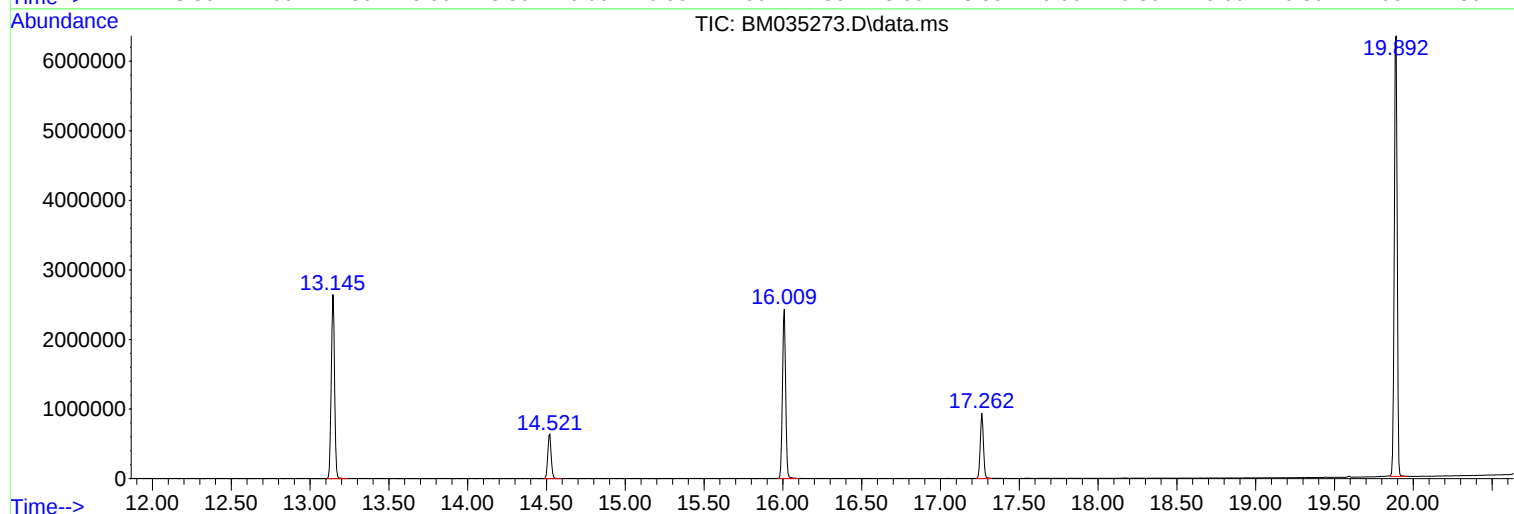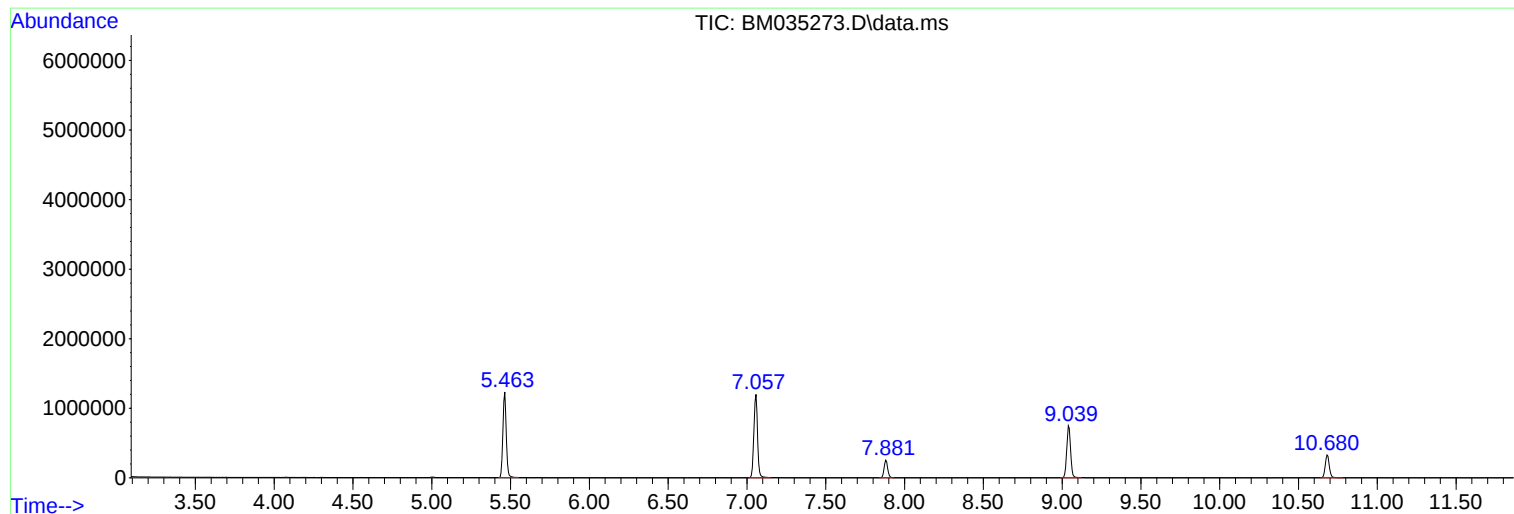

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
Data File : BM035273.D
Acq On : 26 May 2022 18:10
Operator : CG/JU
Sample : PB145138BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145138BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
Data File : BM035273.D
Acq On : 26 May 2022 18:10
Operator : CG/JU
Sample : PB145138BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145138BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------