


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
 Data File : BM035263.D
 Acq On : 26 May 2022 12:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 14:24:42 2022

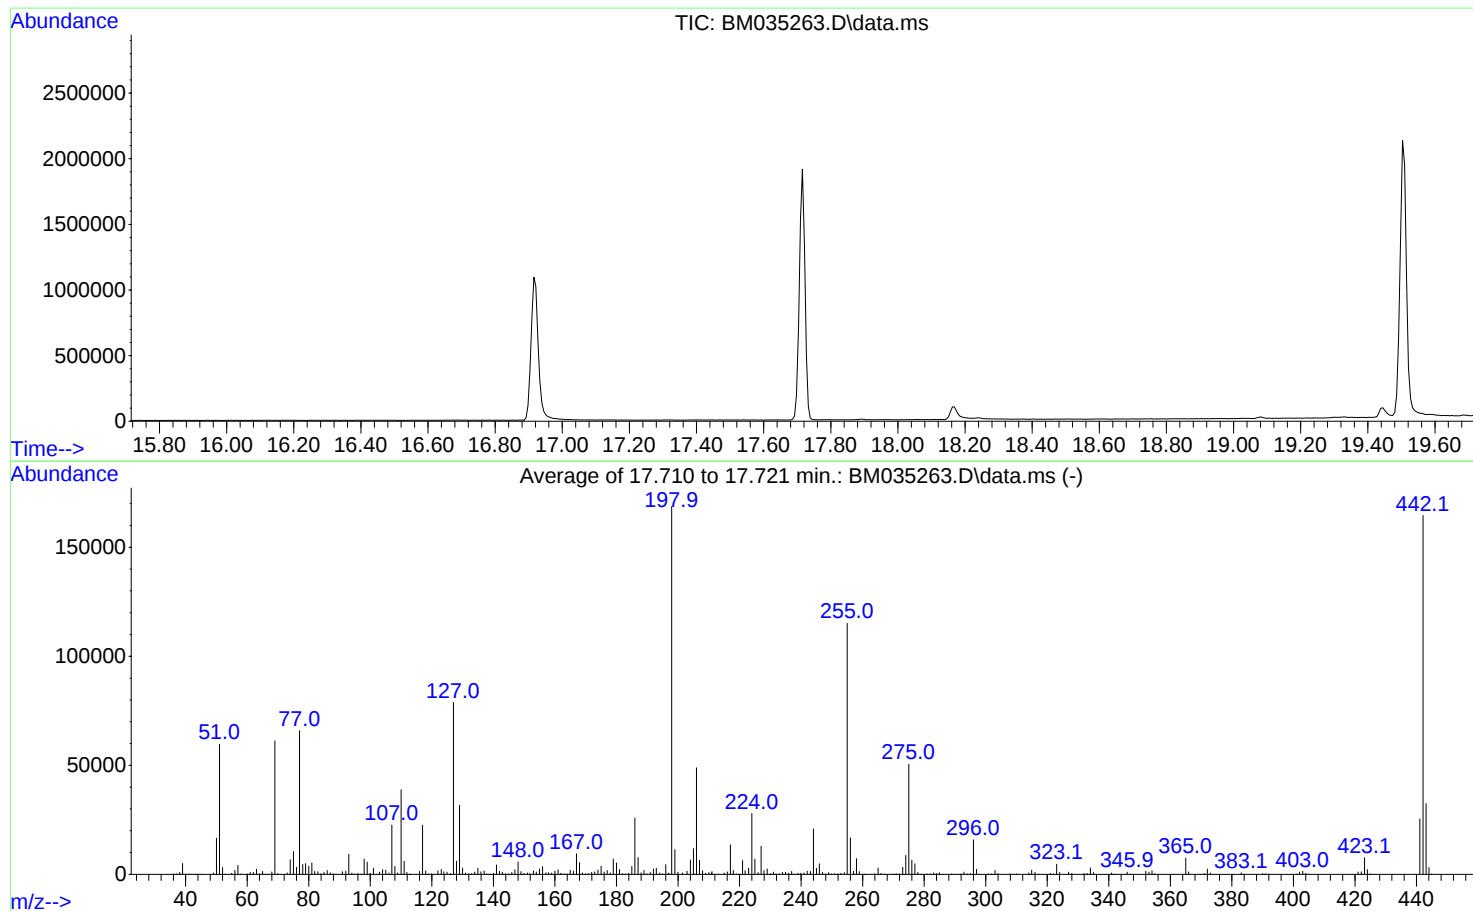




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	59587	PASS
68	69	0.00	2	1.8	1077	PASS
69	198	0.00	100	36.3	61195	PASS
70	69	0.00	2	0.6	338	PASS
127	198	10	80	46.7	78781	PASS
197	198	0.00	2	0.4	597	PASS
198	198	100	100	100.0	168704	PASS
199	198	5	9	6.7	11342	PASS
275	198	10	60	30.0	50595	PASS
365	198	1	100	4.4	7472	PASS
441	198	0.01	100	15.1	25491	PASS
442	442	50	100	100.0	164597	PASS
443	442	15	24	19.7	32421	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
Data File : BM035263.D
Acq On : 26 May 2022 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 26 16:38:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 16:33:46 2022
Response via : Initial Calibration

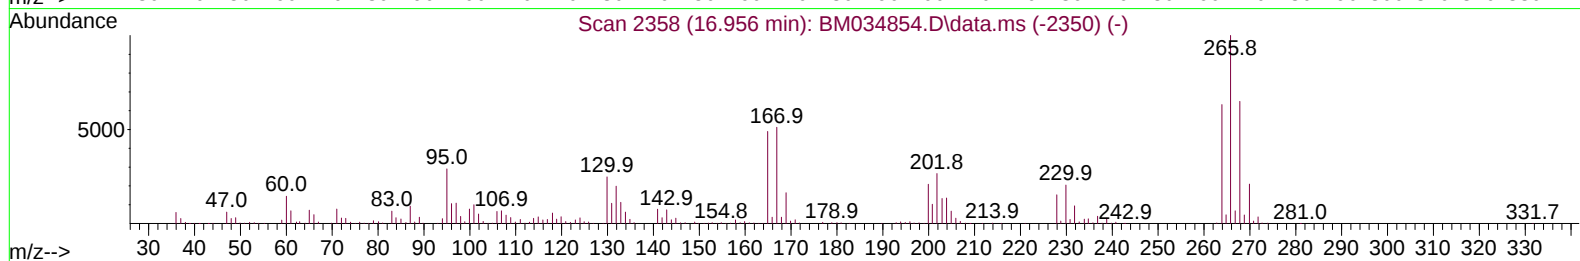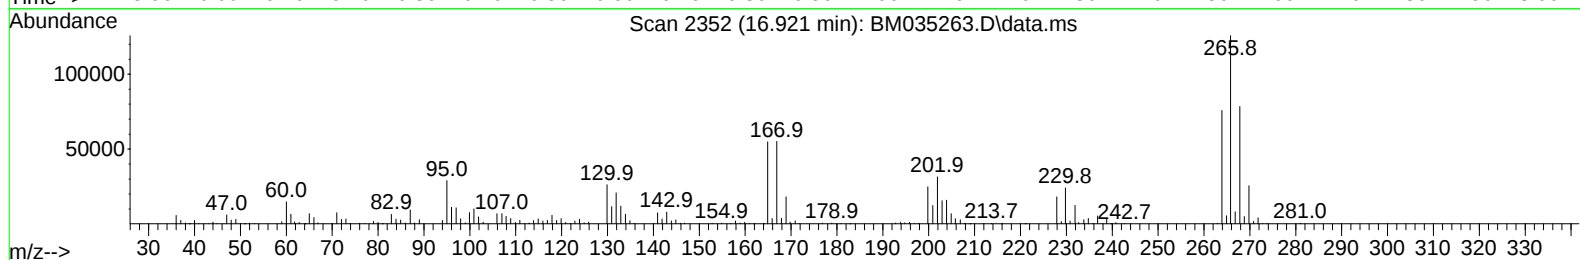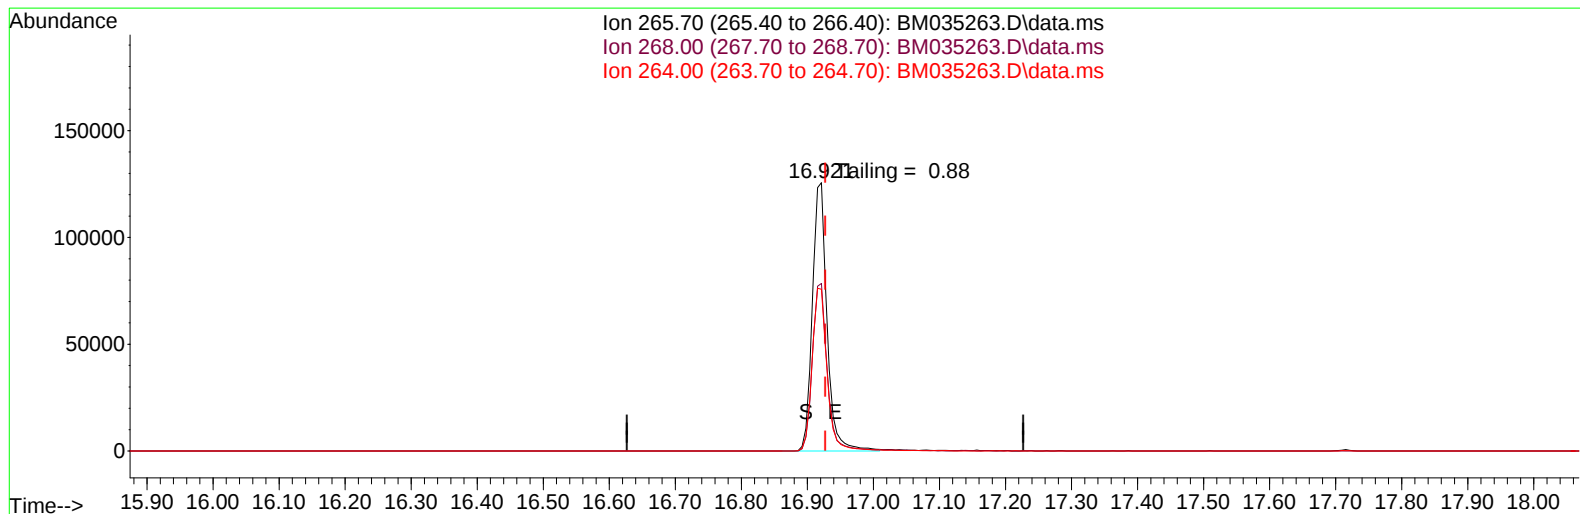

TIC: BM035263.D\data.ms

(70) Pentachlorophenol (C)

16.921min (-0.006) 0.00 ng




response 194847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.42
264.00	63.30	60.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052622\
 Data File : BM035263.D
 Acq On : 26 May 2022 12:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 26 16:38:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 16:33:46 2022
 Response via : Initial Calibration

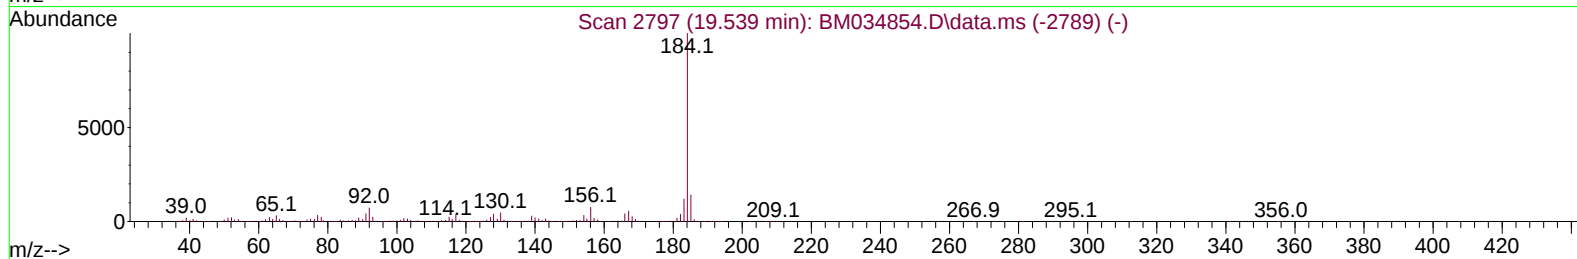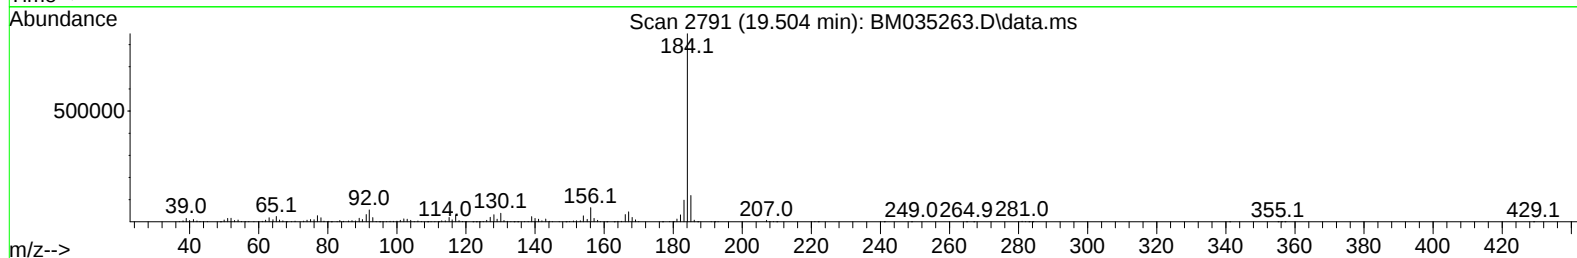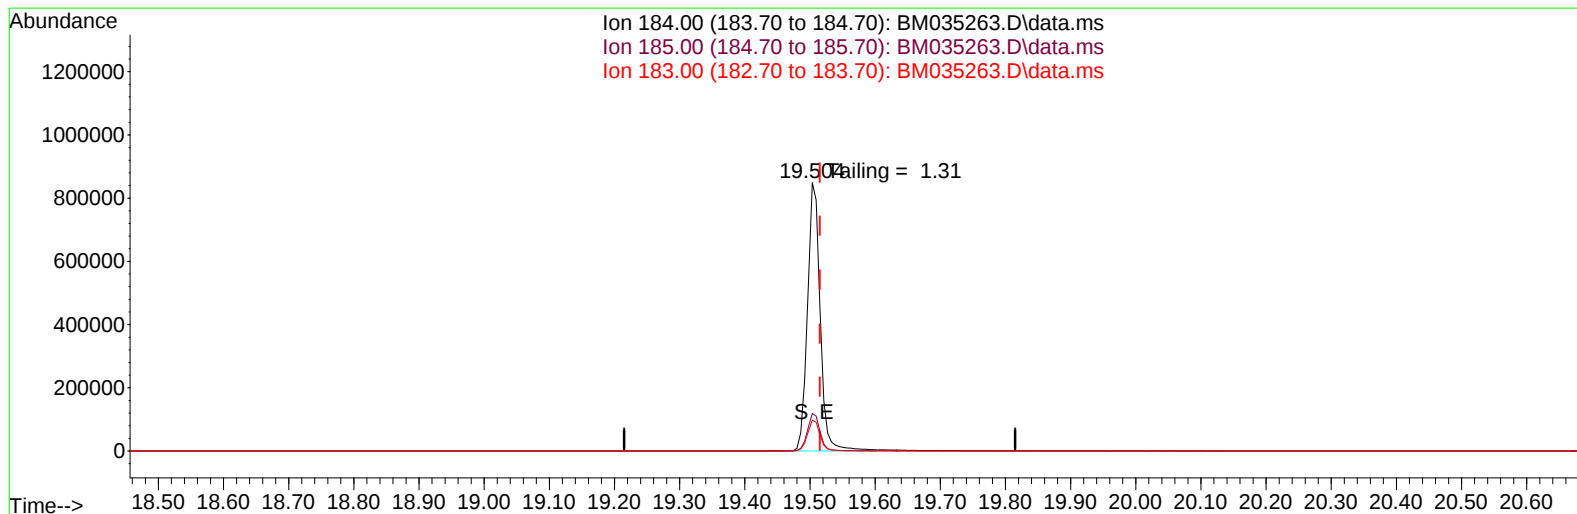

TIC: BM035263.D\data.ms

(77) Benzidine

19.504min (-0.012) 82305.32 ng

response 1164155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.94
183.00	11.90	11.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/26/2022	BNA_M	<u>BM035263.D</u>
Compound Name	Response	Retention Time
DDT	642818	20.74
DDD	2700	20.3
DDE	442	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3142	645960	0.49

Instrument :
BNA_M
ClientSampleId :
DFTPP